


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081522\
 Data File : VV027380.D
 Acq On : 15 Aug 2022 08:29
 Operator : SY/MD
 Sample : BFB353
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB353

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Aug 16 00:24:20 2022

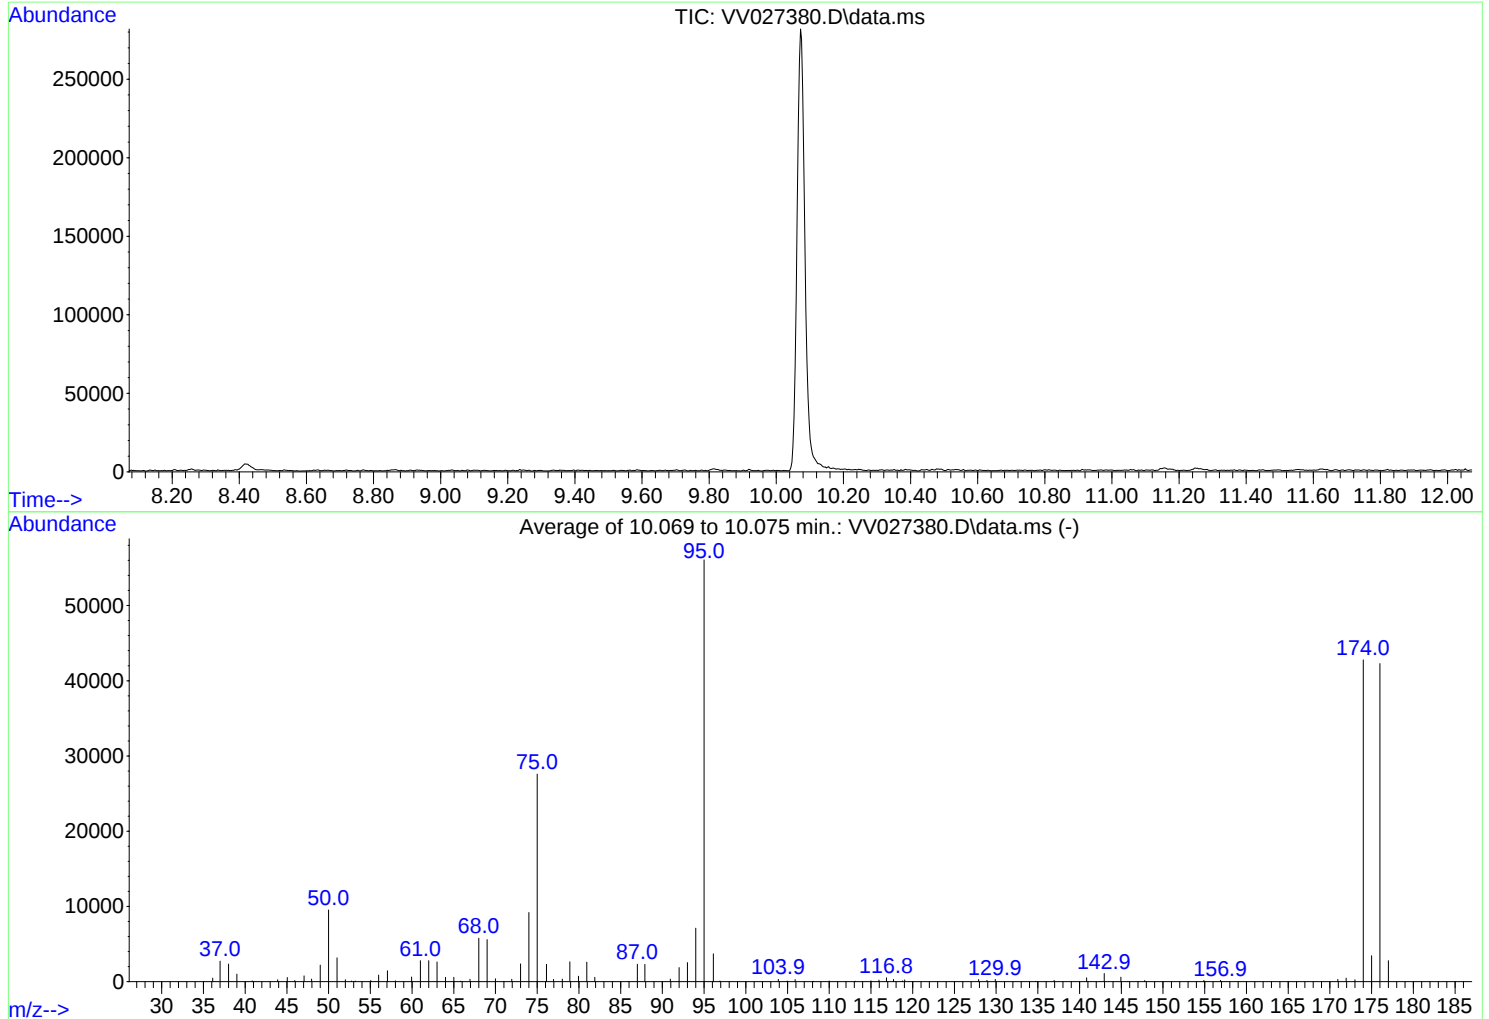

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	9523	PASS
75	95	30	80	49.2	27581	PASS
95	95	100	100	100.0	56075	PASS
96	95	5	9	6.6	3706	PASS
173	174	0.00	2	0.6	256	PASS
174	95	50	120	76.3	42768	PASS
175	174	5	9	8.0	3439	PASS
176	174	95	105	98.9	42285	PASS
177	176	5	10	6.6	2792	PASS

m/z	Abundance
39.90	332.0
41.20	114.0
43.90	358.0

Instrument :
MSVOA_V
ClientSampleId :
BFB353

m/z	Abundance
36.10	464.0
37.00	2655.0
38.00	2248.0
39.00	1030.0
40.80	115.0
43.90	534.0
45.10	514.0
46.00	148.0
47.00	836.0
47.90	338.0
49.00	2077.0
50.00	9243.0
51.00	3036.0
52.00	247.0
55.00	159.0
56.00	836.0
57.10	1306.0
58.10	103.0
59.90	615.0
61.00	2760.0
62.00	2824.0
63.00	2624.0
64.00	577.0
65.00	560.0
65.80	100.0
66.90	339.0
68.00	5720.0
69.00	5434.0
69.90	456.0
72.00	284.0
73.00	2170.0
74.00	8753.0
75.00	26168.0
76.10	2309.0
77.00	297.0
78.00	320.0
78.90	2587.0
79.90	751.0
80.90	2549.0
81.90	593.0
85.90	120.0
87.00	2143.0
87.90	2306.0
90.90	322.0
92.00	1826.0
93.00	2536.0
94.00	6678.0
95.00	53792.0
96.10	3619.0
103.90	312.0
105.90	249.0
110.00	147.0
115.00	100.0
116.00	182.0
116.80	524.0
117.70	282.0
119.00	378.0
127.90	222.0
128.90	221.0
129.90	280.0
137.00	196.0
140.80	507.0
142.90	999.0
144.90	607.0
145.80	102.0
147.80	120.0
149.00	104.0
154.90	147.0
156.90	175.0
170.90	232.0
171.90	438.0
174.00	40792.0
175.00	3410.0
176.00	39784.0
177.00	2836.0

Instrument :
MSVOA_V
ClientSampleId :
BFB353

m/z	Abundance
36.10	475.0
37.00	2875.0
38.00	2372.0
39.00	1021.0
39.80	356.0
40.90	117.0
44.00	623.0
45.10	602.0
46.00	161.0
47.00	783.0
47.90	358.0
49.00	2203.0
50.00	9816.0
51.00	3277.0
52.00	259.0
52.70	140.0
53.20	118.0
55.10	163.0
56.00	922.0
57.00	1501.0
58.00	125.0
59.90	618.0
61.00	2862.0
62.00	2828.0
63.00	2726.0
64.00	583.0
65.00	610.0
65.80	103.0
67.00	351.0
68.00	6011.0
69.00	5722.0
70.00	347.0
71.90	331.0
73.00	2471.0
74.00	9515.0
75.00	28432.0
76.10	2346.0
77.00	308.0
78.00	376.0
78.90	2731.0
80.00	740.0
81.00	2673.0
81.90	588.0
87.00	2387.0
87.90	2352.0
90.90	359.0
92.00	1972.0
93.00	2614.0
94.00	7326.0
95.00	58152.0
96.10	3809.0
96.90	122.0
103.90	304.0
104.90	118.0
105.90	291.0
108.10	101.0
110.00	121.0
113.10	108.0
115.00	106.0
115.90	209.0
116.80	506.0
117.70	302.0
119.10	358.0
127.90	281.0
128.90	173.0
129.90	322.0
134.70	105.0
137.00	193.0
140.80	525.0
143.00	1106.0
144.90	603.0
147.80	161.0
154.90	176.0
156.90	185.0
171.00	312.0
172.00	483.0
174.00	44096.0
175.00	3562.0
176.00	43648.0
177.00	2875.0

Instrument :
MSVOA_V
ClientSampleId :
BFB353

m/z	Abundance
36.10	465.0
37.00	2654.0
38.00	2416.0
39.00	973.0
39.80	403.0
40.90	103.0
44.00	696.0
45.00	567.0
45.90	156.0
47.10	656.0
48.00	330.0
49.00	2305.0
50.00	9510.0
51.00	3193.0
52.00	240.0
52.80	127.0
53.20	127.0
55.10	160.0
56.00	872.0
57.00	1518.0
57.90	115.0
60.00	608.0
61.00	2728.0
62.00	2710.0
63.00	2518.0
64.00	543.0
65.00	561.0
67.00	300.0
68.00	5564.0
69.00	5636.0
70.10	345.0
71.00	117.0
71.90	317.0
73.00	2467.0
74.00	9273.0
75.00	28144.0
76.10	2215.0
76.90	314.0
78.00	343.0
78.90	2625.0
79.90	663.0
81.00	2594.0
81.90	553.0
87.00	2458.0
87.90	2254.0
91.00	333.0
92.00	1830.0
93.00	2473.0
94.00	7301.0
95.00	56280.0
96.10	3689.0
96.90	130.0
103.90	284.0
105.00	142.0
105.90	299.0
113.10	111.0
115.00	111.0
115.90	236.0
116.90	495.0
117.70	291.0
118.80	346.0
127.90	303.0
128.90	116.0
129.90	272.0
136.90	146.0
140.90	486.0
143.00	1177.0
145.00	564.0
147.80	176.0
154.90	165.0
156.90	149.0
171.00	329.0
172.00	506.0
173.00	768.0
174.00	43416.0
175.00	3345.0
176.00	43424.0
177.00	2666.0

Instrument :
MSVOA_V
ClientSampleId :
BFB353