

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
 Data File : VV031800.D
 Acq On : 15 Aug 2023 10:47
 Operator : SY/MD
 Sample : VV0815WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK377

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

Signal : TIC: VV031800.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	220914	233883	13.24%	1.786%
2	1.532	146	153	169	rVB	222237	266521	15.09%	2.035%
3	2.060	308	317	332	rBV	392378	566889	32.09%	4.328%
4	2.577	473	478	481	rBV5	1626	1850	0.10%	0.014%
5	2.693	511	514	518	rBV5	1850	1568	0.09%	0.012%
6	2.764	534	536	538	rBV2	1139	327	0.02%	0.002%
7	2.841	558	560	562	rBV2	903	446	0.03%	0.003%
8	2.918	581	584	585	rBV	816	370	0.02%	0.003%
9	2.966	596	599	601	rBV4	988	652	0.04%	0.005%
10	3.079	631	634	636	rBV2	1486	1037	0.06%	0.008%
11	3.092	636	638	640	rVB3	1256	456	0.03%	0.003%
12	3.140	650	653	655	rBV3	962	703	0.04%	0.005%
13	3.195	668	670	672	rVB2	745	281	0.02%	0.002%
14	3.207	672	674	676	rVB2	1333	508	0.03%	0.004%
15	3.230	676	681	683	rBV5	1394	1023	0.06%	0.008%
16	3.249	683	687	690	rBV5	941	812	0.05%	0.006%
17	3.343	713	716	718	rBV3	1049	716	0.04%	0.005%
18	3.371	723	725	728	rBV3	1070	736	0.04%	0.006%
19	3.397	732	733	734	rBV	479	135	0.01%	0.001%
20	3.423	739	741	744	rBV3	1308	738	0.04%	0.006%
21	3.494	761	763	766	rVB4	1065	502	0.03%	0.004%
22	3.616	798	801	803	rBV3	1035	456	0.03%	0.003%
23	3.635	803	807	809	rVV4	1269	834	0.05%	0.006%
24	3.661	813	815	817	rBV3	611	352	0.02%	0.003%
25	3.680	817	821	822	rBV4	874	550	0.03%	0.004%
26	3.709	827	830	832	rBV3	832	447	0.03%	0.003%
27	3.786	845	854	894	rBV	157739	445645	25.23%	3.402%
28	4.143	963	965	969	rBV4	1749	1152	0.07%	0.009%
29	4.252	985	999	1021	rBV	318278	815813	46.18%	6.228%
30	4.632	1115	1117	1119	rBV4	969	405	0.02%	0.003%
31	4.822	1173	1176	1178	rBV4	1294	842	0.05%	0.006%
32	4.899	1195	1200	1201	rBV5	1605	1262	0.07%	0.010%
33	4.960	1201	1219	1245	rBV2	648731	1766452	100.00%	13.486%
34	5.320	1328	1331	1332	rBV3	1614	832	0.05%	0.006%
35	5.432	1364	1366	1370	rBV5	1704	1556	0.09%	0.012%
36	5.539	1385	1399	1422	rBV	419520	884906	50.10%	6.756%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
 Data File : VV031800.D
 Acq On : 15 Aug 2023 10:47
 Operator : SY/MD
 Sample : VV0815WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK377

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

37	5.825	1480	1488	1504	rBV3	56264	112190	6.35%	0.857%
38	5.992	1527	1540	1560	rBV	435586	908000	51.40%	6.932%
39	6.500	1694	1698	1699	rBV4	1573	861	0.05%	0.007%
40	6.551	1711	1714	1716	rBV4	2120	1585	0.09%	0.012%
41	6.645	1741	1743	1745	rBV2	1232	852	0.05%	0.007%
42	6.757	1776	1778	1781	rBV4	1393	932	0.05%	0.007%
43	6.789	1785	1788	1790	rBV4	932	653	0.04%	0.005%
44	6.825	1797	1799	1803	rBV5	1148	787	0.04%	0.006%
45	6.918	1818	1828	1849	rBV	175118	330135	18.69%	2.520%
46	7.249	1919	1931	1955	rBV	594233	1075693	60.90%	8.212%
47	7.558	2018	2027	2050	rBV	132146	240128	13.59%	1.833%
48	7.767	2088	2092	2095	rBV5	2655	2595	0.15%	0.020%
49	7.989	2157	2161	2163	rBV4	1412	800	0.05%	0.006%
50	8.030	2164	2174	2210	rBV	456022	958774	54.28%	7.320%
51	8.789	2399	2410	2433	rBV	711981	1185694	67.12%	9.052%
52	9.117	2509	2512	2515	rBV5	1766	1510	0.09%	0.012%
53	9.329	2576	2578	2581	rBV4	972	432	0.02%	0.003%
54	9.477	2623	2624	2626	rBV2	1511	704	0.04%	0.005%
55	9.551	2644	2647	2648	rBV3	1344	796	0.05%	0.006%
56	9.709	2694	2696	2698	rBV3	562	311	0.02%	0.002%
57	9.741	2704	2706	2710	rBV6	966	557	0.03%	0.004%
58	10.088	2812	2814	2815	rBV2	576	230	0.01%	0.002%
59	10.159	2824	2836	2857	rBV	596988	962078	54.46%	7.345%
60	10.477	2932	2935	2937	rBV4	1406	984	0.06%	0.008%
61	10.593	2963	2971	2973	rBV7	1234	1366	0.08%	0.010%
62	10.603	2973	2974	2976	rBV2	804	325	0.02%	0.002%
63	10.699	3000	3004	3008	rBV5	1014	799	0.05%	0.006%
64	10.796	3033	3034	3037	rBV3	1222	673	0.04%	0.005%
65	10.943	3077	3080	3082	rBV4	1109	834	0.05%	0.006%
66	10.988	3090	3094	3095	rBV4	1041	799	0.05%	0.006%
67	11.072	3118	3120	3121	rBV2	623	224	0.01%	0.002%
68	11.191	3146	3157	3179	rBV	690235	1077482	61.00%	8.226%
69	11.567	3262	3274	3291	rBV	772576	1218426	68.98%	9.302%
70	12.439	3542	3545	3546	rBV3	1193	747	0.04%	0.006%
71	12.477	3554	3557	3562	rBV7	1335	1504	0.09%	0.011%
72	12.564	3581	3584	3588	rBV5	3011	2860	0.16%	0.022%
73	12.583	3588	3590	3592	rVV3	1597	820	0.05%	0.006%
74	12.731	3633	3636	3637	rBV3	1473	734	0.04%	0.006%
75	12.808	3657	3660	3664	rBV5	1731	1602	0.09%	0.012%
76	13.840	3979	3981	3982	rBV2	1081	436	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
Data File : VV031800.D
Acq On : 15 Aug 2023 10:47
Operator : SY/MD
Sample : VV0815WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK377

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Title : VOC Analysis




Sum of corrected areas: 13098569

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
Data File : VV031800.D
Acq On : 15 Aug 2023 10:47
Operator : SY/MD
Sample : VV0815WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK377

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

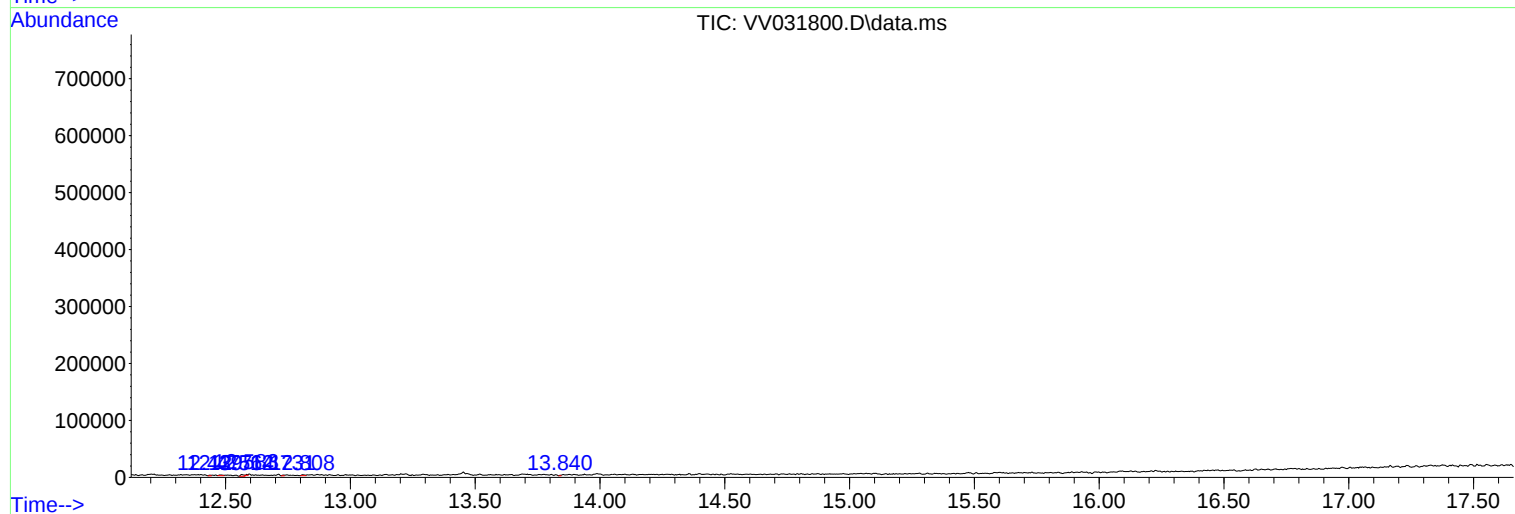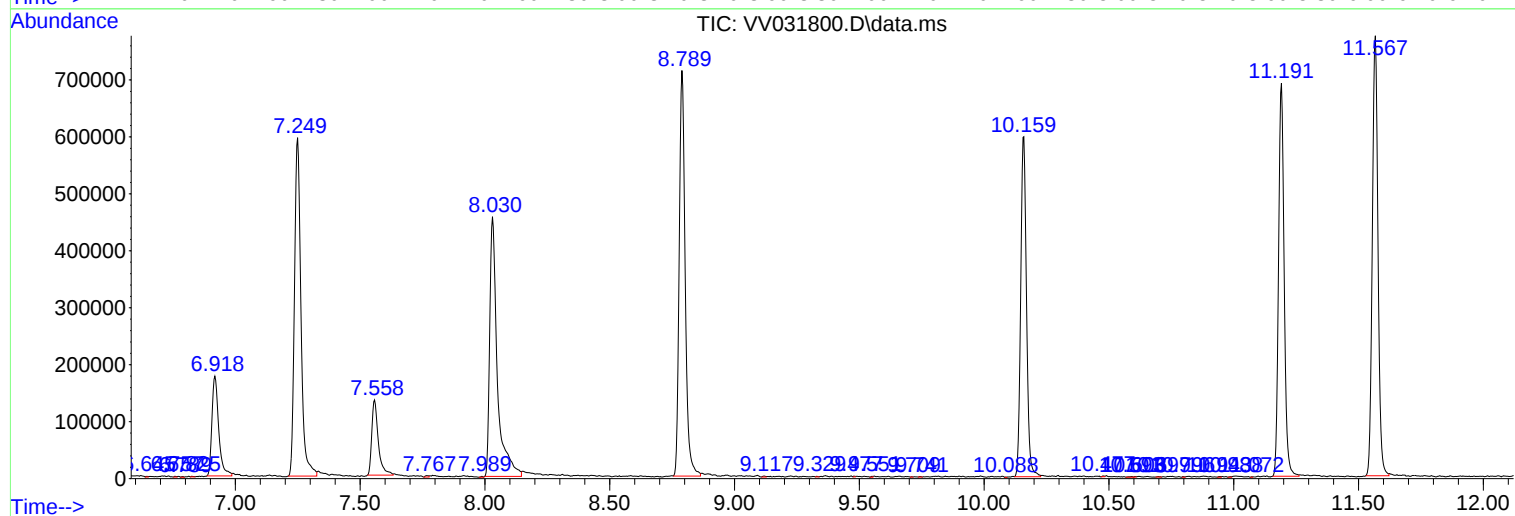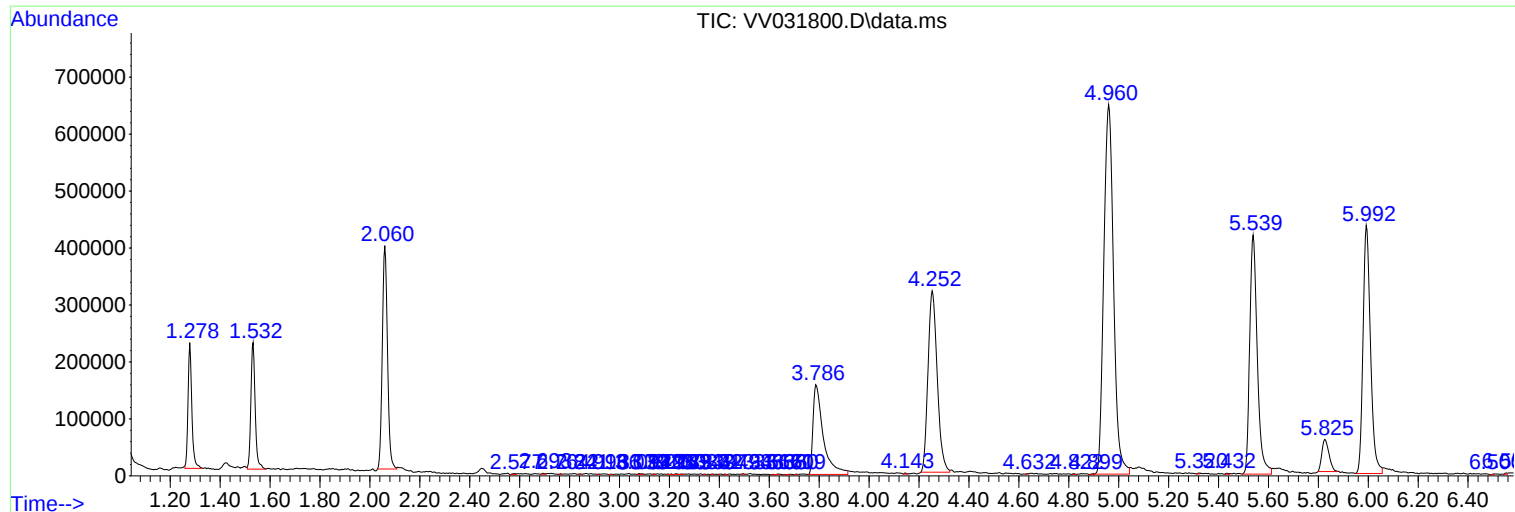

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
Data File : VV031800.D
Acq On : 15 Aug 2023 10:47
Operator : SY/MD
Sample : VV0815WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK377

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
Data File : VV031800.D
Acq On : 15 Aug 2023 10:47
Operator : SY/MD
Sample : VV0815WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK377

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc