

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
 Data File : VV031801.D
 Acq On : 15 Aug 2023 11:19
 Operator : SY/MD
 Sample : 03965-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4880

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

Signal : TIC: VV031801.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	208804	225635	13.00%	1.682%
2	1.532	145	153	169	rVB	210604	256690	14.79%	1.914%
3	2.060	307	317	326	rBV	379618	554283	31.94%	4.133%
4	2.114	327	334	353	rVB	127269	204413	11.78%	1.524%
5	2.455	431	440	444	rBV9	4043	5268	0.30%	0.039%
6	2.555	466	471	473	rBV5	3261	3171	0.18%	0.024%
7	2.696	511	515	518	rBV6	2464	1756	0.10%	0.013%
8	2.796	543	546	549	rVB5	1422	939	0.05%	0.007%
9	2.818	549	553	556	rBV5	1216	1117	0.06%	0.008%
10	2.896	573	577	583	rVB7	1478	1551	0.09%	0.012%
11	3.021	611	616	618	rBV4	1295	1047	0.06%	0.008%
12	3.111	641	644	647	rBV3	1708	1358	0.08%	0.010%
13	3.195	667	670	672	rVV4	1073	935	0.05%	0.007%
14	3.233	676	682	685	rVV5	1249	979	0.06%	0.007%
15	3.455	748	751	755	rVV3	1245	891	0.05%	0.007%
16	3.503	765	766	772	rVB5	1723	1186	0.07%	0.009%
17	3.535	772	776	778	rBV4	1069	878	0.05%	0.007%
18	3.709	827	830	833	rVB5	1418	927	0.05%	0.007%
19	3.789	845	855	884	rBV	146465	416896	24.02%	3.109%
20	4.111	953	955	961	rVB6	1873	1246	0.07%	0.009%
21	4.137	961	963	968	rVB5	2054	1644	0.09%	0.012%
22	4.162	968	971	976	rBV6	1642	1389	0.08%	0.010%
23	4.253	982	999	1027	rBV	315382	825770	47.58%	6.157%
24	4.574	1094	1099	1102	rBV5	2268	2190	0.13%	0.016%
25	4.690	1130	1135	1137	rBV5	1423	1237	0.07%	0.009%
26	4.703	1137	1139	1142	rBV3	1633	925	0.05%	0.007%
27	4.896	1192	1199	1201	rBV6	1428	1478	0.09%	0.011%
28	4.960	1201	1219	1244	rBV2	634761	1735633	100.00%	12.942%
29	5.285	1319	1320	1324	rBV4	1301	999	0.06%	0.007%
30	5.423	1360	1363	1368	rVB4	1377	1172	0.07%	0.009%
31	5.452	1368	1372	1376	rVB6	1494	1264	0.07%	0.009%
32	5.474	1376	1379	1382	rBV4	1239	896	0.05%	0.007%
33	5.539	1386	1399	1422	rBV	426355	899606	51.83%	6.708%
34	5.825	1476	1488	1509	rBV2	73717	157184	9.06%	1.172%
35	5.992	1525	1540	1572	rBV	426937	907284	52.27%	6.765%
36	6.323	1641	1643	1645	rBV3	1572	933	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
 Data File : VV031801.D
 Acq On : 15 Aug 2023 11:19
 Operator : SY/MD
 Sample : 03965-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4880

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

37	6.558	1709	1716	1718	rBV6	3943	4735	0.27%	0.035%
38	6.863	1807	1811	1816	rBV4	1994	2256	0.13%	0.017%
39	6.918	1816	1828	1852	rBV2	170929	337093	19.42%	2.514%
40	7.249	1918	1931	1953	rBV	577366	1061883	61.18%	7.918%
41	7.510	2010	2012	2015	rVB2	1989	957	0.06%	0.007%
42	7.558	2015	2027	2051	rBV	133243	251218	14.47%	1.873%
43	7.770	2091	2093	2098	rVB4	1755	1168	0.07%	0.009%
44	7.793	2098	2100	2104	rVB5	1845	1069	0.06%	0.008%
45	7.883	2120	2128	2138	rVV6	6305	12530	0.72%	0.093%
46	8.030	2164	2174	2206	rBV2	420884	898435	51.76%	6.699%
47	8.191	2218	2224	2232	rVB2	9880	15319	0.88%	0.114%
48	8.744	2393	2396	2397	rBV3	1375	881	0.05%	0.007%
49	8.789	2397	2410	2441	rVV	719393	1210554	69.75%	9.026%
50	8.995	2472	2474	2478	rBV4	1321	888	0.05%	0.007%
51	9.047	2487	2490	2494	rBV5	2131	1932	0.11%	0.014%
52	9.207	2538	2540	2544	rBV5	2517	2115	0.12%	0.016%
53	9.352	2582	2585	2588	rBV5	1427	1097	0.06%	0.008%
54	9.465	2616	2620	2622	rBV4	1282	971	0.06%	0.007%
55	9.487	2622	2627	2628	rBV5	2714	2037	0.12%	0.015%
56	9.651	2674	2678	2680	rBV5	1414	1103	0.06%	0.008%
57	9.728	2697	2702	2703	rBV5	1517	912	0.05%	0.007%
58	9.760	2707	2712	2719	rBV9	4226	6862	0.40%	0.051%
59	9.879	2747	2749	2753	rBV4	1334	963	0.06%	0.007%
60	10.117	2821	2823	2824	rVV2	2132	1074	0.06%	0.008%
61	10.159	2824	2836	2857	rVV	543631	875190	50.42%	6.526%
62	10.329	2882	2889	2899	rVB5	13014	21467	1.24%	0.160%
63	10.403	2906	2912	2914	rBV7	1918	2137	0.12%	0.016%
64	10.651	2983	2989	2994	rBV7	1855	2603	0.15%	0.019%
65	10.815	3035	3040	3043	rBV7	881	998	0.06%	0.007%
66	10.921	3071	3073	3077	rBV6	1472	1162	0.07%	0.009%
67	11.101	3121	3129	3132	rBV7	5390	7630	0.44%	0.057%
68	11.191	3145	3157	3176	rBV	711374	1107084	63.79%	8.255%
69	11.497	3242	3252	3263	rBV4	20781	46581	2.68%	0.347%
70	11.564	3263	3273	3291	rVB	778893	1227761	70.74%	9.155%
71	11.911	3380	3381	3385	rBV4	1744	1198	0.07%	0.009%
72	11.947	3385	3392	3402	rBV6	11377	19163	1.10%	0.143%
73	12.120	3443	3446	3449	rBV4	1502	1134	0.07%	0.008%
74	12.201	3464	3471	3478	rVB3	6984	10259	0.59%	0.076%
75	12.259	3481	3489	3493	rBV9	8784	12622	0.73%	0.094%
76	12.371	3521	3524	3527	rVB5	1764	1141	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
 Data File : VV031801.D
 Acq On : 15 Aug 2023 11:19
 Operator : SY/MD
 Sample : 03965-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4880

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

77	12.464	3551	3553	3556	rVV4	1448	898	0.05%	0.007%
78	12.487	3556	3560	3564	rVB6	1119	1074	0.06%	0.008%
79	12.525	3569	3572	3577	rBV7	1843	1264	0.07%	0.009%
80	12.580	3586	3589	3594	rBV6	1462	1648	0.09%	0.012%
81	12.841	3664	3670	3673	rBV8	1313	1497	0.09%	0.011%
82	12.863	3675	3677	3683	rVB7	2280	1867	0.11%	0.014%
83	12.895	3683	3687	3694	rBV7	1463	1443	0.08%	0.011%
84	13.069	3737	3741	3744	rBV5	1462	1417	0.08%	0.011%
85	13.252	3796	3798	3800	rBV3	1658	926	0.05%	0.007%
86	13.355	3828	3830	3835	rBV5	1393	969	0.06%	0.007%
87	13.384	3837	3839	3844	rVB6	2182	1678	0.10%	0.013%
88	13.410	3844	3847	3850	rBV4	1247	913	0.05%	0.007%
89	13.577	3897	3899	3902	rVV3	1419	989	0.06%	0.007%
90	13.612	3906	3910	3912	rVV4	1462	1010	0.06%	0.008%
91	14.117	4059	4067	4069	rBV9	2044	2433	0.14%	0.018%
92	14.210	4089	4096	4098	rBV7	2174	2301	0.13%	0.017%
93	14.281	4114	4118	4123	rBV5	1400	1455	0.08%	0.011%
94	14.358	4140	4142	4149	rVB5	2225	1848	0.11%	0.014%
95	14.445	4164	4169	4172	rBV5	1090	1242	0.07%	0.009%
96	14.686	4242	4244	4248	rVB5	2265	1608	0.09%	0.012%
97	14.750	4259	4264	4265	rBV4	1813	1611	0.09%	0.012%
98	14.837	4288	4291	4293	rBV4	1489	1140	0.07%	0.009%
99	14.963	4323	4330	4333	rBV7	1999	2185	0.13%	0.016%
100	15.062	4358	4361	4362	rBV3	1655	914	0.05%	0.007%




Sum of corrected areas: 13411282

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
Data File : VV031801.D
Acq On : 15 Aug 2023 11:19
Operator : SY/MD
Sample : 03965-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4880

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

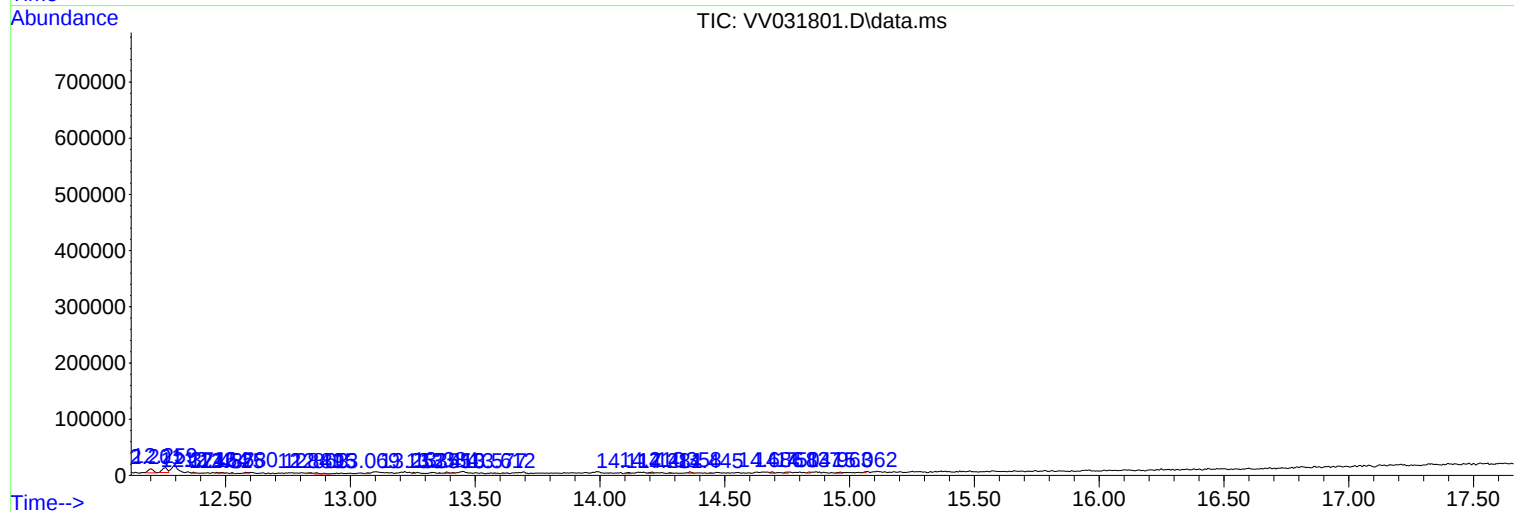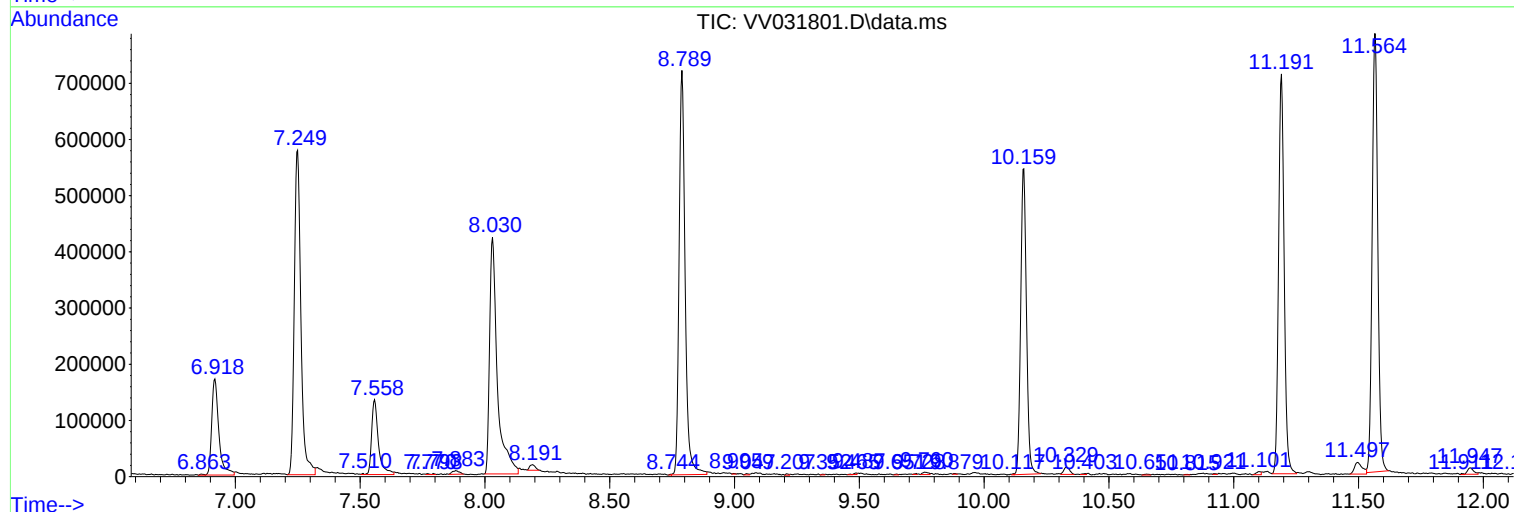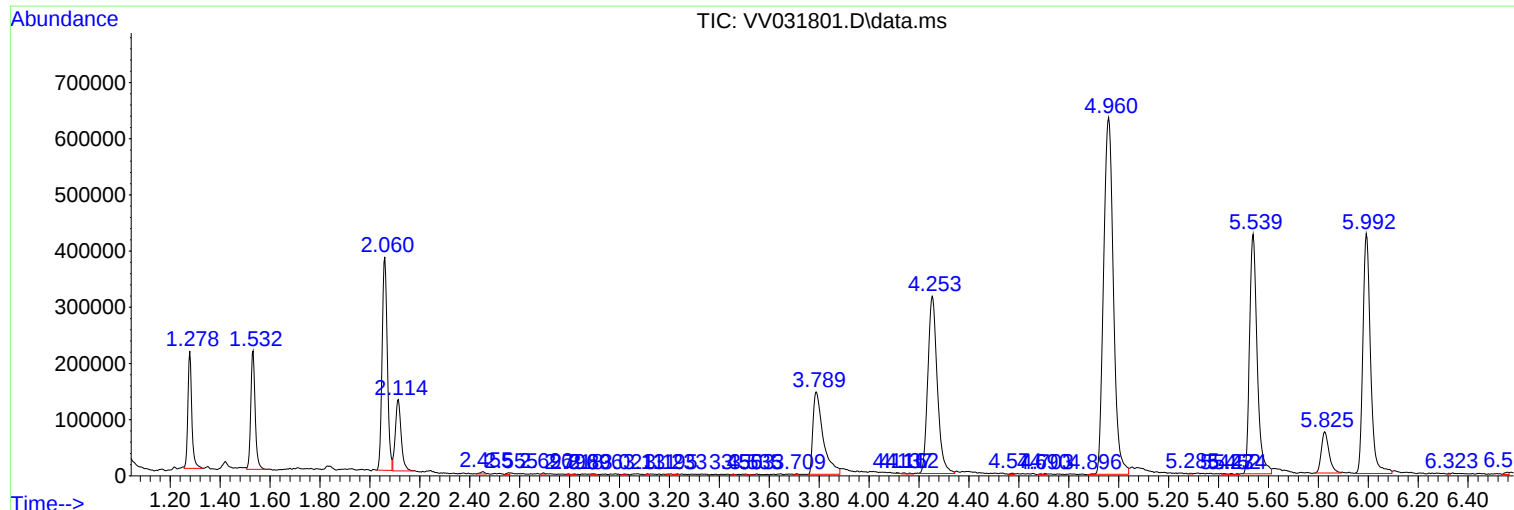

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
Data File : VV031801.D
Acq On : 15 Aug 2023 11:19
Operator : SY/MD
Sample : 03965-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4880

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
Data File : VV031801.D
Acq On : 15 Aug 2023 11:19
Operator : SY/MD
Sample : 03965-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4880

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc