

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
 Data File : VV031802.D
 Acq On : 15 Aug 2023 11:42
 Operator : SY/MD
 Sample : 03967-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A48A0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

Signal : TIC: VV031802.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rVB	194420	205698	11.93%	1.533%
2	1.420	113	118	123	rBV8	12457	14925	0.87%	0.111%
3	1.532	146	153	166	rVB	200452	238645	13.84%	1.778%
4	2.060	307	317	326	rBV	371914	534317	30.99%	3.981%
5	2.114	327	334	348	rVB	134404	209325	12.14%	1.560%
6	2.439	430	435	437	rBV4	2448	2250	0.13%	0.017%
7	2.494	449	452	456	rBV6	1859	1466	0.09%	0.011%
8	2.548	466	469	472	rBV4	1943	1491	0.09%	0.011%
9	2.613	484	489	493	rVB7	1565	1584	0.09%	0.012%
10	2.764	533	536	540	rBV4	1324	1029	0.06%	0.008%
11	2.844	558	561	564	rVB4	1348	917	0.05%	0.007%
12	2.905	575	580	584	rVV5	821	943	0.05%	0.007%
13	3.063	625	629	631	rBV3	1298	1013	0.06%	0.008%
14	3.111	641	644	646	rBV3	1619	993	0.06%	0.007%
15	3.262	683	691	693	rVB5	855	939	0.05%	0.007%
16	3.339	712	715	720	rBV6	1184	981	0.06%	0.007%
17	3.532	772	775	779	rVB5	1776	1310	0.08%	0.010%
18	3.564	779	785	790	rBV8	1068	1320	0.08%	0.010%
19	3.661	811	815	818	rBV4	920	977	0.06%	0.007%
20	3.725	832	835	838	rVB3	1421	922	0.05%	0.007%
21	3.789	845	855	890	rBV	157960	460454	26.70%	3.431%
22	4.256	984	1000	1027	rBV	303561	806028	46.75%	6.005%
23	4.642	1115	1120	1123	rBV6	1703	1707	0.10%	0.013%
24	4.677	1128	1131	1137	rVB4	1258	1114	0.06%	0.008%
25	4.738	1145	1150	1152	rBV5	1486	1195	0.07%	0.009%
26	4.863	1186	1189	1194	rVB4	1666	1181	0.07%	0.009%
27	4.960	1200	1219	1245	rBV2	634553	1724308	100.00%	12.847%
28	5.539	1387	1399	1421	rBV	404208	847010	49.12%	6.311%
29	5.825	1476	1488	1509	rBV2	95921	206426	11.97%	1.538%
30	5.995	1526	1541	1561	rBV	424732	886718	51.42%	6.606%
31	6.217	1607	1610	1615	rBV7	1873	1663	0.10%	0.012%
32	6.246	1616	1619	1621	rBV3	1775	1183	0.07%	0.009%
33	6.339	1644	1648	1652	rBV6	1461	1257	0.07%	0.009%
34	6.449	1680	1682	1686	rVB5	1507	912	0.05%	0.007%
35	6.564	1708	1718	1719	rBV7	3585	4289	0.25%	0.032%
36	6.584	1722	1724	1727	rBV4	2085	1196	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
 Data File : VV031802.D
 Acq On : 15 Aug 2023 11:42
 Operator : SY/MD
 Sample : 03967-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A48A0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

37	6.918	1815	1828	1860	rBV	174047	345016	20.01%	2.570%
38	7.124	1881	1892	1897	rBV	3929	7175	0.42%	0.053%
39	7.249	1919	1931	1951	rBV	573389	1038784	60.24%	7.739%
40	7.432	1986	1988	1996	rVB6	1553	1646	0.10%	0.012%
41	7.558	2018	2027	2054	rBV	132440	243216	14.11%	1.812%
42	7.821	2105	2109	2112	rBV5	1565	1145	0.07%	0.009%
43	7.844	2112	2116	2119	rBV4	1247	959	0.06%	0.007%
44	7.886	2119	2129	2139	rBV3	11694	22251	1.29%	0.166%
45	8.030	2162	2174	2210	rBV2	468355	1018867	59.09%	7.591%
46	8.188	2218	2223	2240	rVB8	18359	35257	2.04%	0.263%
47	8.725	2388	2390	2393	rVB4	2024	1158	0.07%	0.009%
48	8.744	2393	2396	2398	rBV3	1511	983	0.06%	0.007%
49	8.789	2399	2410	2442	rBV	698635	1161076	67.34%	8.650%
50	8.940	2455	2457	2461	rBV4	1474	1218	0.07%	0.009%
51	9.622	2667	2669	2672	rVB3	1644	933	0.05%	0.007%
52	9.677	2678	2686	2689	rBV7	2793	3063	0.18%	0.023%
53	9.764	2706	2713	2725	rBV7	4853	9360	0.54%	0.070%
54	9.960	2771	2774	2779	rVB6	2731	2151	0.12%	0.016%
55	10.082	2809	2812	2816	rBV5	1131	914	0.05%	0.007%
56	10.159	2821	2836	2857	rBV	512838	844609	48.98%	6.293%
57	10.329	2880	2889	2899	rBV2	22100	33300	1.93%	0.248%
58	10.455	2925	2928	2930	rBV4	1540	1145	0.07%	0.009%
59	10.561	2960	2961	2965	rVB4	2214	966	0.06%	0.007%
60	10.599	2965	2973	2976	rVB8	1880	2701	0.16%	0.020%
61	10.686	2998	3000	3006	rVB7	1517	1220	0.07%	0.009%
62	10.738	3012	3016	3018	rBV4	1096	888	0.05%	0.007%
63	10.792	3030	3033	3036	rBV4	1211	903	0.05%	0.007%
64	11.001	3096	3098	3102	rVB5	1773	987	0.06%	0.007%
65	11.085	3119	3124	3125	rBV5	2430	2037	0.12%	0.015%
66	11.101	3125	3129	3134	rVV8	4666	5654	0.33%	0.042%
67	11.191	3146	3157	3181	rBV	685368	1084408	62.89%	8.079%
68	11.297	3186	3190	3196	rVB9	4005	4866	0.28%	0.036%
69	11.390	3215	3219	3224	rVB6	1692	1860	0.11%	0.014%
70	11.432	3229	3232	3236	rVB5	1752	1362	0.08%	0.010%
71	11.461	3239	3241	3244	rBV3	1867	1394	0.08%	0.010%
72	11.497	3244	3252	3262	rBV5	19375	41286	2.39%	0.308%
73	11.564	3263	3273	3290	rVB	785154	1235446	71.65%	9.205%
74	11.950	3386	3393	3404	rBV5	9657	16878	0.98%	0.126%
75	12.027	3414	3417	3418	rBV2	1614	1057	0.06%	0.008%
76	12.062	3426	3428	3435	rVB6	1678	1348	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
 Data File : VV031802.D
 Acq On : 15 Aug 2023 11:42
 Operator : SY/MD
 Sample : 03967-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A48A0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

77	12.136	3447	3451	3453	rBV5	2226	1502	0.09%	0.011%
78	12.201	3462	3471	3479	rBV2	12765	19677	1.14%	0.147%
79	12.255	3479	3488	3494	rBV9	11157	18116	1.05%	0.135%
80	12.484	3555	3559	3564	rVB7	2097	2010	0.12%	0.015%
81	12.513	3564	3568	3570	rVB4	1569	884	0.05%	0.007%
82	12.583	3586	3590	3592	rBV3	1925	1618	0.09%	0.012%
83	12.654	3610	3612	3615	rBV4	1549	1229	0.07%	0.009%
84	13.082	3741	3745	3748	rBV6	3028	3073	0.18%	0.023%
85	13.191	3776	3779	3781	rBV3	1631	1096	0.06%	0.008%
86	13.294	3808	3811	3813	rBV4	1266	965	0.06%	0.007%
87	13.574	3894	3898	3902	rBV6	1533	1425	0.08%	0.011%
88	13.988	4021	4027	4034	rVV10	4106	5204	0.30%	0.039%
89	14.082	4053	4056	4061	rVB4	1506	1225	0.07%	0.009%
90	14.188	4087	4089	4093	rBV5	1449	949	0.06%	0.007%
91	14.242	4103	4106	4108	rBV4	1579	1229	0.07%	0.009%
92	14.304	4123	4125	4130	rVB6	1271	1084	0.06%	0.008%
93	14.355	4136	4141	4146	rBV8	2966	3744	0.22%	0.028%
94	14.541	4196	4199	4202	rBV4	1702	1387	0.08%	0.010%
95	14.831	4286	4289	4293	rBV5	1693	1574	0.09%	0.012%
96	14.979	4332	4335	4338	rBV4	1894	1052	0.06%	0.008%
97	15.040	4351	4354	4356	rBV3	2366	1410	0.08%	0.011%
98	15.143	4383	4386	4387	rBV2	1904	1042	0.06%	0.008%
99	15.570	4517	4519	4521	rBV2	2033	1148	0.07%	0.009%
100	16.165	4701	4704	4707	rBV4	2857	2377	0.14%	0.018%




Sum of corrected areas: 13422193

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
Data File : VV031802.D
Acq On : 15 Aug 2023 11:42
Operator : SY/MD
Sample : 03967-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A48A0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

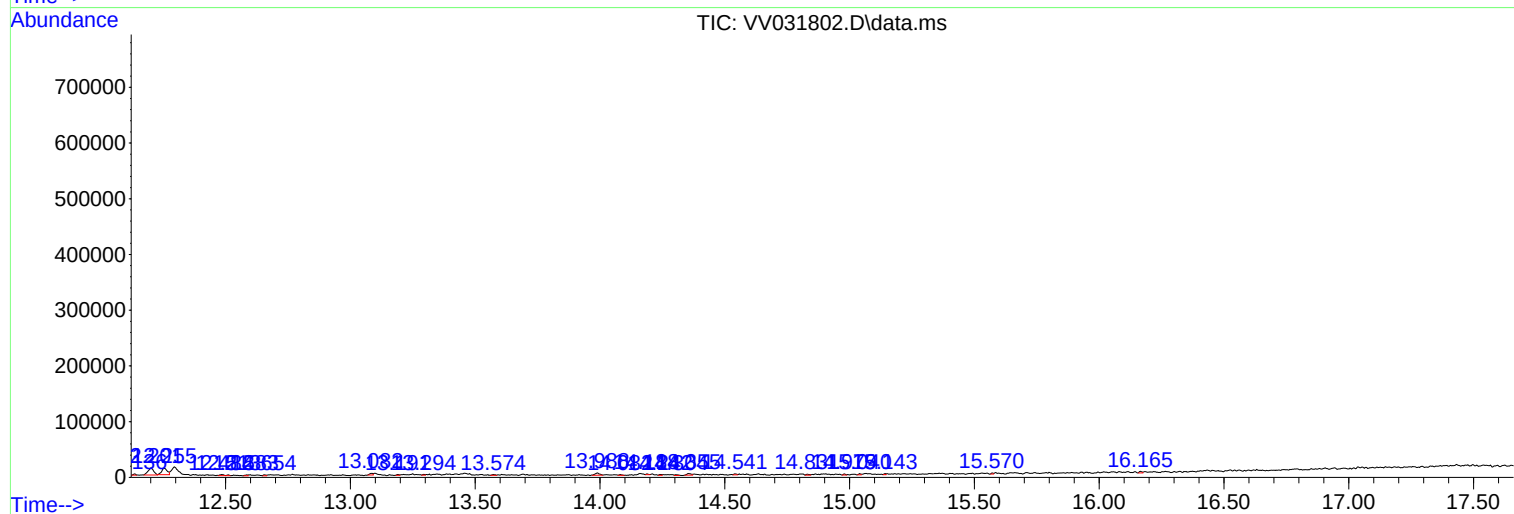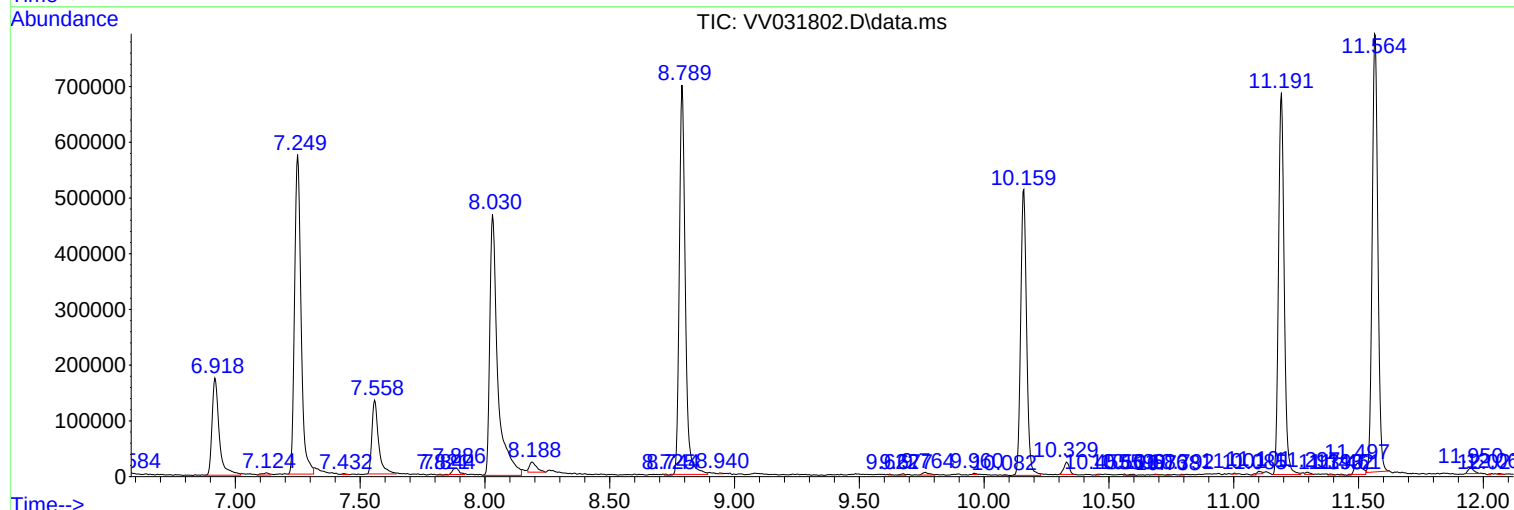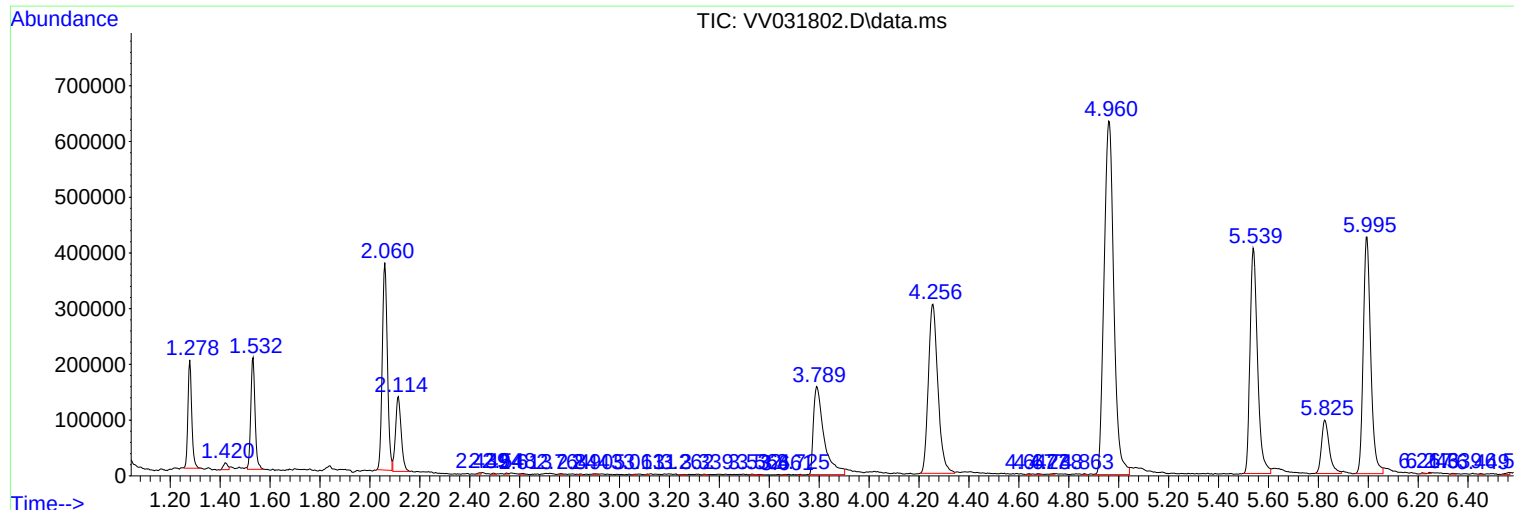

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
Data File : VV031802.D
Acq On : 15 Aug 2023 11:42
Operator : SY/MD
Sample : 03967-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A48A0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
Data File : VV031802.D
Acq On : 15 Aug 2023 11:42
Operator : SY/MD
Sample : 03967-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A48A0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc