

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
 Data File : VV031804.D
 Acq On : 15 Aug 2023 12:29
 Operator : SY/MD
 Sample : 03965-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4880

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M

Title : VOC Analysis

Signal : TIC: VV031804.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	173729	186587	11.18%	1.502%
2	1.532	146	153	168	rVB	190633	235482	14.10%	1.896%
3	2.059	309	317	326	rBV	317385	445538	26.69%	3.586%
4	2.513	455	458	462	rBV5	1626	1307	0.08%	0.011%
5	2.654	500	502	505	rVB3	1778	913	0.05%	0.007%
6	2.670	505	507	509	rBV3	1067	595	0.04%	0.005%
7	2.715	515	521	522	rBV5	1605	1204	0.07%	0.010%
8	2.773	536	539	540	rBV2	609	295	0.02%	0.002%
9	2.783	540	542	546	rVB4	856	443	0.03%	0.004%
10	2.805	546	549	550	rBV3	855	474	0.03%	0.004%
11	2.822	552	554	556	rVB3	761	295	0.02%	0.002%
12	2.844	556	561	562	rBV2	1315	789	0.05%	0.006%
13	2.873	568	570	573	rBV3	881	534	0.03%	0.004%
14	2.921	584	585	588	rBV	658	375	0.02%	0.003%
15	2.957	593	596	601	rBV3	969	993	0.06%	0.008%
16	3.008	609	612	616	rVB4	1075	941	0.06%	0.008%
17	3.027	616	618	623	rBV5	1531	874	0.05%	0.007%
18	3.056	623	627	631	rBV6	916	732	0.04%	0.006%
19	3.082	631	635	636	rBV3	1723	969	0.06%	0.008%
20	3.175	663	664	665	rBV	677	225	0.01%	0.002%
21	3.188	665	668	672	rVB6	1211	905	0.05%	0.007%
22	3.217	672	677	678	rBV5	897	671	0.04%	0.005%
23	3.243	683	685	687	rVV3	850	419	0.03%	0.003%
24	3.285	695	698	703	rBV6	1206	1008	0.06%	0.008%
25	3.339	713	715	716	rBV2	415	191	0.01%	0.002%
26	3.346	716	717	719	rVV2	954	402	0.02%	0.003%
27	3.362	719	722	723	rVV2	850	382	0.02%	0.003%
28	3.371	723	725	729	rVB4	1228	668	0.04%	0.005%
29	3.394	729	732	735	rBV3	758	580	0.03%	0.005%
30	3.413	736	738	741	rVB3	605	263	0.02%	0.002%
31	3.439	744	746	747	rBV2	459	247	0.01%	0.002%
32	3.490	759	762	765	rBV4	1132	927	0.06%	0.007%
33	3.539	776	777	778	rBV4	875	265	0.02%	0.002%
34	3.561	781	784	787	rVV5	1050	865	0.05%	0.007%
35	3.606	795	798	799	rBV3	1110	649	0.04%	0.005%
36	3.625	803	804	805	rBV	680	203	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
 Data File : VV031804.D
 Acq On : 15 Aug 2023 12:29
 Operator : SY/MD
 Sample : 03965-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4880

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

37	3.744	839	841	842	rBV	532	212	0.01%	0.002%
38	3.789	845	855	879	rBV2	167618	443197	26.55%	3.568%
39	4.256	985	1000	1031	rVB	294080	766310	45.90%	6.169%
40	4.555	1090	1093	1098	rBV7	1681	1797	0.11%	0.014%
41	4.741	1148	1151	1152	rBV3	807	432	0.03%	0.003%
42	4.780	1158	1163	1164	rBV3	1315	914	0.05%	0.007%
43	4.815	1170	1174	1177	rVB5	1067	876	0.05%	0.007%
44	4.834	1177	1180	1182	rBV3	961	562	0.03%	0.005%
45	4.863	1187	1189	1194	rBV6	691	601	0.04%	0.005%
46	4.886	1194	1196	1198	rVB2	978	429	0.03%	0.003%
47	4.899	1198	1200	1201	rBV	820	434	0.03%	0.003%
48	4.960	1201	1219	1251	rBV2	609630	1669534	100.00%	13.439%
49	5.538	1387	1399	1423	rBV2	377117	817130	48.94%	6.578%
50	5.828	1479	1489	1507	rBV3	81007	166181	9.95%	1.338%
51	5.995	1529	1541	1559	rBV	407444	839342	50.27%	6.756%
52	6.410	1666	1670	1673	rBV4	2543	2067	0.12%	0.017%
53	6.484	1691	1693	1694	rBV2	846	283	0.02%	0.002%
54	6.526	1704	1706	1707	rBV2	1302	361	0.02%	0.003%
55	6.545	1707	1712	1714	rBV6	1849	1573	0.09%	0.013%
56	6.789	1785	1788	1790	rBV4	964	698	0.04%	0.006%
57	6.828	1797	1800	1801	rBV2	907	456	0.03%	0.004%
58	6.841	1801	1804	1808	rVV6	1101	1059	0.06%	0.009%
59	6.876	1813	1815	1817	rBV4	979	629	0.04%	0.005%
60	6.918	1817	1828	1853	rBV	170409	325275	19.48%	2.618%
61	7.249	1919	1931	1955	rBV	536468	979911	58.69%	7.888%
62	7.558	2018	2027	2052	rBV	129020	239134	14.32%	1.925%
63	7.844	2114	2116	2117	rBV2	1676	626	0.04%	0.005%
64	8.030	2164	2174	2214	rBV2	471860	1019874	61.09%	8.210%
65	8.789	2400	2410	2437	rBV	661075	1092720	65.45%	8.796%
66	9.214	2539	2542	2543	rBV3	1087	513	0.03%	0.004%
67	9.329	2575	2578	2579	rBV3	1181	806	0.05%	0.006%
68	9.365	2585	2589	2591	rVB4	1180	825	0.05%	0.007%
69	9.432	2608	2610	2612	rBV2	732	334	0.02%	0.003%
70	9.448	2612	2615	2617	rVV4	813	488	0.03%	0.004%
71	9.487	2623	2627	2629	rBV3	1680	1305	0.08%	0.011%
72	9.500	2629	2631	2637	rVV7	2963	2798	0.17%	0.023%
73	10.014	2789	2791	2794	rVB3	1508	712	0.04%	0.006%
74	10.101	2816	2818	2821	rBV4	798	499	0.03%	0.004%
75	10.159	2824	2836	2855	rBV	558860	893899	53.54%	7.196%
76	10.329	2879	2889	2898	rBV4	16376	29448	1.76%	0.237%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
 Data File : VV031804.D
 Acq On : 15 Aug 2023 12:29
 Operator : SY/MD
 Sample : 03965-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4880

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M

Title : VOC Analysis

77	10.558	2956	2960	2962	rBV5	1635	1257	0.08%	0.010%
78	10.622	2977	2980	2981	rBV2	1153	661	0.04%	0.005%
79	10.693	2998	3002	3004	rBV5	1378	1278	0.08%	0.010%
80	10.783	3028	3030	3034	rBV4	1114	739	0.04%	0.006%
81	10.857	3051	3053	3058	rBV5	1965	1632	0.10%	0.013%
82	11.191	3146	3157	3178	rBV	644475	1002206	60.03%	8.068%
83	11.390	3217	3219	3222	rBV2	1513	662	0.04%	0.005%
84	11.496	3245	3252	3262	rBV4	22359	38654	2.32%	0.311%
85	11.564	3263	3273	3292	rVB	737903	1174625	70.36%	9.455%
86	12.133	3447	3450	3454	rBV5	2311	1795	0.11%	0.014%
87	12.467	3552	3554	3556	rBV2	1281	536	0.03%	0.004%
88	12.619	3600	3601	3602	rBV	901	266	0.02%	0.002%
89	13.535	3882	3886	3888	rBV5	1853	1694	0.10%	0.014%
90	13.754	3952	3954	3958	rBV4	1255	1137	0.07%	0.009%
91	14.104	4061	4063	4065	rBV2	1993	1019	0.06%	0.008%
92	14.342	4134	4137	4140	rBV4	2233	2140	0.13%	0.017%




Sum of corrected areas: 12422755

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
Data File : VV031804.D
Acq On : 15 Aug 2023 12:29
Operator : SY/MD
Sample : 03965-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4880

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

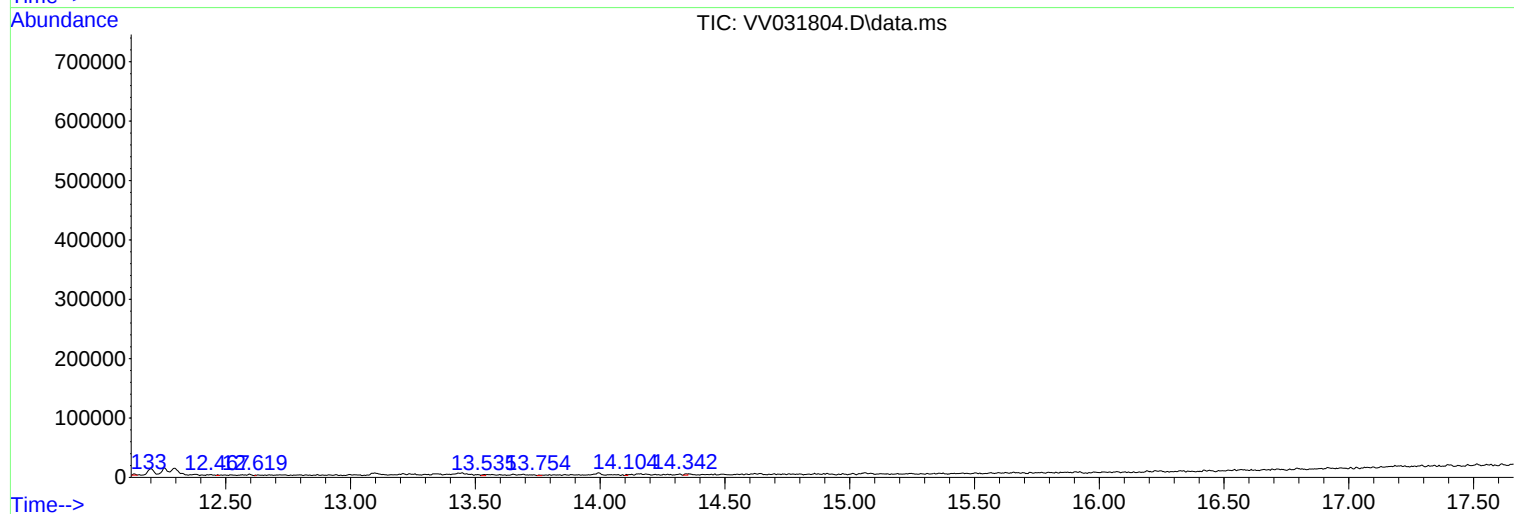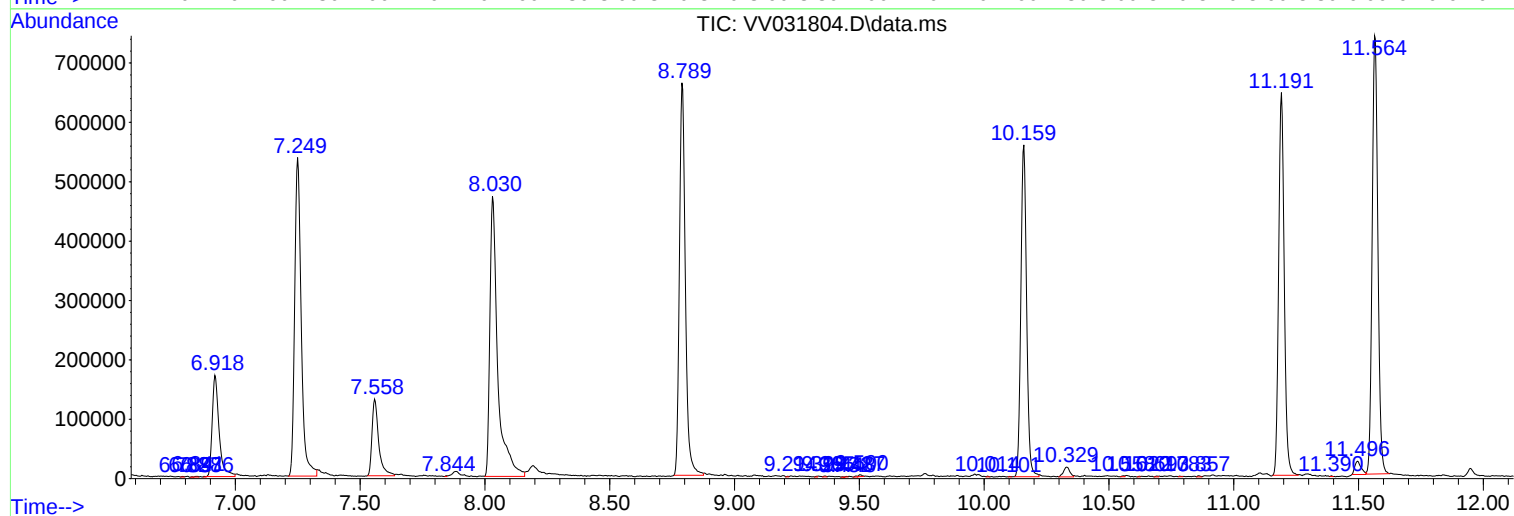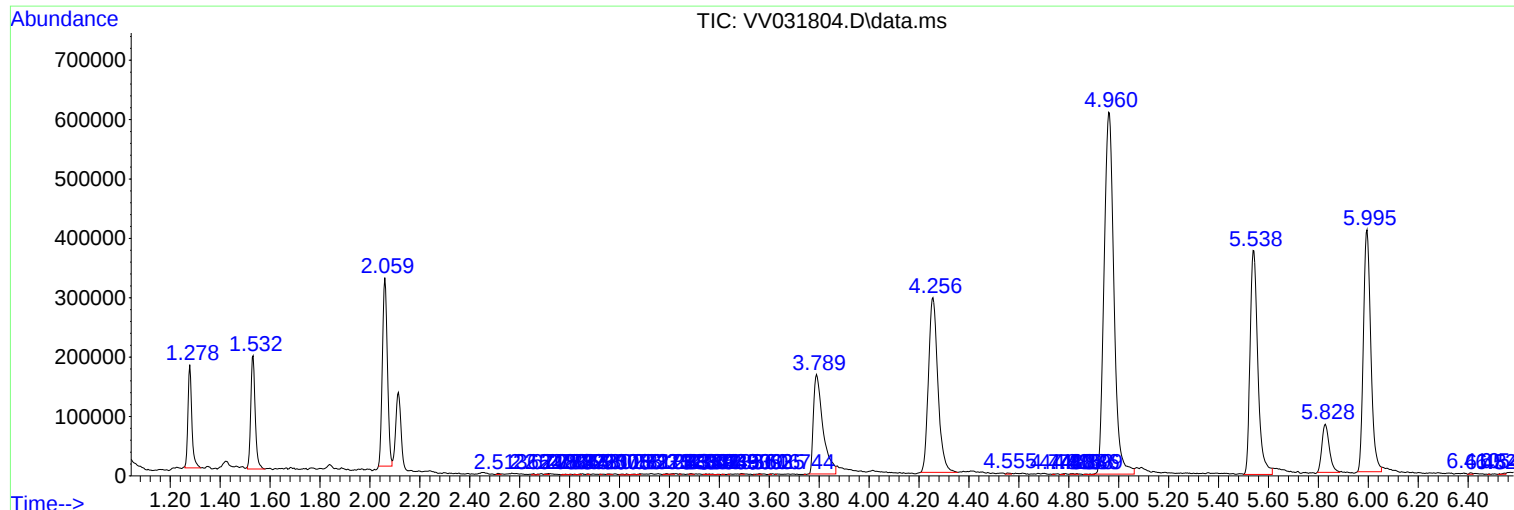

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
Data File : VV031804.D
Acq On : 15 Aug 2023 12:29
Operator : SY/MD
Sample : 03965-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4880

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
Data File : VV031804.D
Acq On : 15 Aug 2023 12:29
Operator : SY/MD
Sample : 03965-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4880

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc