

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
 Data File : VV031805.D
 Acq On : 15 Aug 2023 12:53
 Operator : SY/MD
 Sample : 03967-10ME
 Misc : 5.50g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A48L8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

Signal : TIC: VV031805.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	68	73	91	rVB	128861	182950	11.60%	1.486%
2	2.037	302	310	330	rVB	340133	493486	31.29%	4.007%
3	2.381	410	417	431	rBV2	33027	55772	3.54%	0.453%
4	2.728	524	525	527	rBV2	1123	457	0.03%	0.004%
5	2.799	545	547	549	rBV3	1305	744	0.05%	0.006%
6	2.822	553	554	557	rVB4	1186	582	0.04%	0.005%
7	2.873	567	570	573	rVB5	1937	1179	0.07%	0.010%
8	2.889	573	575	576	rBV3	674	275	0.02%	0.002%
9	2.915	576	583	585	rBV5	1407	1517	0.10%	0.012%
10	3.014	612	614	615	rBV2	1342	548	0.03%	0.004%
11	3.066	628	630	631	rBV2	832	249	0.02%	0.002%
12	3.101	638	641	642	rBV2	1233	725	0.05%	0.006%
13	3.127	646	649	650	rBV2	1117	708	0.04%	0.006%
14	3.175	662	664	665	rBV3	1053	391	0.02%	0.003%
15	3.236	680	683	686	rBV5	543	366	0.02%	0.003%
16	3.256	686	689	692	rVB5	978	510	0.03%	0.004%
17	3.381	723	728	730	rBV4	1523	1165	0.07%	0.009%
18	3.410	735	737	739	rVB2	788	373	0.02%	0.003%
19	3.429	741	743	744	rVB2	799	207	0.01%	0.002%
20	3.452	744	750	751	rBV5	1538	1246	0.08%	0.010%
21	3.471	754	756	758	rVV3	816	361	0.02%	0.003%
22	3.494	758	763	768	rVV7	1837	1726	0.11%	0.014%
23	3.535	774	776	780	rVB5	1459	1081	0.07%	0.009%
24	3.555	780	782	784	rVB3	427	176	0.01%	0.001%
25	3.571	785	787	789	rBV3	893	409	0.03%	0.003%
26	3.593	793	794	795	rBV	494	147	0.01%	0.001%
27	3.616	800	801	804	rVB3	398	125	0.01%	0.001%
28	3.645	804	810	813	rBV7	1486	1318	0.08%	0.011%
29	3.661	813	815	817	rBV3	1254	692	0.04%	0.006%
30	3.735	836	838	840	rBV4	747	370	0.02%	0.003%
31	3.764	844	847	848	rBV3	708	386	0.02%	0.003%
32	3.802	849	859	895	rBV	119606	407810	25.85%	3.312%
33	4.252	982	999	1032	rBV	267158	729330	46.24%	5.922%
34	4.500	1072	1076	1080	rBV7	1760	1698	0.11%	0.014%
35	4.783	1161	1164	1167	rBV5	1805	1282	0.08%	0.010%
36	4.818	1173	1175	1176	rBV2	1167	376	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
 Data File : VV031805.D
 Acq On : 15 Aug 2023 12:53
 Operator : SY/MD
 Sample : 03967-10ME
 Misc : 5.50g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A48L8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

37	4.866	1187	1190	1191	rBV3	1471	684	0.04%	0.006%
38	4.892	1196	1198	1200	rBV2	606	313	0.02%	0.003%
39	4.953	1200	1217	1250	rBV2	601470	1577317	100.00%	12.808%
40	5.297	1319	1324	1327	rBV7	1452	1570	0.10%	0.013%
41	5.371	1345	1347	1351	rBV3	2179	1781	0.11%	0.014%
42	5.538	1387	1399	1424	rBV	412233	888641	56.34%	7.216%
43	5.725	1455	1457	1461	rBV5	2024	1430	0.09%	0.012%
44	5.828	1479	1489	1506	rVB3	47099	100768	6.39%	0.818%
45	5.992	1528	1540	1565	rBV	372224	793821	50.33%	6.446%
46	6.342	1645	1649	1650	rBV5	1219	836	0.05%	0.007%
47	6.374	1656	1659	1667	rVB8	1656	1577	0.10%	0.013%
48	6.410	1667	1670	1675	rBV7	1487	1518	0.10%	0.012%
49	6.448	1679	1682	1685	rBV5	2206	1853	0.12%	0.015%
50	6.513	1700	1702	1703	rBV2	990	460	0.03%	0.004%
51	6.918	1818	1828	1855	rBV3	158554	320223	20.30%	2.600%
52	7.249	1919	1931	1960	rBV	518485	965290	61.20%	7.839%
53	7.558	2019	2027	2049	rBV	118507	231953	14.71%	1.884%
54	7.828	2110	2111	2112	rBV	871	324	0.02%	0.003%
55	7.995	2162	2163	2164	rBV	921	208	0.01%	0.002%
56	8.046	2167	2179	2216	rVV2	363008	944930	59.91%	7.673%
57	8.673	2371	2374	2375	rBV	1326	771	0.05%	0.006%
58	8.718	2383	2388	2391	rBV7	1152	1046	0.07%	0.008%
59	8.792	2398	2411	2431	rBV	673102	1186790	75.24%	9.637%
60	9.059	2492	2494	2497	rBV3	1639	1078	0.07%	0.009%
61	9.300	2566	2569	2570	rBV3	980	546	0.03%	0.004%
62	9.371	2589	2591	2592	rVB2	849	297	0.02%	0.002%
63	9.403	2597	2601	2604	rBV4	1440	1264	0.08%	0.010%
64	9.435	2609	2611	2615	rVB4	2462	1730	0.11%	0.014%
65	9.458	2615	2618	2619	rBV2	1311	888	0.06%	0.007%
66	9.493	2625	2629	2630	rBV4	2235	1420	0.09%	0.012%
67	9.535	2638	2642	2644	rBV4	1755	1446	0.09%	0.012%
68	9.615	2665	2667	2670	rBV4	1224	961	0.06%	0.008%
69	9.651	2676	2678	2679	rBV2	818	410	0.03%	0.003%
70	9.677	2684	2686	2688	rVV2	1137	491	0.03%	0.004%
71	9.728	2700	2702	2704	rBV3	1145	604	0.04%	0.005%
72	9.940	2765	2768	2770	rBV4	1553	913	0.06%	0.007%
73	10.162	2825	2837	2854	rBV	574593	951483	60.32%	7.726%
74	10.403	2909	2912	2917	rBV6	2467	2460	0.16%	0.020%
75	10.464	2928	2931	2932	rBV3	465	198	0.01%	0.002%
76	11.107	3127	3131	3133	rBV4	1889	1484	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
 Data File : VV031805.D
 Acq On : 15 Aug 2023 12:53
 Operator : SY/MD
 Sample : 03967-10ME
 Misc : 5.50g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A48L8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M

Title : VOC Analysis

77	11.194	3147	3158	3181	rBV	760646	1189867	75.44%	9.662%
78	11.445	3234	3236	3237	rBV2	1163	429	0.03%	0.003%
79	11.567	3263	3274	3296	rBV	749512	1182200	74.95%	9.600%
80	11.792	3340	3344	3348	rVB5	1677	1431	0.09%	0.012%
81	11.818	3348	3352	3354	rBV5	1893	1538	0.10%	0.012%
82	11.892	3372	3375	3376	rBV3	2034	1180	0.07%	0.010%
83	11.927	3384	3386	3387	rBV2	1166	498	0.03%	0.004%
84	12.246	3481	3485	3490	rBV7	1414	1686	0.11%	0.014%
85	12.754	3638	3643	3645	rBV6	2035	1854	0.12%	0.015%
86	13.114	3748	3755	3759	rBV9	2003	2668	0.17%	0.022%
87	13.779	3960	3962	3968	rBV6	1645	1543	0.10%	0.013%
88	13.811	3969	3972	3978	rBV7	2325	2350	0.15%	0.019%
89	13.889	3990	3996	3998	rBV7	2452	2296	0.15%	0.019%
90	14.368	4137	4145	4155	rBV3	26144	40879	2.59%	0.332%
91	14.618	4221	4223	4226	rBV3	2576	1742	0.11%	0.014%




Sum of corrected areas: 12314675

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
Data File : VV031805.D
Acq On : 15 Aug 2023 12:53
Operator : SY/MD
Sample : 03967-10ME
Misc : 5.50g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A48L8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

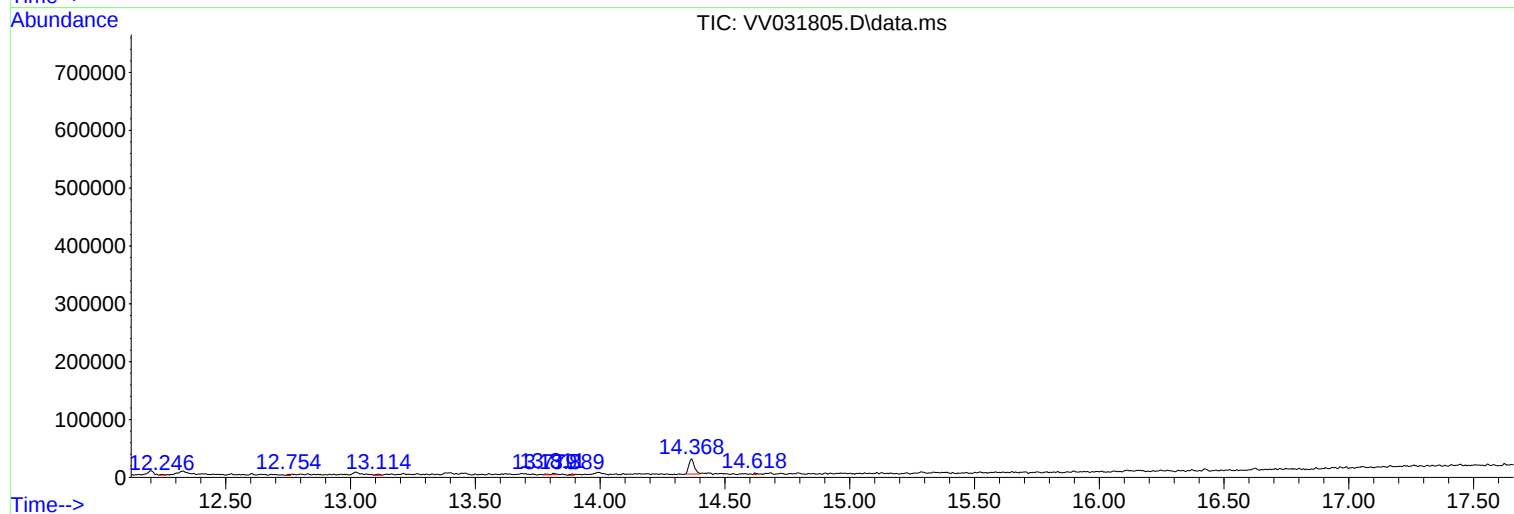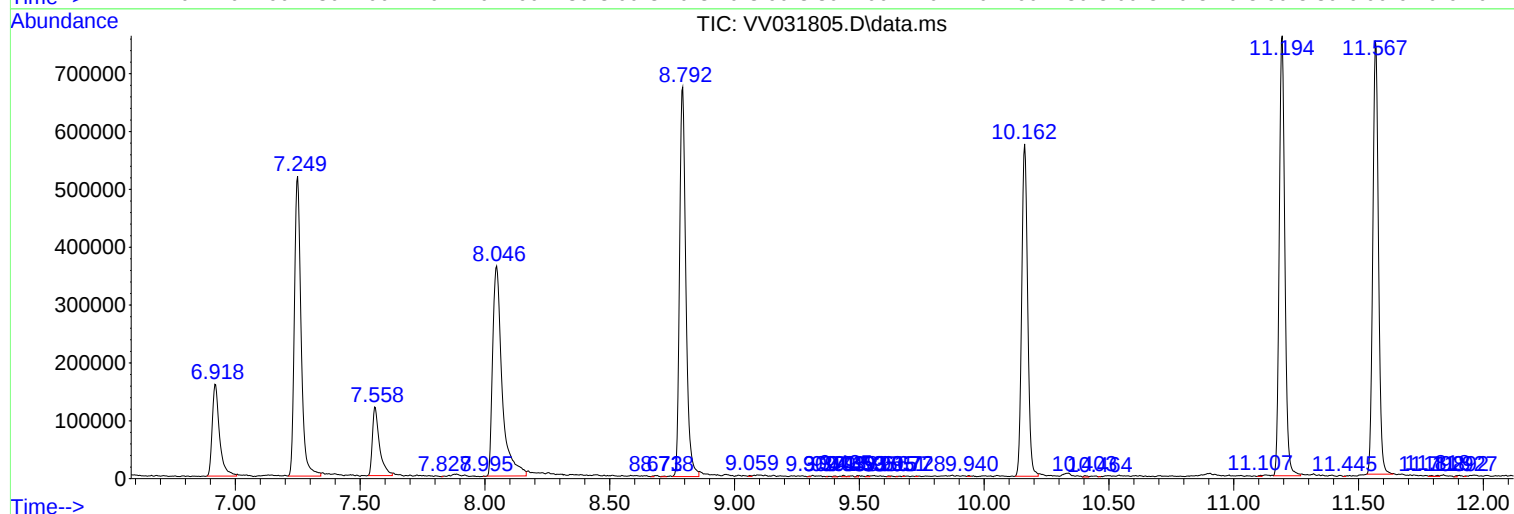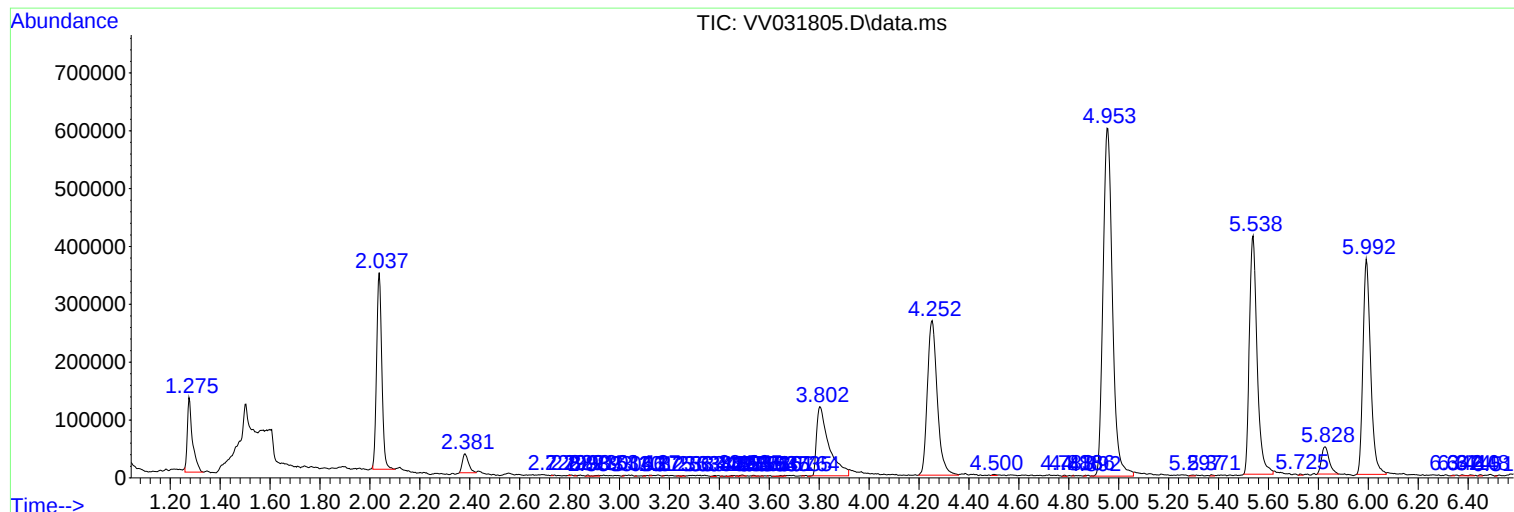

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
Data File : VV031805.D
Acq On : 15 Aug 2023 12:53
Operator : SY/MD
Sample : 03967-10ME
Misc : 5.50g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A48L8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
Data File : VV031805.D
Acq On : 15 Aug 2023 12:53
Operator : SY/MD
Sample : 03967-10ME
Misc : 5.50g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A48L8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc