

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
 Data File : VV031807.D
 Acq On : 15 Aug 2023 13:40
 Operator : SY/MD
 Sample : 03967-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A48A0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

Signal : TIC: VV031807.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	93	rVB	142149	158552	11.63%	1.496%
2	1.532	146	153	165	rVB	156964	191952	14.07%	1.811%
3	2.060	307	317	326	rBV	265768	386871	28.37%	3.650%
4	2.114	327	334	357	rVB	139103	226643	16.62%	2.138%
5	2.436	430	434	435	rBV4	1622	1151	0.08%	0.011%
6	2.462	438	442	446	rVB6	2026	2020	0.15%	0.019%
7	2.966	593	599	600	rBV6	1114	1126	0.08%	0.011%
8	3.002	607	610	615	rVB7	1782	1256	0.09%	0.012%
9	3.034	615	620	623	rBV6	1817	1493	0.11%	0.014%
10	3.060	623	628	631	rVV5	1067	974	0.07%	0.009%
11	3.076	631	633	638	rVB6	1941	1309	0.10%	0.012%
12	3.108	638	643	647	rBV8	1607	1314	0.10%	0.012%
13	3.208	671	674	678	rBV4	1552	1319	0.10%	0.012%
14	3.384	727	729	733	rVV4	1893	1418	0.10%	0.013%
15	3.568	780	786	788	rBV5	1142	1074	0.08%	0.010%
16	3.609	797	799	803	rVB4	1402	909	0.07%	0.009%
17	3.728	832	836	840	rBV4	1425	1134	0.08%	0.011%
18	3.793	846	856	884	rBV	145384	414181	30.37%	3.907%
19	4.256	984	1000	1022	rBV2	246351	641007	47.00%	6.047%
20	4.548	1088	1091	1095	rVB6	1866	1759	0.13%	0.017%
21	4.574	1095	1099	1100	rBV3	2021	1567	0.11%	0.015%
22	4.600	1104	1107	1113	rBV7	2087	1950	0.14%	0.018%
23	4.645	1117	1121	1122	rBV2	1437	929	0.07%	0.009%
24	4.825	1175	1177	1180	rBV2	1361	877	0.06%	0.008%
25	4.847	1180	1184	1187	rBV3	1752	1661	0.12%	0.016%
26	4.963	1202	1220	1250	rBV3	496293	1363831	100.00%	12.866%
27	5.233	1299	1304	1307	rVB6	1494	1193	0.09%	0.011%
28	5.323	1326	1332	1333	rBV4	1657	1328	0.10%	0.013%
29	5.362	1339	1344	1345	rBV4	1373	1062	0.08%	0.010%
30	5.449	1367	1371	1374	rBV6	1418	1412	0.10%	0.013%
31	5.542	1387	1400	1425	rBV	312981	679215	49.80%	6.408%
32	5.773	1470	1472	1477	rVB5	1609	996	0.07%	0.009%
33	5.828	1477	1489	1507	rBV2	68205	146888	10.77%	1.386%
34	5.995	1528	1541	1560	rBV	337360	691792	50.72%	6.526%
35	6.362	1651	1655	1657	rVB4	2354	1742	0.13%	0.016%
36	6.384	1657	1662	1666	rBV6	1899	2062	0.15%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
 Data File : VV031807.D
 Acq On : 15 Aug 2023 13:40
 Operator : SY/MD
 Sample : 03967-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A48A0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

37	6.474	1686	1690	1693	rVB5	1567	1216	0.09%	0.011%
38	6.558	1710	1716	1717	rBV5	1906	1713	0.13%	0.016%
39	6.918	1816	1828	1846	rBV	130666	259790	19.05%	2.451%
40	7.101	1882	1885	1887	rBV3	1561	1135	0.08%	0.011%
41	7.249	1920	1931	1954	rBV	416430	771713	56.58%	7.280%
42	7.561	2018	2028	2054	rBV2	102323	195534	14.34%	1.845%
43	7.789	2096	2099	2101	rVV4	2206	1056	0.08%	0.010%
44	7.947	2145	2148	2151	rBV6	1271	975	0.07%	0.009%
45	8.030	2164	2174	2207	rBV2	406012	865966	63.50%	8.170%
46	8.535	2329	2331	2334	rBV4	1588	1137	0.08%	0.011%
47	8.712	2384	2386	2389	rVB4	2013	1153	0.08%	0.011%
48	8.789	2399	2410	2435	rBV	545390	915438	67.12%	8.636%
49	8.953	2459	2461	2464	rBV3	1306	941	0.07%	0.009%
50	9.037	2484	2487	2491	rVB6	1550	1339	0.10%	0.013%
51	9.079	2496	2500	2501	rBV4	1730	1370	0.10%	0.013%
52	9.127	2511	2515	2519	rBV5	2041	1969	0.14%	0.019%
53	9.191	2532	2535	2539	rBV5	1510	1032	0.08%	0.010%
54	9.233	2543	2548	2551	rBV7	1192	1091	0.08%	0.010%
55	9.297	2565	2568	2572	rBV4	1191	1115	0.08%	0.011%
56	9.429	2606	2609	2611	rVV3	1839	1152	0.08%	0.011%
57	9.484	2623	2626	2628	rBV4	1226	915	0.07%	0.009%
58	9.516	2634	2636	2642	rVB7	1624	1701	0.12%	0.016%
59	9.760	2706	2712	2714	rBV6	3828	3937	0.29%	0.037%
60	9.805	2724	2726	2730	rVB4	1861	1088	0.08%	0.010%
61	9.837	2730	2736	2740	rBV7	1452	1698	0.12%	0.016%
62	9.963	2769	2775	2779	rBV6	2379	2740	0.20%	0.026%
63	10.066	2803	2807	2810	rBV6	1619	1319	0.10%	0.012%
64	10.114	2816	2822	2823	rBV5	1364	1197	0.09%	0.011%
65	10.159	2824	2836	2860	rVB	468650	763226	55.96%	7.200%
66	10.323	2883	2887	2888	rBV4	3985	2763	0.20%	0.026%
67	10.436	2920	2922	2926	rVB4	1669	944	0.07%	0.009%
68	10.468	2929	2932	2934	rBV4	1446	937	0.07%	0.009%
69	10.519	2945	2948	2952	rVB6	1800	958	0.07%	0.009%
70	10.567	2960	2963	2969	rBV6	1399	1342	0.10%	0.013%
71	10.616	2977	2978	2983	rVB5	1290	881	0.06%	0.008%
72	10.780	3026	3029	3031	rBV3	1710	1076	0.08%	0.010%
73	11.075	3117	3121	3123	rBV5	1232	1011	0.07%	0.010%
74	11.104	3123	3130	3131	rBV6	3701	3424	0.25%	0.032%
75	11.191	3146	3157	3178	rBV	537566	831721	60.98%	7.847%
76	11.500	3243	3253	3262	rBV4	16643	34983	2.57%	0.330%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
 Data File : VV031807.D
 Acq On : 15 Aug 2023 13:40
 Operator : SY/MD
 Sample : 03967-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A48A0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

77	11.567	3263	3274	3296	rVB	574093	921184	67.54%	8.691%
78	11.950	3387	3393	3402	rVB6	8770	12131	0.89%	0.114%
79	12.079	3430	3433	3437	rBV6	1347	922	0.07%	0.009%
80	12.194	3463	3469	3471	rBV7	5649	5090	0.37%	0.048%
81	12.255	3481	3488	3494	rBV9	10224	14867	1.09%	0.140%
82	12.570	3583	3586	3589	rBV5	1546	1011	0.07%	0.010%
83	12.754	3641	3643	3647	rBV5	1360	1093	0.08%	0.010%
84	12.821	3660	3664	3666	rBV4	1724	1513	0.11%	0.014%
85	12.898	3683	3688	3690	rBV4	1305	1215	0.09%	0.011%
86	12.953	3701	3705	3707	rBV4	1731	1423	0.10%	0.013%
87	13.053	3733	3736	3739	rBV3	1248	1003	0.07%	0.009%
88	13.082	3740	3745	3748	rBV6	2513	2683	0.20%	0.025%
89	13.384	3836	3839	3842	rBV4	1724	1235	0.09%	0.012%
90	13.506	3875	3877	3881	rVB4	1801	1199	0.09%	0.011%
91	13.580	3898	3900	3903	rBV3	1457	1183	0.09%	0.011%
92	13.937	4005	4011	4013	rVB5	1567	1474	0.11%	0.014%
93	13.988	4025	4027	4033	rBV7	1767	1754	0.13%	0.017%
94	14.445	4165	4169	4172	rBV4	2050	1691	0.12%	0.016%
95	14.545	4197	4200	4201	rBV2	2135	1081	0.08%	0.010%
96	14.712	4249	4252	4256	rBV6	2053	1570	0.12%	0.015%
97	14.950	4324	4326	4328	rBV3	1746	892	0.07%	0.008%
98	14.972	4331	4333	4336	rBV3	1710	948	0.07%	0.009%
99	15.030	4349	4351	4354	rBV4	1520	924	0.07%	0.009%
100	15.107	4373	4375	4378	rVB4	2030	1120	0.08%	0.011%




Sum of corrected areas: 10599869

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
Data File : VV031807.D
Acq On : 15 Aug 2023 13:40
Operator : SY/MD
Sample : 03967-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A48A0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

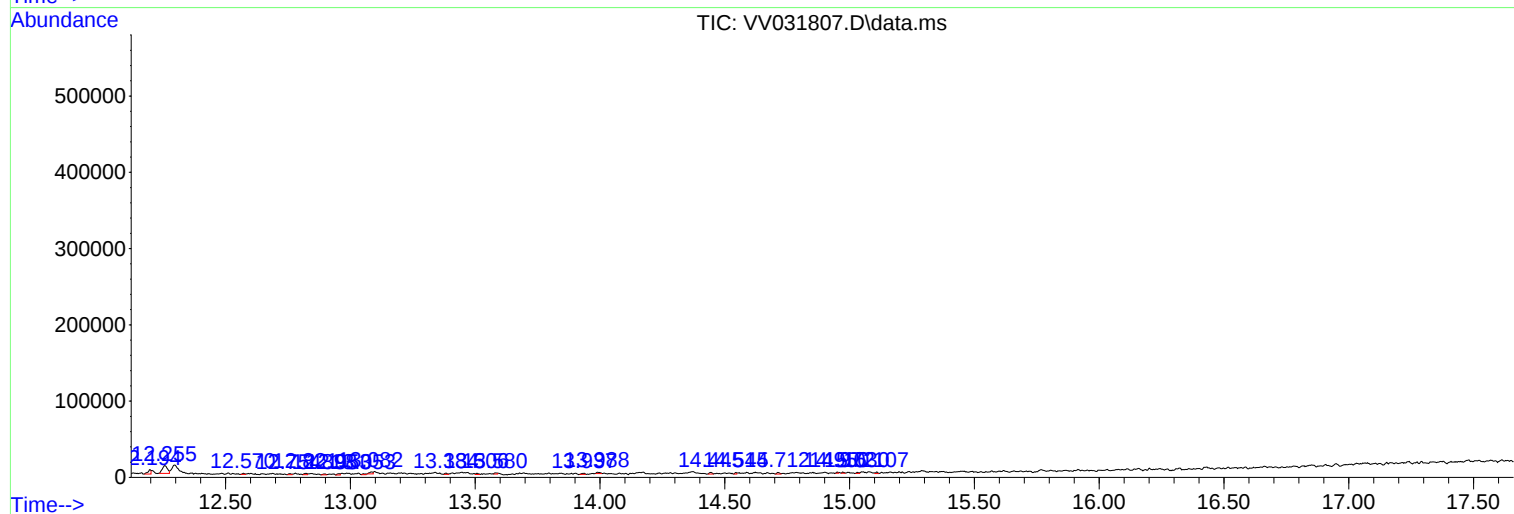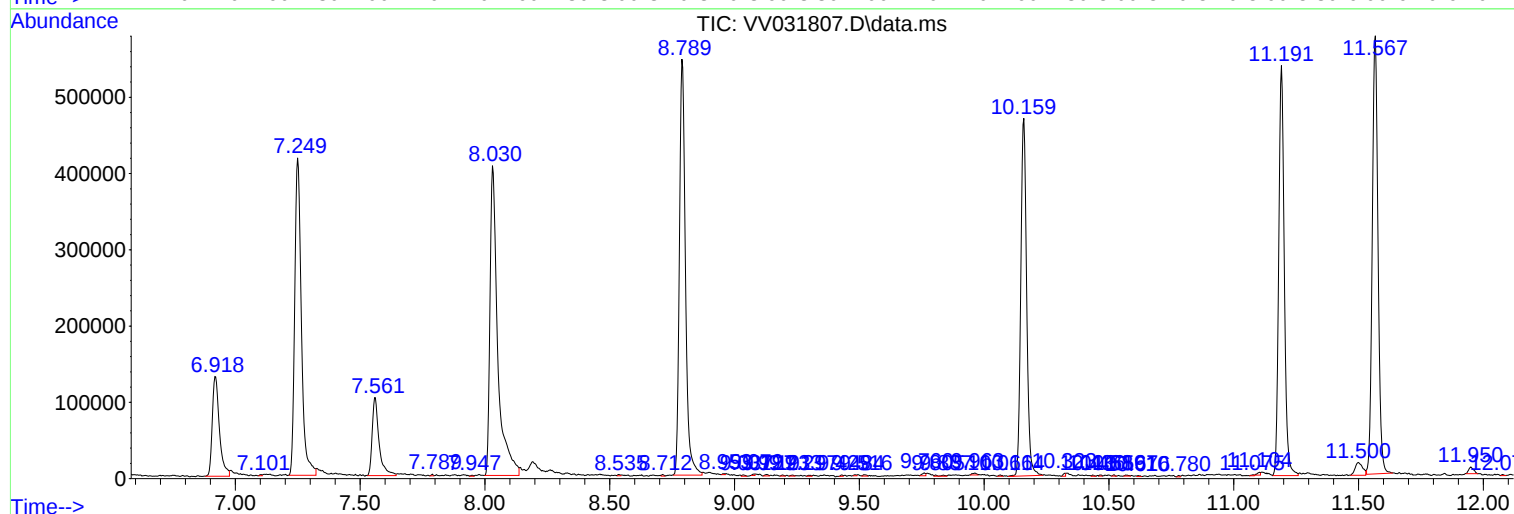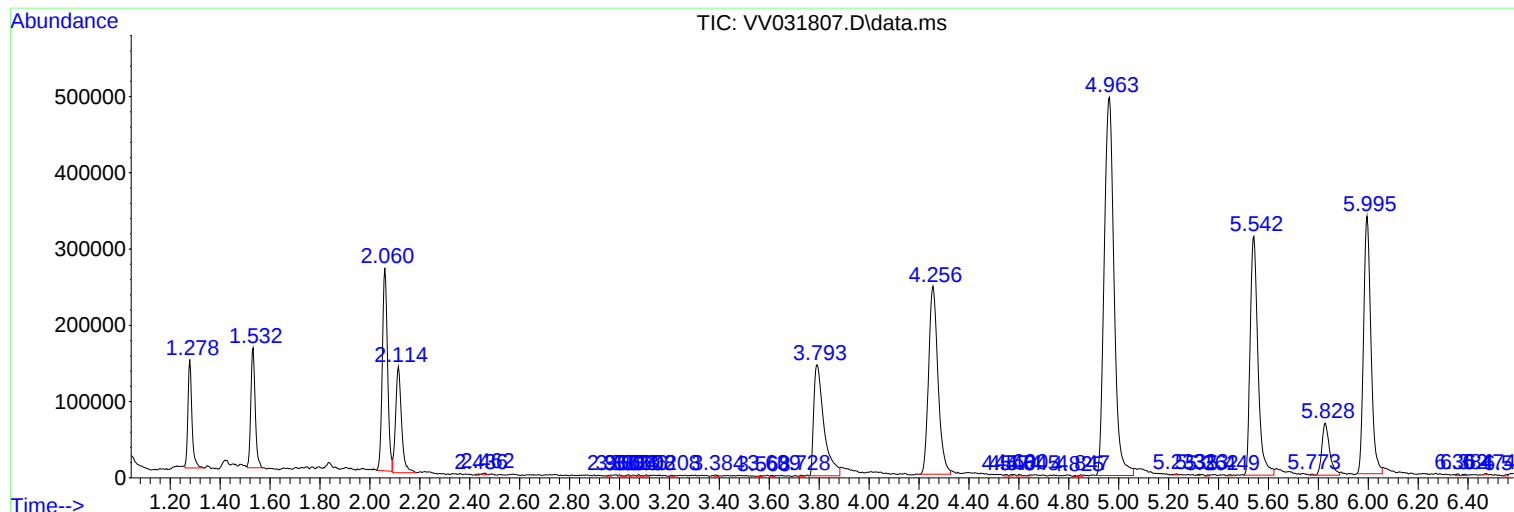

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
Data File : VV031807.D
Acq On : 15 Aug 2023 13:40
Operator : SY/MD
Sample : 03967-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A48A0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
Data File : VV031807.D
Acq On : 15 Aug 2023 13:40
Operator : SY/MD
Sample : 03967-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A48A0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------