

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
 Data File : VV031812.D
 Acq On : 15 Aug 2023 16:21
 Operator : SY/MD
 Sample : 03965-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

Signal : TIC: VV031812.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	91	rVB	153997	166066	11.42%	1.434%
2	1.532	147	153	168	rVB	169769	205357	14.12%	1.773%
3	2.060	309	317	335	rVB	294592	422160	29.03%	3.645%
4	2.320	396	398	402	rBV3	1445	1118	0.08%	0.010%
5	2.529	461	463	465	rBV2	1007	446	0.03%	0.004%
6	2.587	479	481	483	rVB3	1024	304	0.02%	0.003%
7	2.635	494	496	499	rVB2	1133	620	0.04%	0.005%
8	2.693	511	514	515	rBV3	1044	725	0.05%	0.006%
9	2.745	529	530	531	rBV	581	200	0.01%	0.002%
10	2.796	543	546	550	rBV5	761	510	0.04%	0.004%
11	2.867	567	568	572	rVB4	774	264	0.02%	0.002%
12	2.950	587	594	595	rBV3	1189	1195	0.08%	0.010%
13	3.021	614	616	619	rVB	661	275	0.02%	0.002%
14	3.040	619	622	623	rBV2	837	503	0.03%	0.004%
15	3.098	637	640	645	rBV5	1109	861	0.06%	0.007%
16	3.118	645	646	650	rVB3	831	450	0.03%	0.004%
17	3.137	650	652	653	rBV2	581	213	0.01%	0.002%
18	3.146	653	655	657	rBV2	727	317	0.02%	0.003%
19	3.233	679	682	685	rVB3	998	507	0.03%	0.004%
20	3.253	685	688	692	rBV5	1132	786	0.05%	0.007%
21	3.323	707	710	712	rBV3	792	445	0.03%	0.004%
22	3.336	712	714	718	rBV3	411	317	0.02%	0.003%
23	3.378	725	727	732	rVB5	1286	886	0.06%	0.008%
24	3.404	733	735	737	rBV3	499	224	0.02%	0.002%
25	3.478	756	758	761	rVV4	761	300	0.02%	0.003%
26	3.497	761	764	765	rVB2	615	338	0.02%	0.003%
27	3.529	771	774	775	rBV2	277	133	0.01%	0.001%
28	3.542	775	778	779	rVV2	1041	556	0.04%	0.005%
29	3.571	783	787	794	rBV8	1360	1631	0.11%	0.014%
30	3.600	794	796	799	rVB3	807	363	0.02%	0.003%
31	3.619	799	802	805	rBV4	854	701	0.05%	0.006%
32	3.654	810	813	814	rBV3	733	368	0.03%	0.003%
33	3.693	823	825	827	rVB2	536	185	0.01%	0.002%
34	3.716	830	832	834	rVB2	863	330	0.02%	0.003%
35	3.732	834	837	839	rBV3	770	482	0.03%	0.004%
36	3.793	847	856	893	rBV	140499	416698	28.65%	3.598%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW081523\
 Data File : VW031812.D
 Acq On : 15 Aug 2023 16:21
 Operator : SY/MD
 Sample : 03965-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

37	4.256	985	1000	1028	rBV2	273569	709032	48.75%	6.123%
38	4.706	1138	1140	1142	rBV3	910	529	0.04%	0.005%
39	4.844	1181	1183	1187	rBV4	1375	1291	0.09%	0.011%
40	4.963	1203	1220	1244	rBV3	535373	1454420	100.00%	12.559%
41	5.400	1353	1356	1358	rBV3	1955	1210	0.08%	0.010%
42	5.458	1371	1374	1375	rBV2	1123	665	0.05%	0.006%
43	5.542	1388	1400	1423	rBV	399186	845788	58.15%	7.304%
44	5.831	1480	1490	1509	rBV2	41523	87276	6.00%	0.754%
45	5.995	1529	1541	1560	rBV	365700	749924	51.56%	6.476%
46	6.410	1668	1670	1675	rBV4	908	725	0.05%	0.006%
47	6.442	1675	1680	1684	rVV8	1128	1292	0.09%	0.011%
48	6.468	1686	1688	1690	rVB3	870	316	0.02%	0.003%
49	6.497	1695	1697	1703	rVB6	1310	1071	0.07%	0.009%
50	6.770	1779	1782	1784	rVB2	953	491	0.03%	0.004%
51	6.783	1784	1786	1788	rVB3	719	289	0.02%	0.002%
52	6.796	1788	1790	1792	rBV2	1034	461	0.03%	0.004%
53	6.918	1818	1828	1860	rBV	144675	284253	19.54%	2.455%
54	7.249	1920	1931	1958	rBV	474008	872016	59.96%	7.530%
55	7.558	2018	2027	2053	rBV2	110035	209697	14.42%	1.811%
56	7.969	2151	2155	2156	rBV	1721	1073	0.07%	0.009%
57	8.031	2164	2174	2217	rBV2	434053	914761	62.90%	7.899%
58	8.522	2323	2327	2328	rBV4	2127	1725	0.12%	0.015%
59	8.558	2336	2338	2341	rBV3	1179	497	0.03%	0.004%
60	8.606	2351	2353	2354	rBV2	974	532	0.04%	0.005%
61	8.699	2378	2382	2383	rBV2	1203	738	0.05%	0.006%
62	8.735	2391	2393	2396	rBV3	919	343	0.02%	0.003%
63	8.789	2399	2410	2434	rBV	685754	1156474	79.51%	9.986%
64	9.252	2551	2554	2555	rBV3	974	494	0.03%	0.004%
65	9.670	2681	2684	2686	rBV4	1195	673	0.05%	0.006%
66	9.748	2706	2708	2710	rBV4	1096	528	0.04%	0.005%
67	9.799	2722	2724	2726	rBV	1532	818	0.06%	0.007%
68	9.966	2773	2776	2779	rBV4	1729	1187	0.08%	0.010%
69	10.021	2790	2793	2799	rVB7	1630	1448	0.10%	0.013%
70	10.053	2799	2803	2804	rBV3	1269	915	0.06%	0.008%
71	10.159	2824	2836	2858	rBV	579506	924724	63.58%	7.985%
72	10.333	2885	2890	2896	rBV9	2135	2952	0.20%	0.025%
73	10.397	2907	2910	2913	rBV4	989	736	0.05%	0.006%
74	10.555	2956	2959	2962	rVB3	1974	1398	0.10%	0.012%
75	10.641	2982	2986	2988	rBV4	1102	839	0.06%	0.007%
76	10.686	2998	3000	3002	rBV2	898	454	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
 Data File : VV031812.D
 Acq On : 15 Aug 2023 16:21
 Operator : SY/MD
 Sample : 03965-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M

Title : VOC Analysis

77	10.725	3009	3012	3014	rBV3	1446	912	0.06%	0.008%
78	10.792	3028	3033	3035	rBV5	1666	1410	0.10%	0.012%
79	10.899	3064	3066	3069	rBV4	670	325	0.02%	0.003%
80	10.931	3072	3076	3079	rBV5	1582	1325	0.09%	0.011%
81	11.008	3098	3100	3103	rBV4	734	360	0.02%	0.003%
82	11.069	3117	3119	3121	rBV3	579	157	0.01%	0.001%
83	11.143	3140	3142	3145	rVB3	1303	659	0.05%	0.006%
84	11.191	3145	3157	3176	rBV	672603	1062780	73.07%	9.177%
85	11.567	3262	3274	3293	rBV	661804	1045446	71.88%	9.028%
86	11.828	3352	3355	3356	rBV3	1417	697	0.05%	0.006%
87	11.873	3367	3369	3372	rBV3	810	378	0.03%	0.003%
88	11.899	3373	3377	3379	rBV4	1654	1148	0.08%	0.010%
89	11.960	3392	3396	3399	rBV4	1757	1916	0.13%	0.017%
90	12.043	3420	3422	3424	rBV3	935	429	0.03%	0.004%
91	12.513	3565	3568	3575	rBV9	1420	1722	0.12%	0.015%




Sum of corrected areas: 11580553

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
Data File : VV031812.D
Acq On : 15 Aug 2023 16:21
Operator : SY/MD
Sample : 03965-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

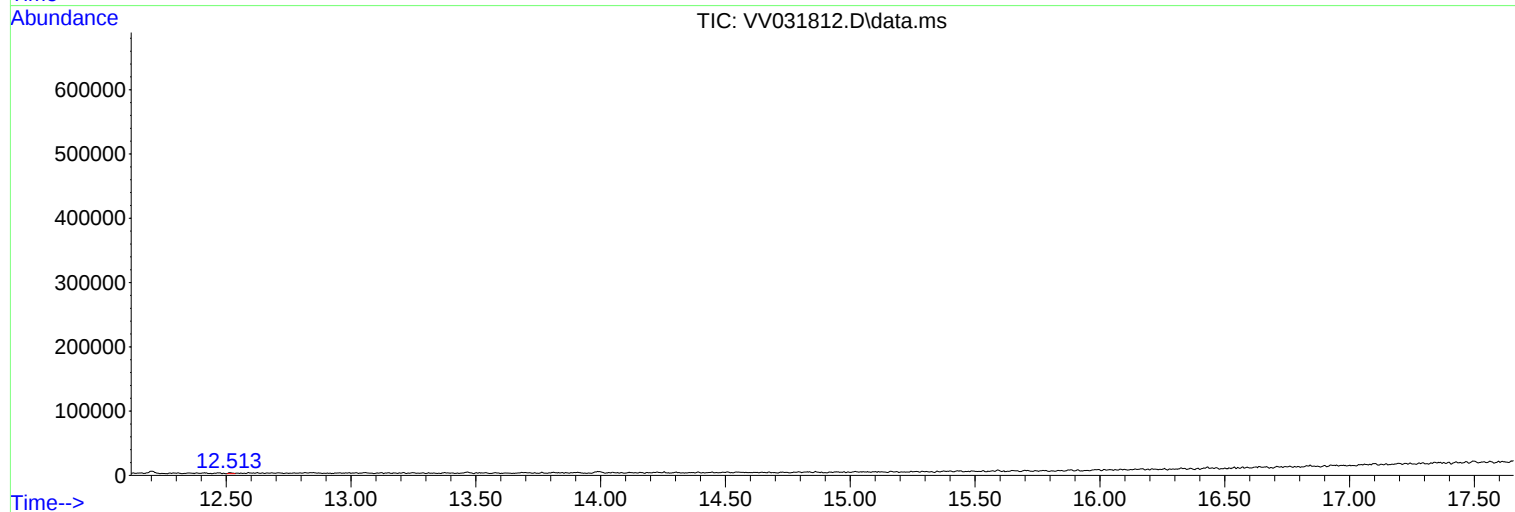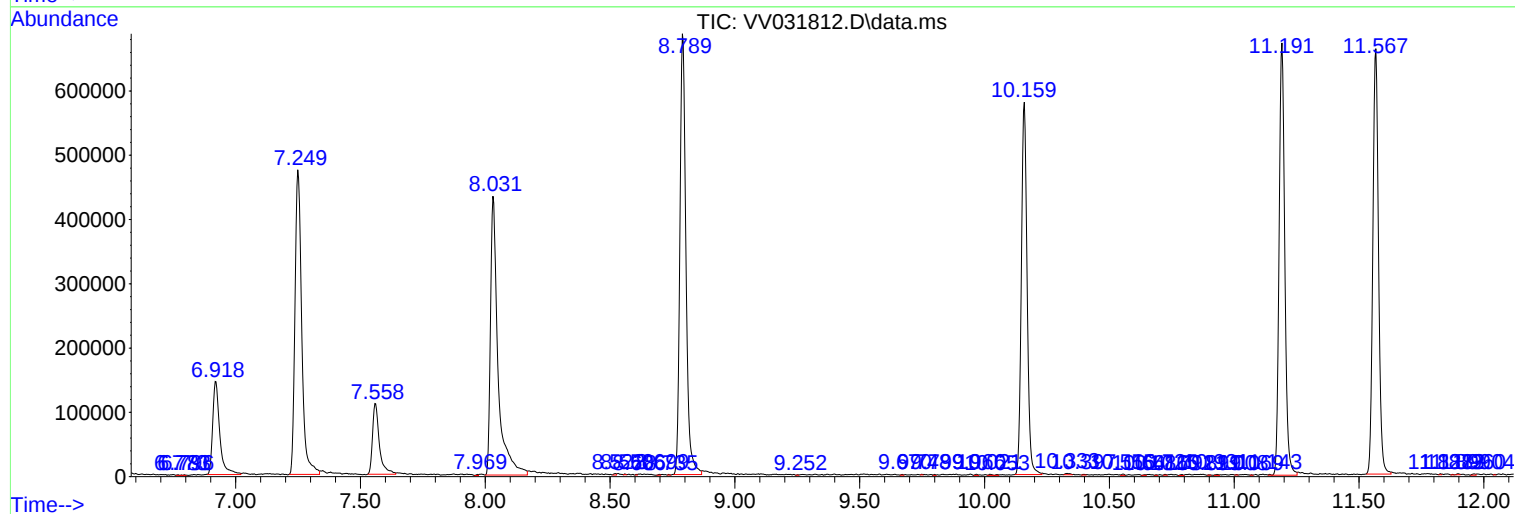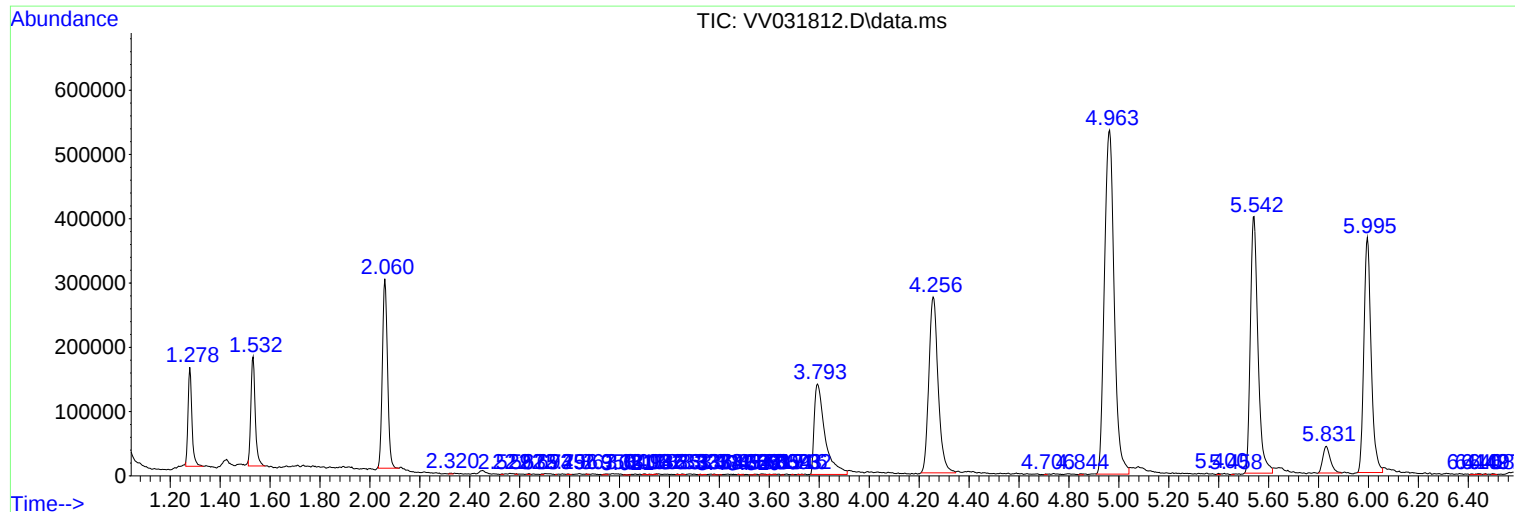

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
Data File : VV031812.D
Acq On : 15 Aug 2023 16:21
Operator : SY/MD
Sample : 03965-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
Data File : VV031812.D
Acq On : 15 Aug 2023 16:21
Operator : SY/MD
Sample : 03965-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------