


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081523\
Data File : VV031797.D
Acq On : 15 Aug 2023 08:55
Operator : SY/MD
Sample : BFB202
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB202

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Title : VOC Analysis
Last Update : Wed Aug 16 02:07:29 2023

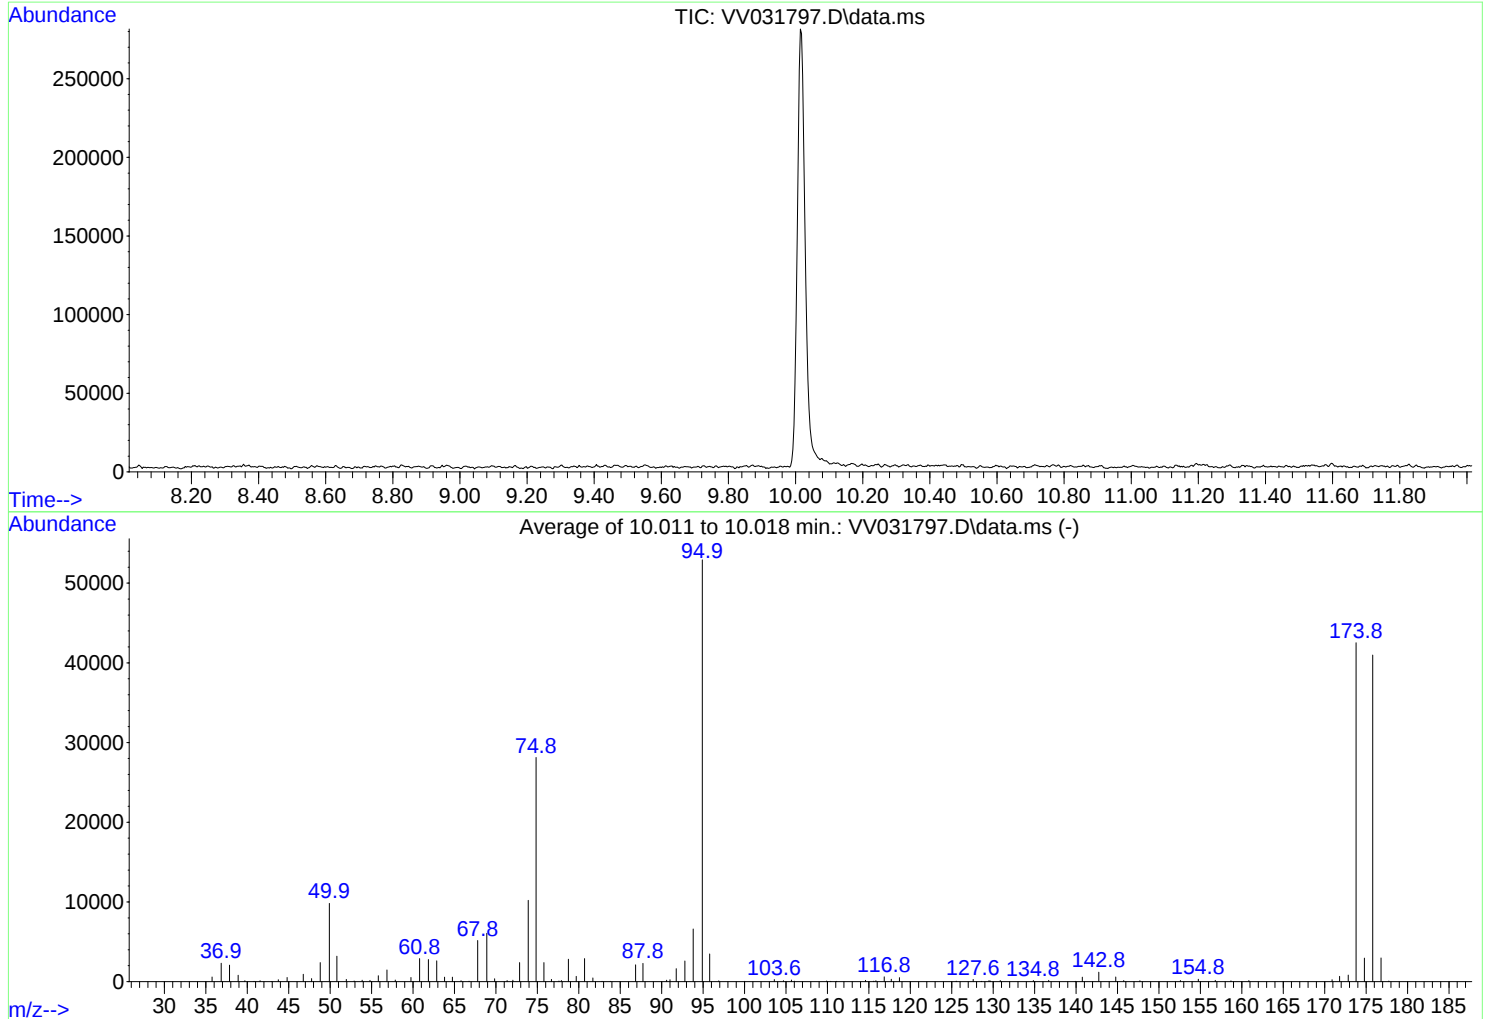

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2780

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.6	9825	PASS
75	95	30	80	53.1	28128	PASS
95	95	100	100	100.0	52923	PASS
96	95	5	9	6.6	3468	PASS
173	174	0.00	2	2.0	832	PASS
174	95	50	120	80.3	42517	PASS
175	174	5	9	7.0	2958	PASS
176	174	95	105	96.4	40971	PASS
177	176	5	10	7.3	2971	PASS

m/z	Abundance
35.80	567.0
36.90	2371.0
37.90	2108.0
38.90	938.0
39.70	567.0
41.50	121.0
42.00	135.0
42.90	217.0
43.80	941.0
44.80	525.0
45.80	140.0
46.80	957.0
47.70	378.0
48.80	2521.0
49.90	10242.0
50.80	3373.0
52.00	289.0
52.90	115.0
53.90	189.0
54.80	161.0
55.80	771.0
56.80	1521.0
57.90	207.0
59.80	551.0
60.80	3010.0
61.90	2965.0
62.80	2730.0
63.80	683.0
64.80	568.0
65.80	121.0
66.70	188.0
67.80	5430.0
68.90	6299.0
69.80	365.0
71.40	193.0
72.10	264.0
72.80	2615.0
73.90	10654.0
74.90	28960.0
75.80	2465.0
76.70	388.0
77.90	223.0
78.80	2893.0
79.70	694.0
80.70	3004.0
81.70	476.0
86.80	2203.0
87.70	2364.0
90.60	244.0
91.00	237.0
91.70	1649.0
92.80	2648.0
93.80	6898.0
94.90	54752.0
95.80	3581.0
96.90	129.0
103.60	265.0
104.70	108.0
105.70	204.0
109.90	111.0
114.60	175.0
115.80	179.0
116.90	667.0
117.70	332.0
118.70	525.0
125.50	103.0
127.60	272.0
129.50	233.0
130.90	149.0
134.80	129.0
136.70	159.0
140.80	556.0
142.80	1257.0
144.80	624.0
145.80	145.0
147.70	116.0
152.60	155.0
154.70	318.0
156.80	145.0
158.70	143.0
160.80	167.0
170.90	233.0
171.80	725.0
172.80	855.0
173.80	44080.0
174.80	3058.0
175.80	42456.0
176.80	3061.0
177.70	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

m/z	Abundance
35.80	648.0
36.80	2290.0
37.90	2064.0
38.90	1019.0
39.70	515.0
40.80	114.0
41.60	100.0
42.00	127.0
42.90	233.0
43.80	845.0
44.80	543.0
46.80	1019.0
47.80	443.0
48.80	2356.0
49.90	9576.0
50.80	3395.0
51.90	239.0
52.90	159.0
53.80	156.0
54.70	203.0
55.80	693.0
56.90	1374.0
57.80	237.0
59.70	541.0
60.80	3086.0
61.90	2878.0
62.80	2719.0
63.80	699.0
64.80	684.0
65.80	111.0
66.70	176.0
67.80	5125.0
68.90	6035.0
69.90	364.0
71.30	203.0
72.00	292.0
72.80	2467.0
73.90	9974.0
74.80	27816.0
75.80	2376.0
76.80	314.0
77.90	217.0
78.80	2959.0
79.70	679.0
80.70	3184.0
81.70	472.0
82.80	104.0
86.90	2153.0
87.80	2368.0
90.60	320.0
91.10	205.0
91.80	1774.0
92.80	2533.0
93.80	6865.0
94.90	54288.0
95.80	3466.0
96.90	151.0
100.00	114.0
103.60	218.0
104.80	142.0
105.60	202.0
110.40	104.0
114.60	131.0
115.90	185.0
116.80	538.0
117.70	297.0
118.70	593.0
127.60	271.0
129.70	236.0
130.80	134.0
134.90	160.0
136.70	138.0
139.90	104.0
140.80	595.0
142.70	1134.0
144.80	634.0
145.70	149.0
147.70	120.0
152.60	139.0
154.70	402.0
156.90	197.0
158.70	138.0
160.80	120.0
170.80	245.0
171.80	781.0
172.90	934.0
173.80	44440.0
174.80	3162.0
175.80	42760.0
176.80	3086.0
177.80	142.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

m/z	Abundance
36.40	170.0
37.10	123.0
37.50	155.0
38.20	106.0
38.90	127.0
39.80	427.0
41.90	209.0
43.00	171.0
43.70	665.0
45.70	155.0
47.10	107.0
60.50	157.0
61.80	109.0
63.70	101.0
66.80	121.0
73.00	162.0
76.70	110.0
93.40	112.0
175.40	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

m/z	Abundance
35.70	510.0
36.90	2247.0
37.80	2037.0
38.90	846.0
39.70	586.0
41.60	126.0
41.90	106.0
42.90	155.0
43.80	949.0
44.80	478.0
45.80	192.0
46.70	798.0
47.70	346.0
48.80	2321.0
49.90	9657.0
50.80	2836.0
52.00	298.0
53.90	213.0
54.90	113.0
55.80	744.0
56.80	1498.0
57.90	172.0
59.80	505.0
60.80	2596.0
61.90	2821.0
62.90	2405.0
63.90	592.0
64.70	444.0
65.80	137.0
66.80	193.0
67.80	4897.0
68.90	5837.0
69.80	384.0
72.90	2562.0
73.90	9999.0
74.90	27608.0
75.80	2326.0
76.70	466.0
77.60	250.0
78.70	2608.0
79.70	647.0
80.70	2492.0
81.70	448.0
83.80	108.0
86.80	1999.0
87.70	2161.0
90.90	259.0
91.70	1435.0
92.80	2568.0
93.80	6041.0
94.90	49728.0
95.80	3356.0
103.60	316.0
104.60	117.0
105.70	185.0
106.00	171.0
109.90	108.0
111.10	139.0
114.60	175.0
115.60	192.0
116.90	582.0
117.70	262.0
118.70	369.0
125.60	100.0
127.60	280.0
128.60	116.0
129.50	184.0
130.90	152.0
134.80	117.0
136.70	161.0
140.70	543.0
142.80	1184.0
144.80	522.0
145.80	157.0
147.70	153.0
152.60	106.0
154.80	192.0
156.70	135.0
160.90	160.0
171.00	226.0
171.80	505.0
172.80	707.0
173.80	39032.0
174.80	2655.0
175.80	37696.0
176.80	2765.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202