


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081618\
Data File : VV007033.D
Acq On : 16 Aug 2018 09:03
Operator : SY/MD
Sample : BFB85
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB85

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Aug 17 01:13:44 2018

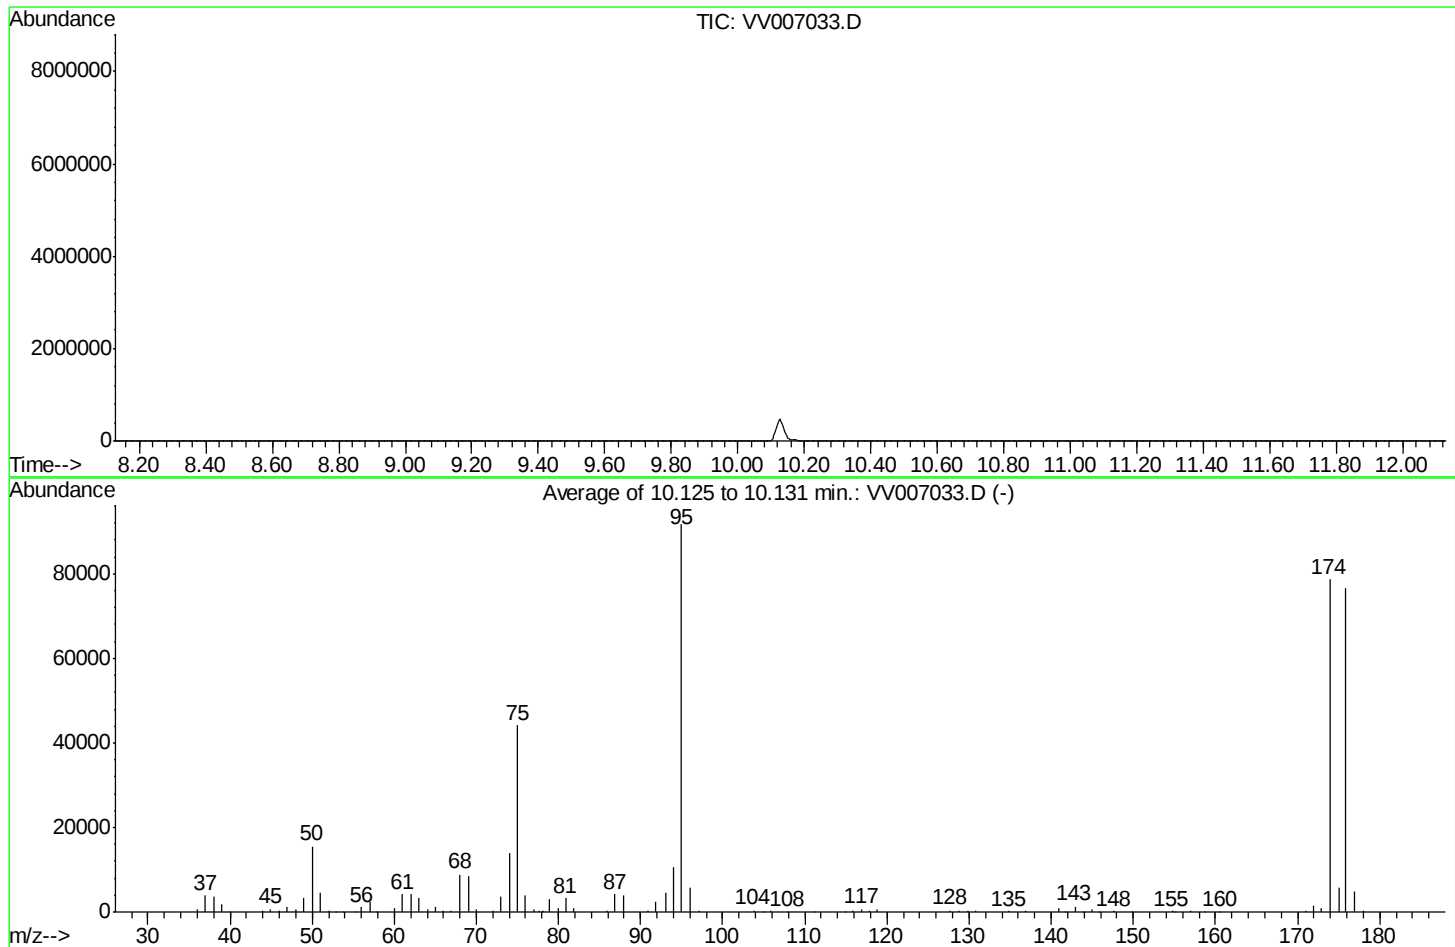

AutoFind: Scans 2872, 2873, 2874; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	15505	PASS
75	95	30	80	48.2	44192	PASS
95	95	100	100	100.0	91701	PASS
96	95	5	9	6.1	5613	PASS
173	174	0.00	2	1.3	1032	PASS
174	95	50	120	85.8	78661	PASS
175	174	5	9	7.5	5902	PASS
176	174	95	101	97.5	76680	PASS
177	176	5	9	6.3	4833	PASS

Scan 2858 (10.080 min): VV007033.D
BFB85

m/z	Abundance
39.90	517.0
43.90	1023.0
206.90	182.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

m/z	Abundance
36.00	585.0
37.00	3875.0
38.00	3446.0
39.10	1908.0
39.90	546.0
43.90	1455.0
45.00	749.0
46.00	253.0
46.90	1393.0
47.90	479.0
49.00	3361.0
50.00	16142.0
51.00	4936.0
52.00	419.0
52.90	189.0
53.80	103.0
55.20	169.0
56.00	1201.0
57.00	2402.0
57.90	158.0
60.00	785.0
61.00	4402.0
62.00	4155.0
63.00	3538.0
64.00	834.0
64.90	1204.0
66.00	195.0
66.90	215.0
68.00	9272.0
69.00	8839.0
70.00	705.0
72.00	440.0
73.00	3728.0
74.00	14383.0
75.00	45800.0
76.00	4188.0
76.90	594.0
78.00	436.0
78.90	3088.0
79.90	815.0
80.90	3356.0
81.90	856.0
85.90	207.0
86.90	4450.0
88.00	4419.0
90.80	313.0
91.90	2417.0
93.00	4603.0
94.00	10888.0
95.00	93776.0
96.00	5950.0
97.20	265.0
103.80	388.0
104.80	132.0
105.80	403.0
107.90	150.0
114.90	104.0
115.90	351.0
116.90	621.0
117.90	382.0
118.80	641.0
127.70	389.0
128.70	203.0
129.80	369.0
130.90	168.0
134.90	197.0
136.90	158.0
140.90	875.0
142.90	1265.0
144.00	104.0
144.90	632.0
145.80	153.0
147.70	244.0
149.90	105.0
154.80	209.0
155.10	190.0
156.90	172.0
171.00	263.0
172.00	1349.0
172.90	926.0
173.90	78744.0
175.00	6194.0
175.90	76680.0
176.90	4991.0
178.00	181.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

m/z	Abundance
36.00	542.0
37.00	4029.0
38.00	3674.0
39.10	1937.0
39.90	553.0
44.00	1502.0
45.00	752.0
46.00	222.0
46.90	1268.0
48.00	524.0
49.00	3471.0
50.00	15892.0
51.00	4645.0
52.00	413.0
52.80	133.0
53.80	137.0
55.20	122.0
56.00	1240.0
57.00	2415.0
57.90	162.0
60.00	792.0
61.00	4326.0
62.00	4227.0
63.00	3511.0
64.00	744.0
64.90	1190.0
66.00	210.0
66.90	188.0
68.00	9143.0
69.00	8624.0
70.00	529.0
72.00	406.0
73.00	3727.0
74.00	14257.0
75.00	45720.0
76.00	4080.0
76.90	593.0
77.70	425.0
78.20	425.0
78.90	3103.0
80.00	815.0
80.90	3357.0
81.90	847.0
86.00	164.0
86.90	4262.0
87.90	4224.0
90.80	323.0
91.90	2573.0
93.00	4699.0
94.00	11117.0
95.00	94168.0
96.00	5751.0
97.20	227.0
103.80	342.0
104.90	134.0
105.80	338.0
107.90	112.0
111.10	121.0
115.90	392.0
117.00	673.0
117.90	324.0
118.80	658.0
127.70	379.0
128.80	207.0
129.80	313.0
130.80	210.0
134.90	206.0
136.90	195.0
140.90	858.0
142.90	1306.0
144.00	117.0
144.90	685.0
145.80	147.0
147.70	199.0
149.80	120.0
154.80	179.0
155.10	168.0
156.90	179.0
158.70	101.0
171.00	280.0
171.90	1485.0
172.90	1068.0
173.90	80920.0
175.00	6079.0
175.90	79064.0
176.90	4989.0
178.00	252.0
206.80	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

m/z	Abundance
36.10	528.0
37.00	3776.0
38.00	3472.0
39.00	1712.0
40.00	485.0
44.00	1498.0
44.90	724.0
46.00	197.0
46.90	1073.0
48.00	508.0
49.00	3188.0
50.00	14482.0
51.00	4074.0
52.00	322.0
53.90	126.0
55.00	116.0
56.00	1168.0
57.00	2148.0
57.90	140.0
60.00	750.0
61.00	3787.0
62.00	3999.0
63.00	3241.0
64.00	623.0
65.00	1044.0
66.00	174.0
66.90	178.0
68.00	8325.0
69.00	7861.0
70.00	422.0
72.00	402.0
73.00	3387.0
74.00	13187.0
75.00	41056.0
76.00	3698.0
77.00	579.0
77.70	435.0
78.10	384.0
78.90	2882.0
80.00	802.0
80.90	3170.0
81.90	733.0
86.00	171.0
86.90	3752.0
87.90	3594.0
90.90	354.0
91.90	2377.0
93.00	4134.0
94.00	10200.0
95.00	87160.0
96.00	5139.0
97.20	136.0
103.80	290.0
104.90	160.0
105.80	261.0
111.10	105.0
115.90	381.0
117.00	639.0
117.80	286.0
118.80	604.0
127.70	274.0
128.80	196.0
129.80	268.0
130.80	186.0
134.90	211.0
136.90	205.0
140.90	732.0
141.70	103.0
142.90	1223.0
143.90	109.0
145.00	691.0
145.80	137.0
147.80	135.0
149.80	132.0
154.70	151.0
156.90	163.0
160.60	107.0
171.00	253.0
171.90	1377.0
172.90	1104.0
173.90	76320.0
175.00	5433.0
175.90	74296.0
176.90	4521.0
178.00	238.0
206.90	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85