

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081619\
 Data File : VV012265.D
 Acq On : 16 Aug 2019 12:43
 Operator : SY/MD
 Sample : K4373-08
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH6

Quant Time: Aug 17 00:05:43 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 16 23:35:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	165117	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	164476	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	64094	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	76940	7.56	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	151.20%#
7) Chloroethane-d5	1.58	69	55353	7.12	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	142.40%#
11) 1,1-Dichloroethene-d2	2.13	63	76225	4.58	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	91.60%
20) 2-Butanone-d5	3.96	46	167722	76.34	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	152.68%#
24) Chloroform-d	4.40	84	145904	7.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	144.80%#
26) 1,2-Dichloroethane-d4	5.08	65	72584	7.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	152.20%#
32) Benzene-d6	5.10	84	290546	6.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	139.60%#
36) 1,2-Dichloropropane-d6	6.12	67	87661	7.15	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	143.00%#
41) Toluene-d8	7.36	98	242670	6.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	127.80%
43) trans-1,3-Dichloropropene-	7.66	79	29782	6.34	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	126.80%
46) 2-Hexanone-d5	8.14	63	86729	57.60	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	115.20%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	53613	6.27	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	125.40%#
64) 1,2-Dichlorobenzene-d4	11.67	152	83161	7.67	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	153.40%#


Target Compounds					Ovalue
13) Acetone	2.22	43	9445	6.898 ug/L	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081619\
Data File : VV012265.D
Acq On : 16 Aug 2019 12:43
Operator : SY/MD
Sample : K4373-08
Misc : 25mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH6

Quant Time: Aug 17 00:05:43 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 16 23:35:37 2019
Response via : Initial Calibration

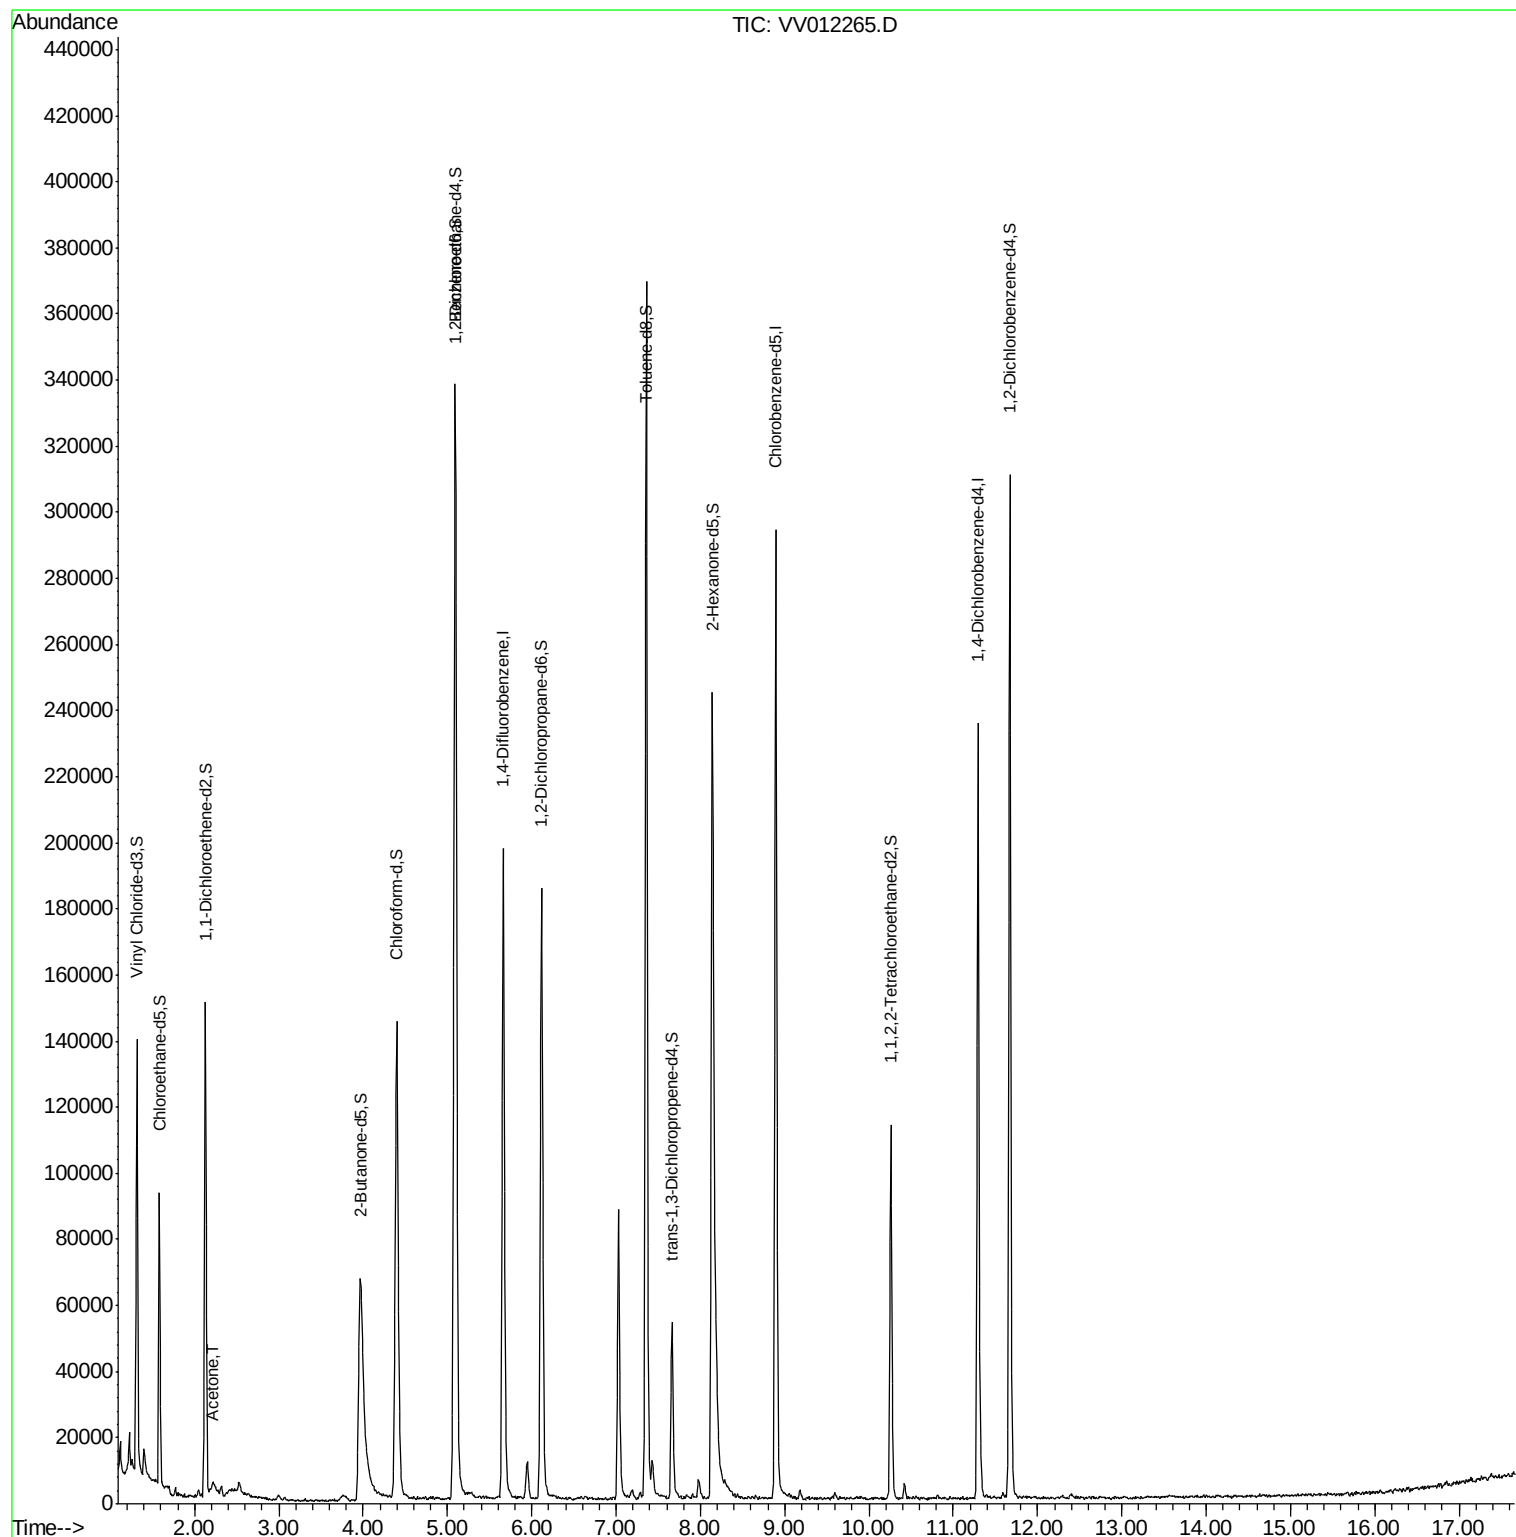

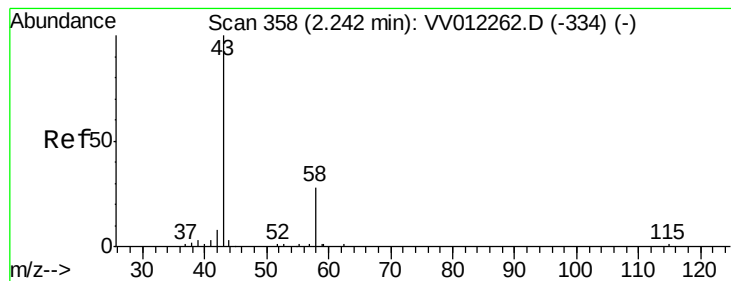

#13
 Acetone
 Concen: 6.898 ug/L
 RT: 2.22 min Scan# 351
 Delta R.T. -0.02 min
 Lab File: VV012265.D
 Acq: 16 Aug 2019 12:43

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH6

Tot Ion: 43 Resp: 9445
 Ion Ratio Lower Upper
 43 100
 58 9.9 0.0 59.4

