

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081619\
 Data File : VV012266.D
 Acq On : 16 Aug 2019 13:11
 Operator : SY/MD
 Sample : K4373-09
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ4

Quant Time: Aug 17 00:09:41 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 16 23:35:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	179807	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	179630	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	70838	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	77576	7.00	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	140.00%#
7) Chloroethane-d5	1.58	69	40622	4.80	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.00%
11) 1,1-Dichloroethene-d2	2.13	63	76895	4.24	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.80%
20) 2-Butanone-d5	3.96	46	166809	69.72	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	139.44%#
24) Chloroform-d	4.40	84	145453	6.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	132.60%#
26) 1,2-Dichloroethane-d4	5.08	65	69943	6.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	134.80%#
32) Benzene-d6	5.10	84	289682	6.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	127.40%#
36) 1,2-Dichloropropane-d6	6.12	67	85053	6.35	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	127.00%
41) Toluene-d8	7.36	98	241088	5.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	116.20%
43) trans-1,3-Dichloropropene-	7.66	79	29603	5.77	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	115.40%
46) 2-Hexanone-d5	8.14	63	88896	54.06	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.12%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	53022	5.68	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	113.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	84768	7.07	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	141.40%#


Target Compounds					Ovalue
13) Acetone	2.23	43	7884	5.288 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081619\
Data File : VV012266.D
Acq On : 16 Aug 2019 13:11
Operator : SY/MD
Sample : K4373-09
Misc : 25mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ4

Quant Time: Aug 17 00:09:41 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 16 23:35:37 2019
Response via : Initial Calibration

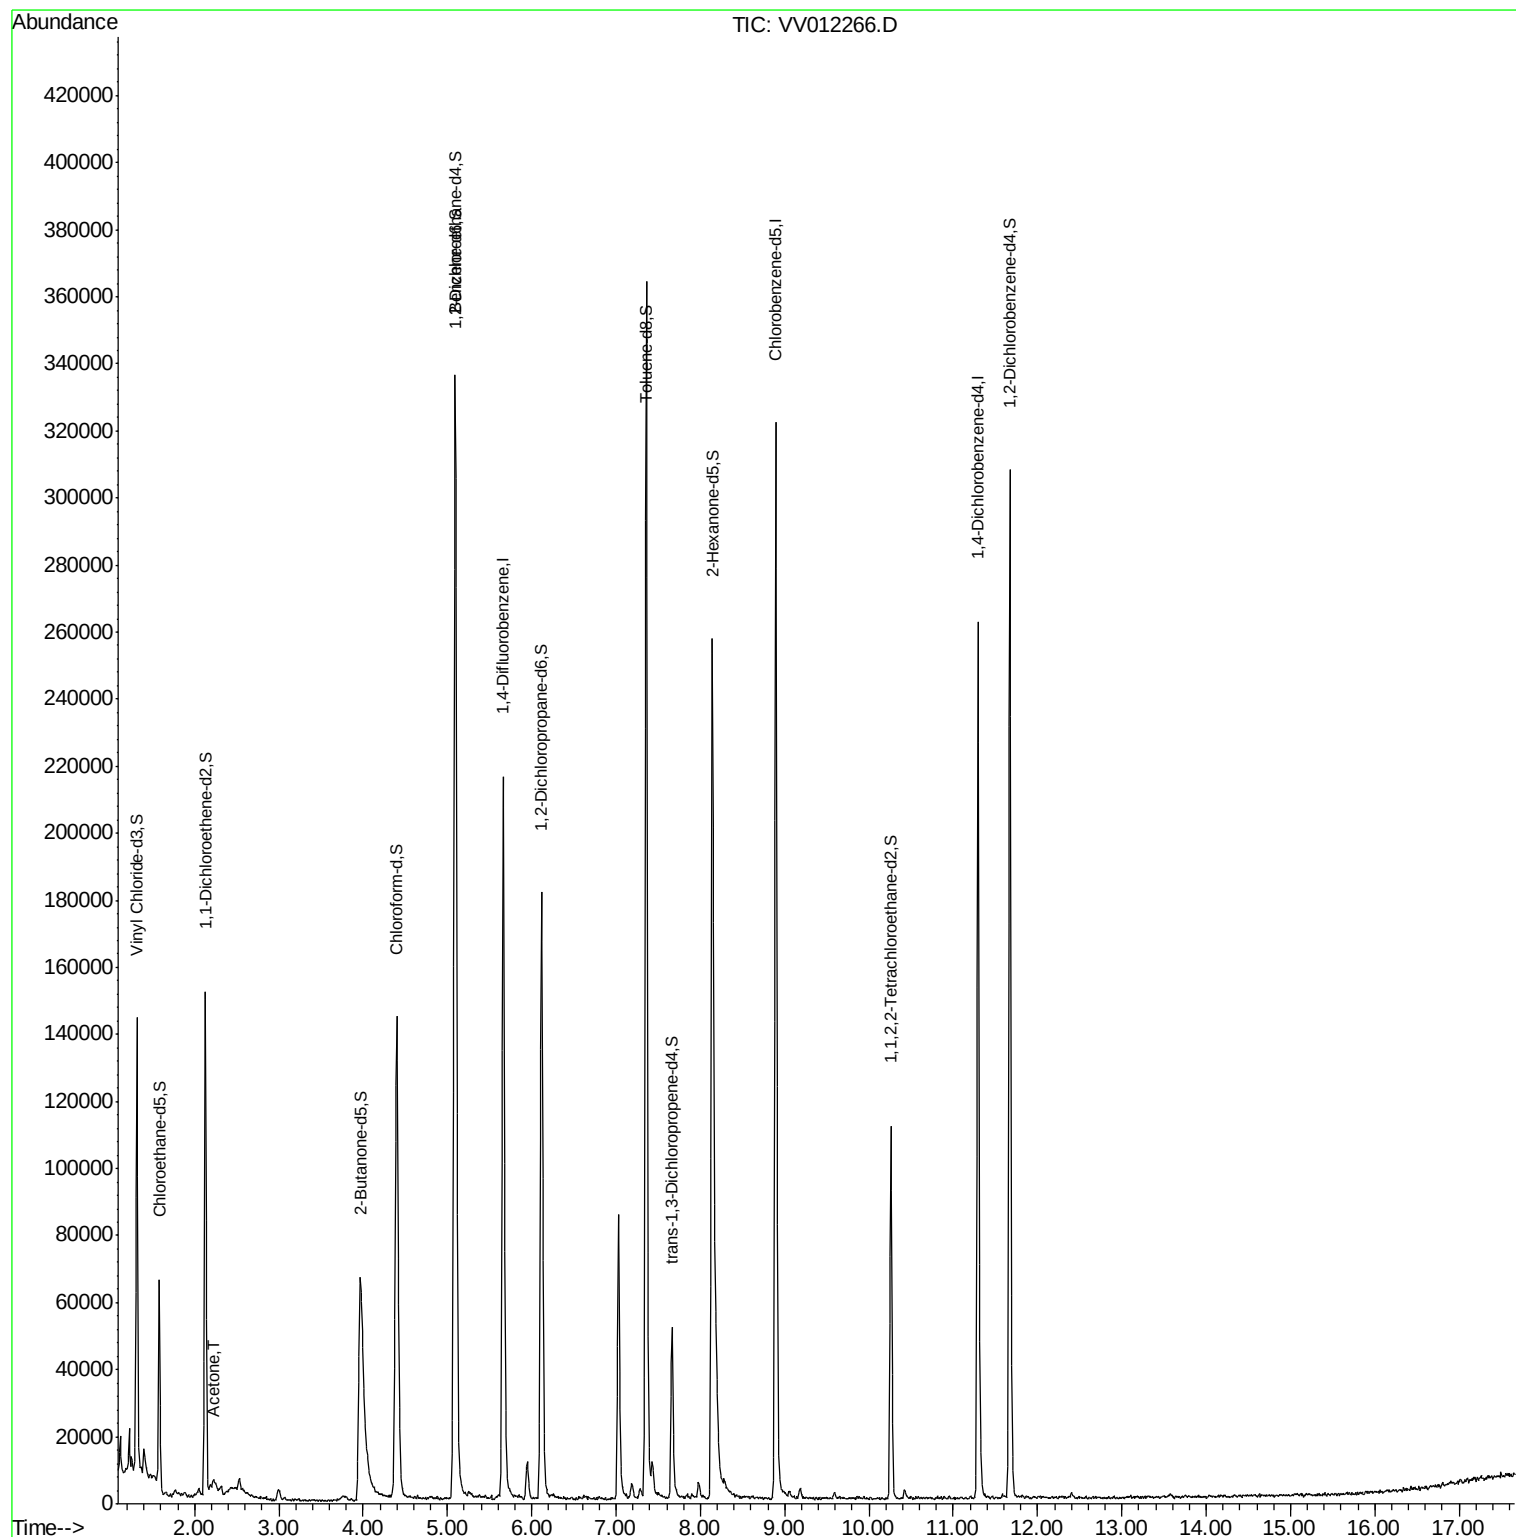

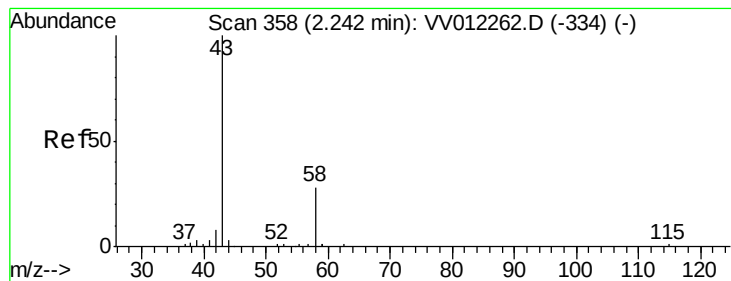

#13

Acetone

Concen: 5.288 ug/L

RT: 2.23 min Scan# 353

Delta R.T. -0.02 min

Lab File: VV012266.D

Acq: 16 Aug 2019 13:11

Instrument :
MSVOA_V
ClientSampleId :
C0AJ4

Tot Ion: 43 Resp: 7884

Ion Ratio Lower Upper

43 100

58 26.5 0.0 59.4

