

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081619\
 Data File : VV012268.D
 Acq On : 16 Aug 2019 14:06
 Operator : SY/MD
 Sample : K4373-06
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF4

Quant Time: Aug 17 00:49:53 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 16 23:35:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	166648	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	163896	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	64518	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	76370	7.44	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	148.80%#
7) Chloroethane-d5	1.58	69	61770	7.87	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	157.40%#
11) 1,1-Dichloroethene-d2	2.13	63	69235	4.12	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.40%
20) 2-Butanone-d5	3.94	46	41594	18.76	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	37.52%#
24) Chloroform-d	4.40	84	111896	5.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.00%
26) 1,2-Dichloroethane-d4	5.08	65	61020	6.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	126.80%
32) Benzene-d6	5.10	84	255382	6.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	123.20%
36) 1,2-Dichloropropane-d6	6.12	67	83572	6.84	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	136.80%
41) Toluene-d8	7.36	98	242048	6.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	127.80%
43) trans-1,3-Dichloropropene-	7.66	79	26869	5.74	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	114.80%
46) 2-Hexanone-d5	8.13	63	77436	51.61	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.22%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	52864	6.21	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	124.20%#
64) 1,2-Dichlorobenzene-d4	11.67	152	84956	7.78	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	155.60%#


Target Compounds					Ovalue
13) Acetone	2.19	43	4250	3.076 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081619\
Data File : VV012268.D
Acq On : 16 Aug 2019 14:06
Operator : SY/MD
Sample : K4373-06
Misc : 25mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF4

Quant Time: Aug 17 00:49:53 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 16 23:35:37 2019
Response via : Initial Calibration

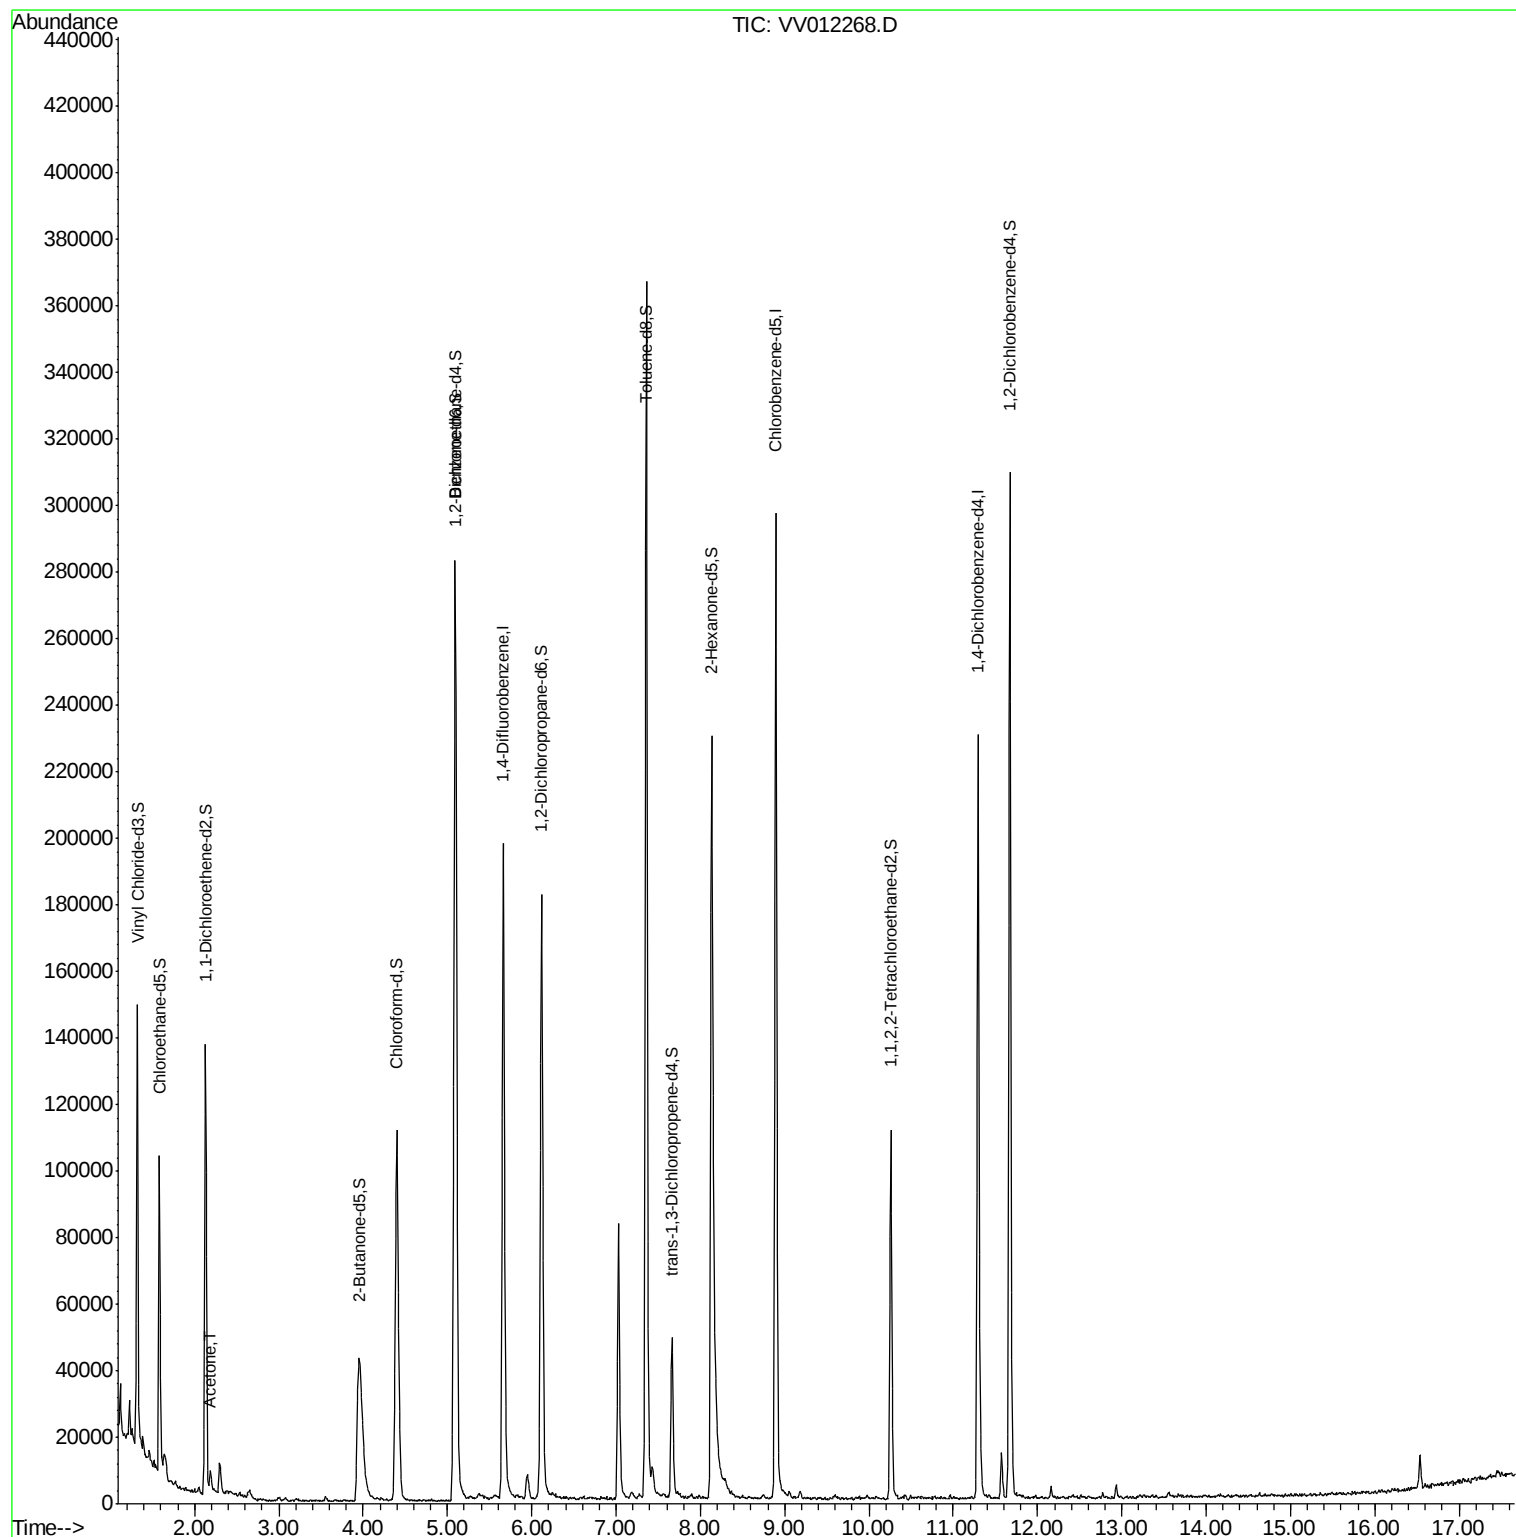

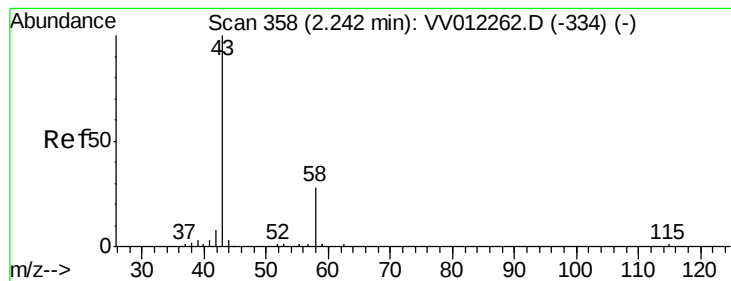

#13
 Acetone
 Concen: 3.076 ug/L
 RT: 2.19 min Scan# 341
 Delta R.T. -0.05 min
 Lab File: VV012268.D
 Acq: 16 Aug 2019 14:06

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF4

Tot Ion: 43 Resp: 4250
 Ion Ratio Lower Upper
 43 100
 58 28.2 0.0 59.4

