

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081619\
 Data File : VV012271.D
 Acq On : 16 Aug 2019 15:27
 Operator : SY/MD
 Sample : K4337-17
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH5

Quant Time: Aug 17 00:45:06 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 16 23:35:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	202201	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	202993	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	80613	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	75283	6.04	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	120.80%
7) Chloroethane-d5	1.58	69	58844	6.18	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	123.60%
11) 1,1-Dichloroethene-d2	2.13	63	65860	3.23	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.60%
20) 2-Butanone-d5	3.94	46	150385	55.89	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.78%
24) Chloroform-d	4.40	84	128471	5.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.20%
26) 1,2-Dichloroethane-d4	5.08	65	73743	6.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	126.40%
32) Benzene-d6	5.10	84	293666	5.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	114.20%
36) 1,2-Dichloropropane-d6	6.12	67	87557	5.79	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	115.80%
41) Toluene-d8	7.36	98	241029	5.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.80%
43) trans-1,3-Dichloropropene-	7.66	79	29599	5.11	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	102.20%
46) 2-Hexanone-d5	8.14	63	102599	55.21	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	110.42%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	56698	5.38	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	88414	6.48	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	129.60%#


Target Compounds					Ovalue
13) Acetone	2.20	43	10984	6.551 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081619\
Data File : VV012271.D
Acq On : 16 Aug 2019 15:27
Operator : SY/MD
Sample : K4337-17
Misc : 25mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH5

Quant Time: Aug 17 00:45:06 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 16 23:35:37 2019
Response via : Initial Calibration

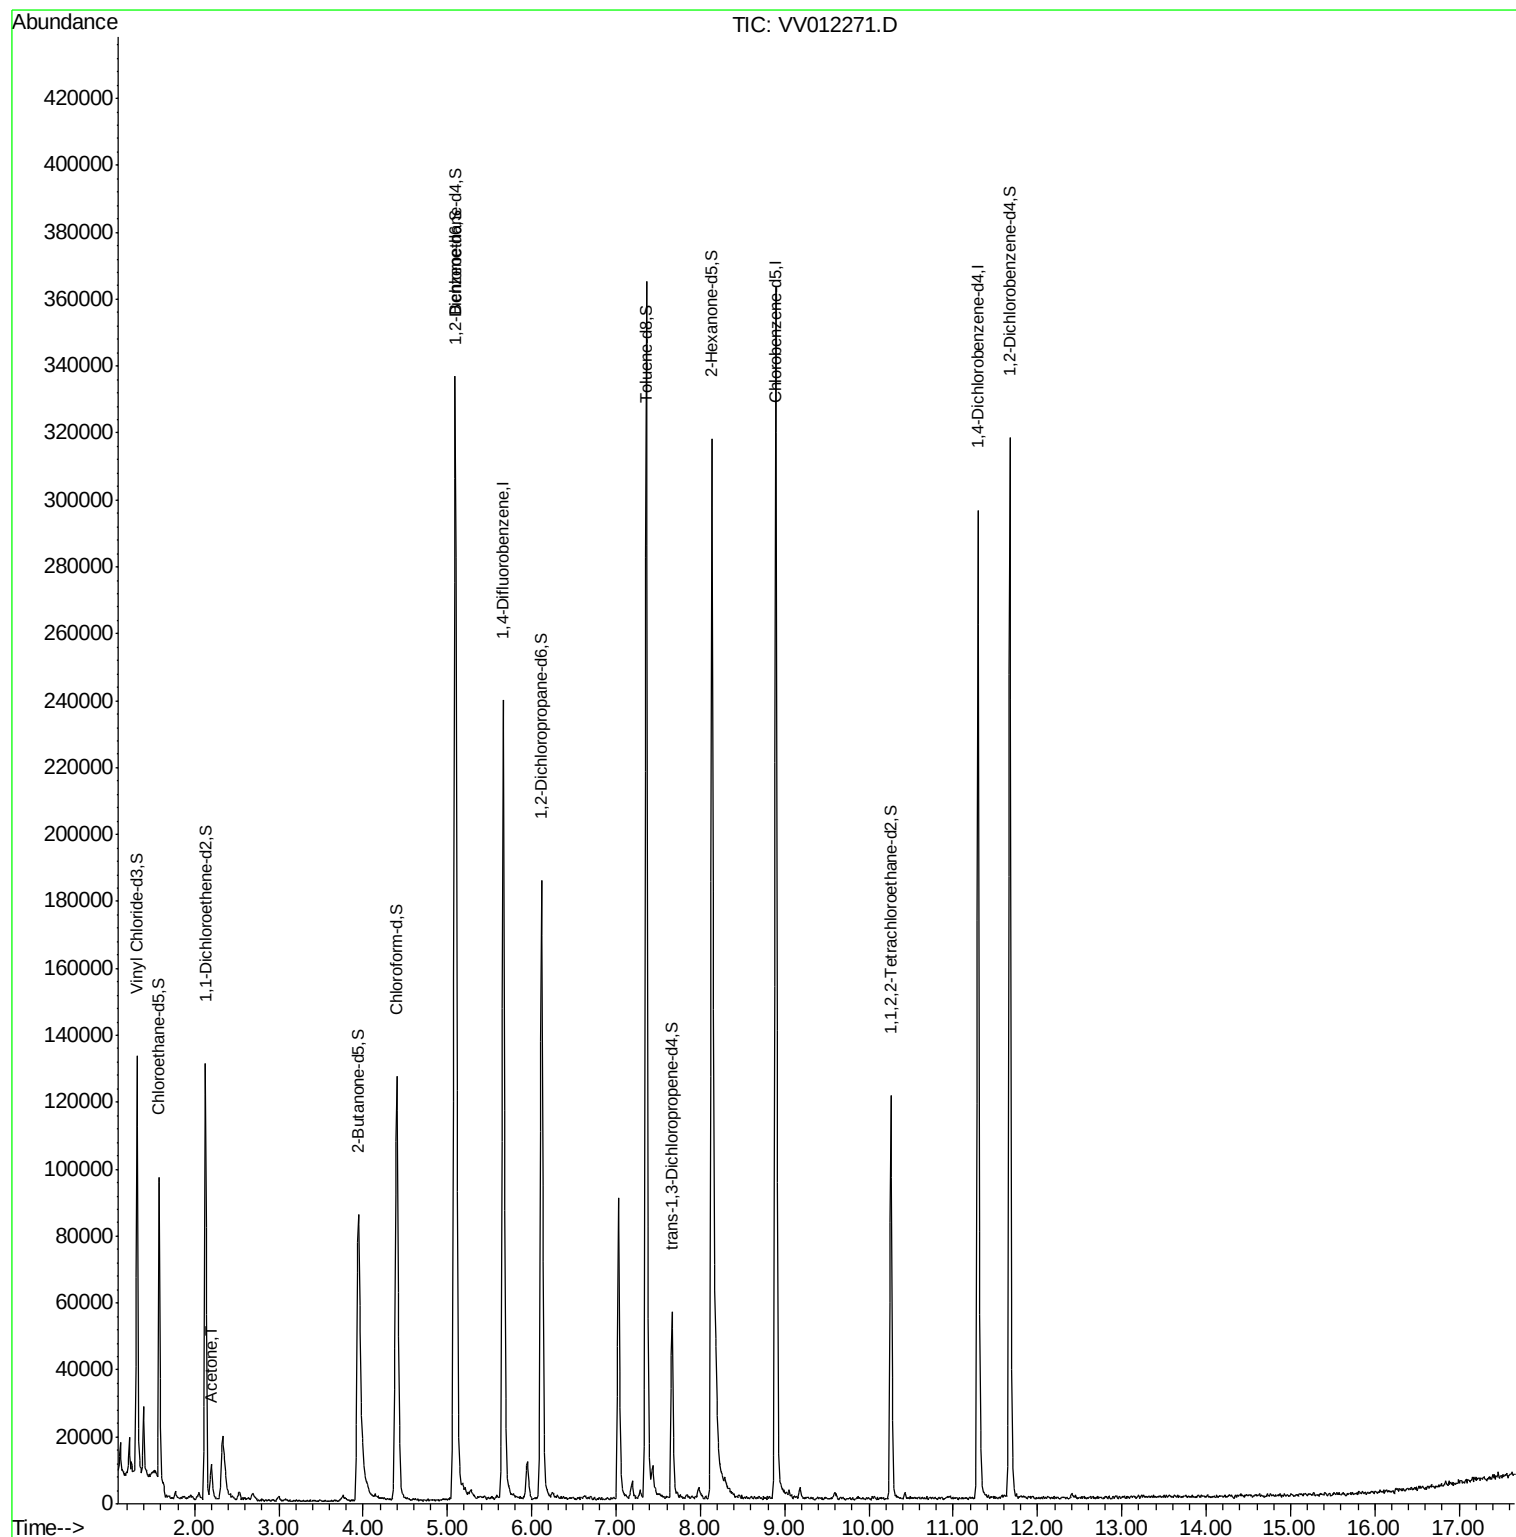

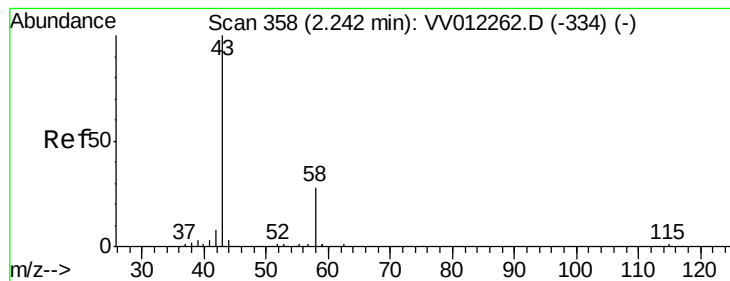

#13

Acetone

Concen: 6.551 ug/L

RT: 2.20 min Scan# 345

Delta R.T. -0.04 min

Lab File: VV012271.D

Acq: 16 Aug 2019 15:27

Instrument :
MSVOA_V
ClientSampleId :
C0AH5

Tot Ion: 43 Resp: 10984

Ion Ratio Lower Upper

43 100

58 27.9 0.0 59.4

