

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081619\
 Data File : VV012272.D
 Acq On : 16 Aug 2019 15:54
 Operator : SY/MD
 Sample : K4337-18
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ3

Quant Time: Aug 17 00:53:03 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 16 23:35:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	162254	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	168042	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	75743	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	71057	7.11	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	142.20%#
7) Chloroethane-d5	1.58	69	56063	7.34	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	146.80%#
11) 1,1-Dichloroethene-d2	2.13	63	56081	3.43	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.60%
20) 2-Butanone-d5	3.96	46	117429	54.39	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.78%
24) Chloroform-d	4.40	84	105453	5.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.60%
26) 1,2-Dichloroethane-d4	5.08	65	54614	5.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	116.60%
32) Benzene-d6	5.10	84	213359	5.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.40%
36) 1,2-Dichloropropane-d6	6.12	67	62633	5.00	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.00%
41) Toluene-d8	7.36	98	190827	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.40%
43) trans-1,3-Dichloropropene-	7.67	79	25368	5.29	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	105.80%
46) 2-Hexanone-d5	8.14	63	81042	52.68	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.36%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	50728	5.81	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	116.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	80362	6.27	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	125.40%#


Target Compounds					Ovalue
13) Acetone	2.21	43	9652	7.174 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081619\
Data File : VV012272.D
Acq On : 16 Aug 2019 15:54
Operator : SY/MD
Sample : K4337-18
Misc : 25mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ3

Quant Time: Aug 17 00:53:03 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 16 23:35:37 2019
Response via : Initial Calibration

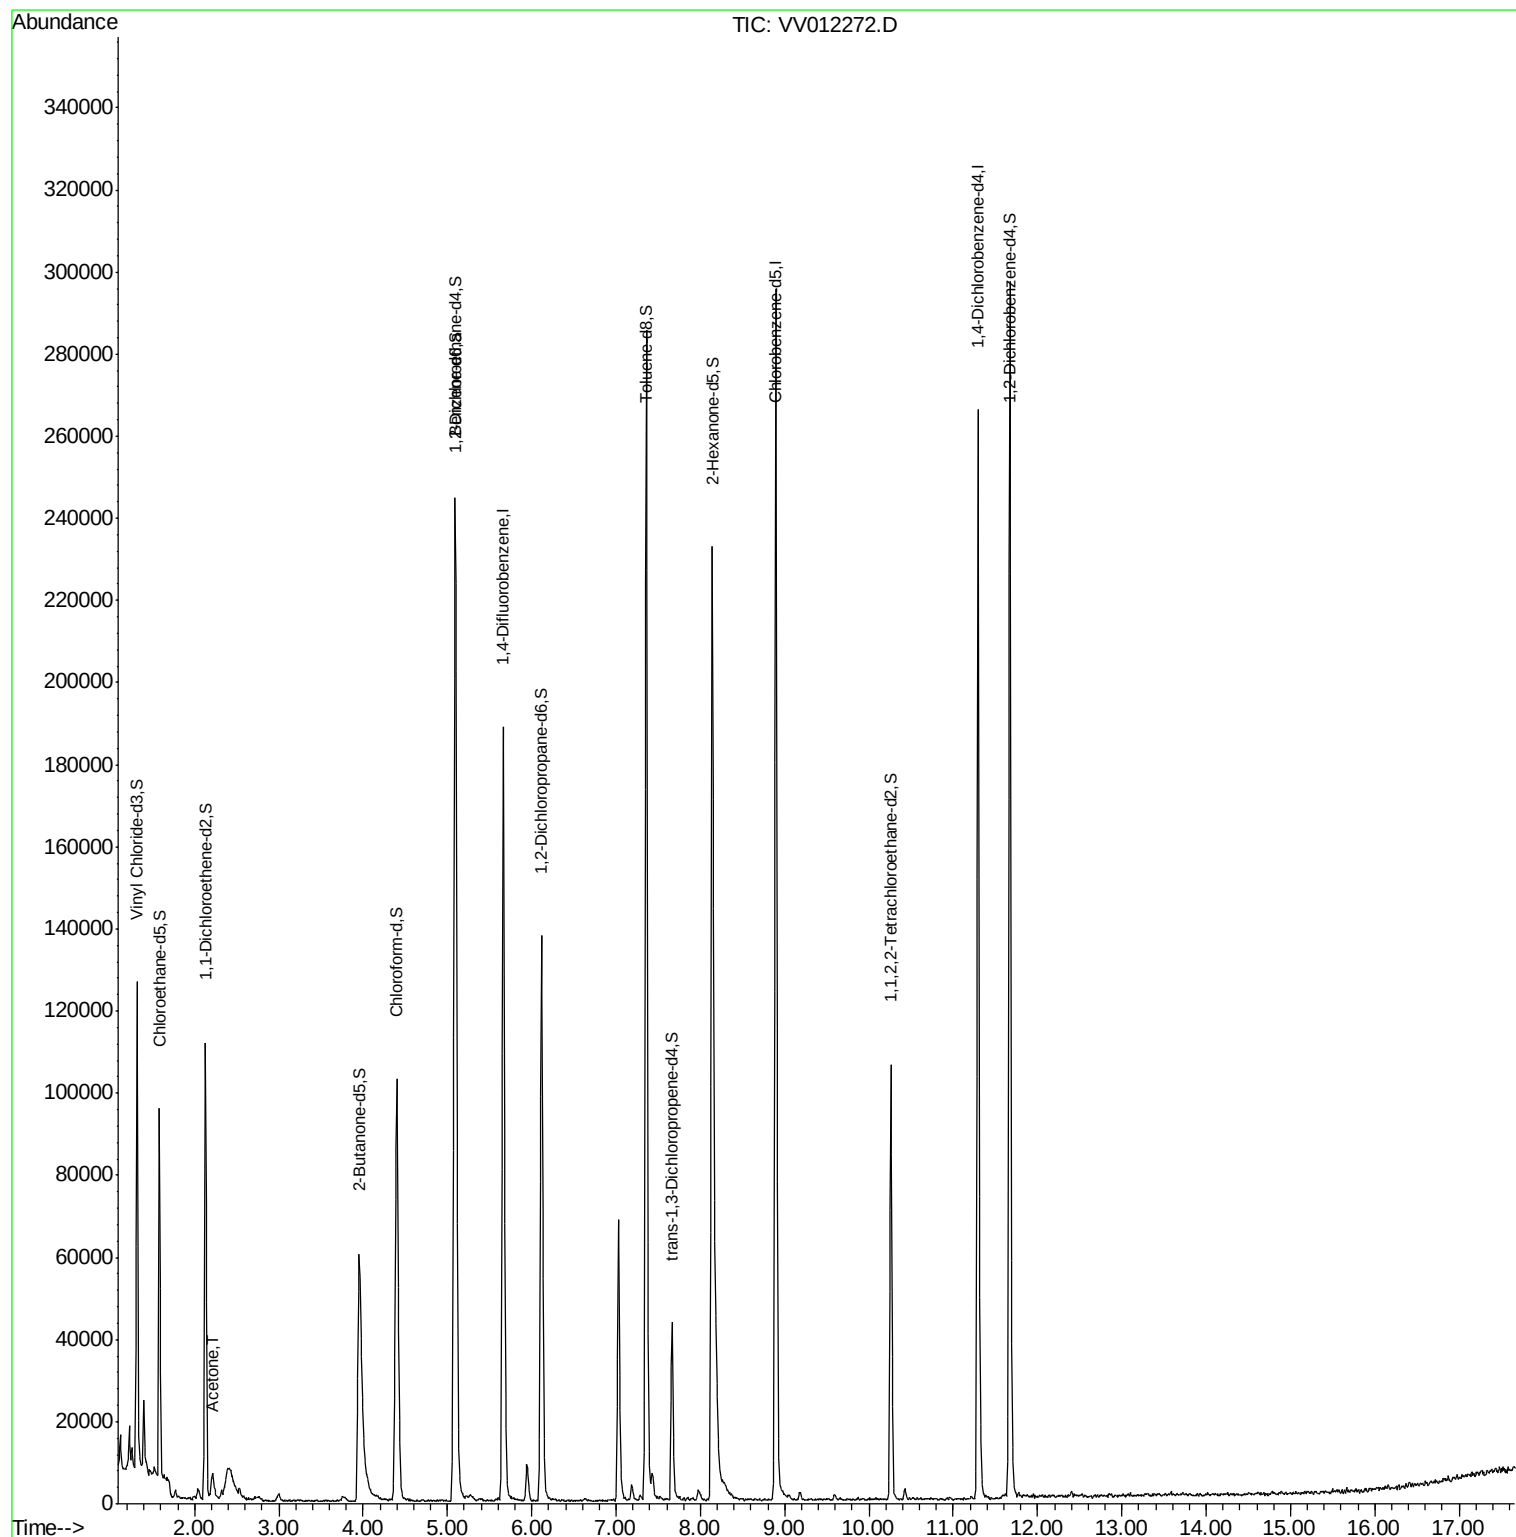

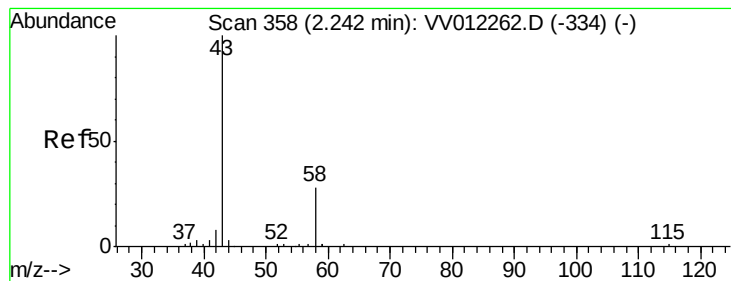

#13
 Acetone
 Concen: 7.174 ug/L
 RT: 2.21 min Scan# 349
 Delta R.T. -0.03 min
 Lab File: VV012272.D
 Acq: 16 Aug 2019 15:54

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ3

Tot Ion: 43 Resp: 9652
 Ion Ratio Lower Upper
 43 100
 58 24.3 0.0 59.4

