


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV081619\
 Data File : VV012261.D
 Acq On : 16 Aug 2019 08:43
 Operator : SY/MD
 Sample : BFB49
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB49

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081319WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Aug 16 23:35:37 2019

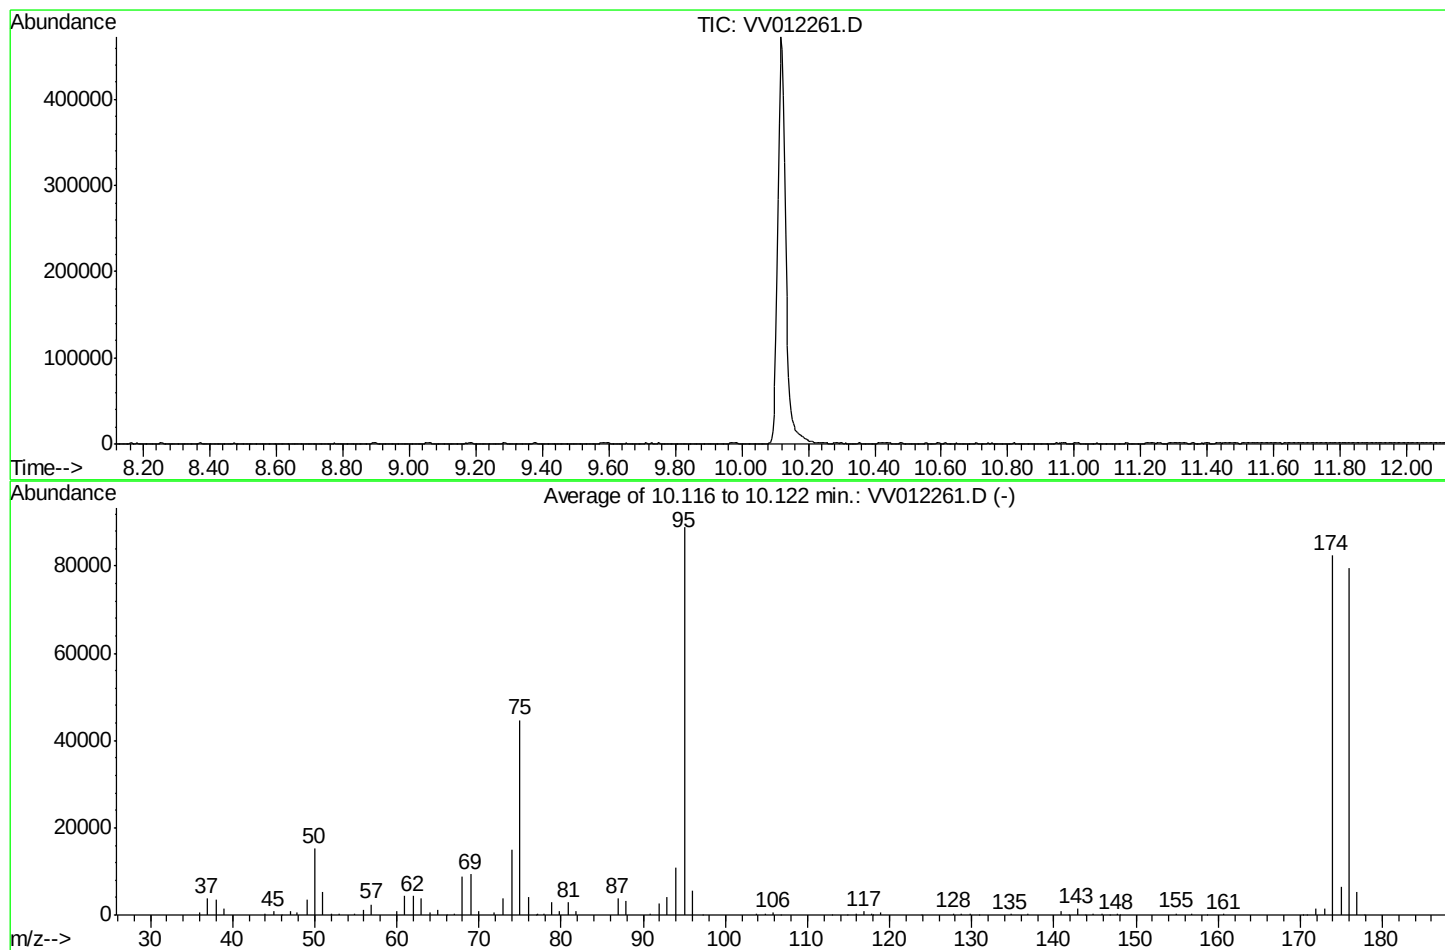

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	15140	PASS
75	95	30	80	50.3	44690	PASS
95	95	100	100	100.0	88890	PASS
96	95	5	9	6.4	5716	PASS
173	174	0.00	2	1.6	1348	PASS
174	95	50	120	92.8	82472	PASS
175	174	5	9	7.7	6355	PASS
176	174	95	101	96.5	79608	PASS
177	176	5	9	6.7	5294	PASS

m/z	Abundance
35.90	639.0
36.90	3805.0
38.00	3485.0
39.00	1460.0
39.90	314.0
44.00	643.0
44.90	752.0
47.00	823.0
47.90	555.0
49.00	3185.0
50.00	15202.0
51.00	5036.0
52.10	260.0
53.00	191.0
54.90	337.0
56.00	1199.0
56.90	2247.0
60.00	914.0
60.90	4158.0
62.00	4279.0
63.00	3874.0
63.90	527.0
65.00	1064.0
67.00	263.0
68.00	8492.0
69.00	9400.0
70.00	750.0
71.90	605.0
73.00	3998.0
73.90	14293.0
75.00	43584.0
76.00	4005.0
76.90	399.0
77.80	353.0
78.90	2628.0
79.90	950.0
80.90	2687.0
81.80	745.0
86.90	3555.0
87.90	3241.0
90.80	336.0
91.90	2672.0
92.90	4051.0
93.90	10818.0
95.00	86856.0
96.00	5703.0
97.20	143.0
103.80	492.0
104.90	148.0
105.90	469.0
106.80	131.0
114.90	124.0
115.90	380.0
116.90	729.0
117.80	349.0
118.80	559.0
123.90	102.0
127.80	359.0
128.70	191.0
129.90	276.0
130.90	111.0
134.80	221.0
136.70	148.0
140.90	851.0
142.90	1332.0
143.80	157.0
144.90	328.0
145.80	172.0
146.80	107.0
147.70	164.0
148.00	185.0
154.90	339.0
156.90	156.0
158.70	164.0
160.70	149.0
170.90	134.0
171.90	1216.0
173.00	1324.0
173.90	79008.0
174.90	5926.0
175.90	74944.0
176.90	5104.0
177.80	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

m/z	Abundance
35.90	663.0
36.90	3884.0
37.90	3611.0
39.00	1637.0
39.90	319.0
44.00	620.0
45.00	819.0
46.00	106.0
47.00	998.0
47.90	599.0
49.00	3503.0
50.00	15490.0
51.00	5367.0
52.00	286.0
53.00	191.0
54.90	387.0
56.00	1236.0
56.90	2491.0
60.00	861.0
60.90	4480.0
62.00	4552.0
62.90	3994.0
64.00	517.0
65.00	1080.0
66.10	103.0
67.00	259.0
67.90	9093.0
69.00	9632.0
70.00	762.0
71.80	588.0
73.00	4095.0
74.00	15489.0
75.00	46256.0
76.00	4283.0
77.10	443.0
77.90	395.0
78.90	2896.0
79.80	988.0
80.90	2899.0
81.80	777.0
86.90	3839.0
87.90	3354.0
90.80	327.0
91.90	2845.0
92.90	4317.0
94.00	11406.0
95.00	91656.0
96.00	5980.0
97.20	158.0
103.80	428.0
104.80	162.0
105.80	526.0
106.80	117.0
112.90	107.0
115.90	409.0
116.90	794.0
117.80	299.0
118.90	623.0
127.90	410.0
128.80	221.0
129.80	309.0
130.90	131.0
134.80	266.0
136.80	169.0
140.80	929.0
141.80	130.0
142.90	1469.0
143.90	156.0
144.80	328.0
145.80	175.0
146.90	125.0
147.70	178.0
148.00	177.0
154.90	337.0
156.90	209.0
158.70	153.0
160.80	190.0
170.30	121.0
170.90	159.0
171.90	1419.0
173.00	1409.0
173.90	85200.0
174.90	6538.0
175.90	82144.0
176.90	5484.0
177.80	142.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

m/z	Abundance
35.90	634.0
36.90	3629.0
37.90	3294.0
39.00	1774.0
40.00	320.0
44.00	634.0
44.90	830.0
47.00	1076.0
47.90	556.0
49.00	3530.0
50.00	14730.0
51.00	5090.0
52.00	341.0
53.00	158.0
54.90	333.0
56.00	1147.0
56.90	2478.0
60.00	728.0
60.90	4206.0
62.00	4246.0
62.90	3628.0
64.10	479.0
65.00	1022.0
66.90	251.0
67.90	8777.0
69.00	8880.0
70.00	750.0
71.80	562.0
72.90	3722.0
74.00	15208.0
75.00	44232.0
76.00	3970.0
77.10	446.0
77.90	392.0
78.90	2926.0
79.80	907.0
80.90	2918.0
81.80	776.0
86.90	3816.0
87.90	3192.0
90.80	292.0
91.90	2717.0
92.90	4208.0
94.00	10806.0
95.00	88160.0
96.00	5466.0
97.20	136.0
103.80	325.0
104.80	176.0
105.80	514.0
106.80	101.0
112.90	149.0
115.90	353.0
116.90	772.0
118.00	264.0
119.00	643.0
127.90	443.0
128.80	226.0
129.80	322.0
130.90	123.0
134.80	270.0
136.80	176.0
140.80	1053.0
141.70	158.0
142.90	1325.0
143.80	132.0
144.80	277.0
145.80	184.0
146.90	117.0
147.70	211.0
155.00	241.0
156.80	186.0
158.70	142.0
160.80	207.0
170.80	168.0
171.90	1388.0
172.90	1313.0
173.90	83208.0
175.00	6602.0
175.90	81736.0
176.90	5295.0
177.80	143.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

Scan 2794 (10.074 min): VV012261.D
BFB49

m/z	Abundance
39.90	410.0
43.80	241.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49