




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081621\
 Data File : VV021792.D
 Acq On : 16 Aug 2021 15:41
 Operator : SY/MD
 Sample : M3364-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKC6

Manual Integrations
 APPROVED

MMDadoda
 8/19/2021 3:35:03 PM

Quant Time: Aug 17 04:30:31 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 17 04:08:59 2021
 Response via : Initial Calibration

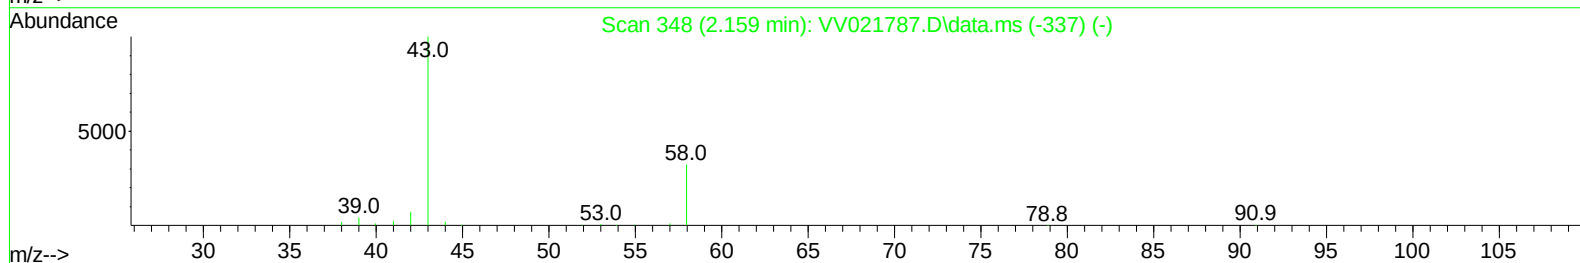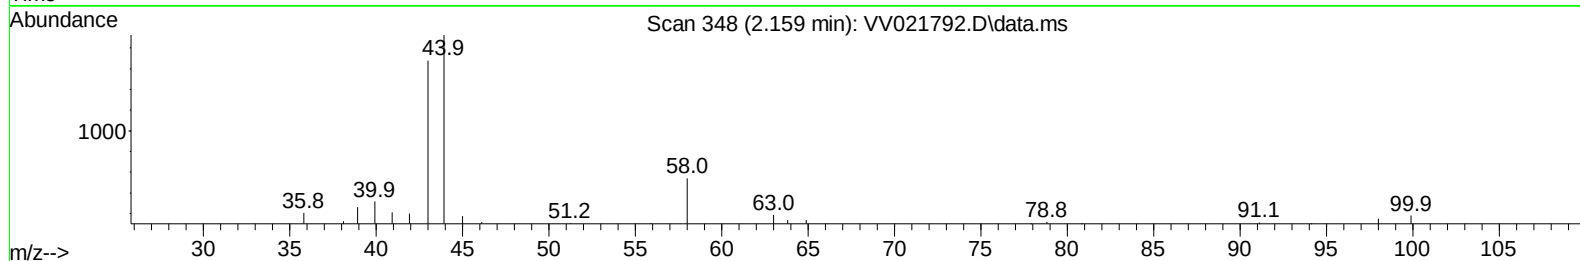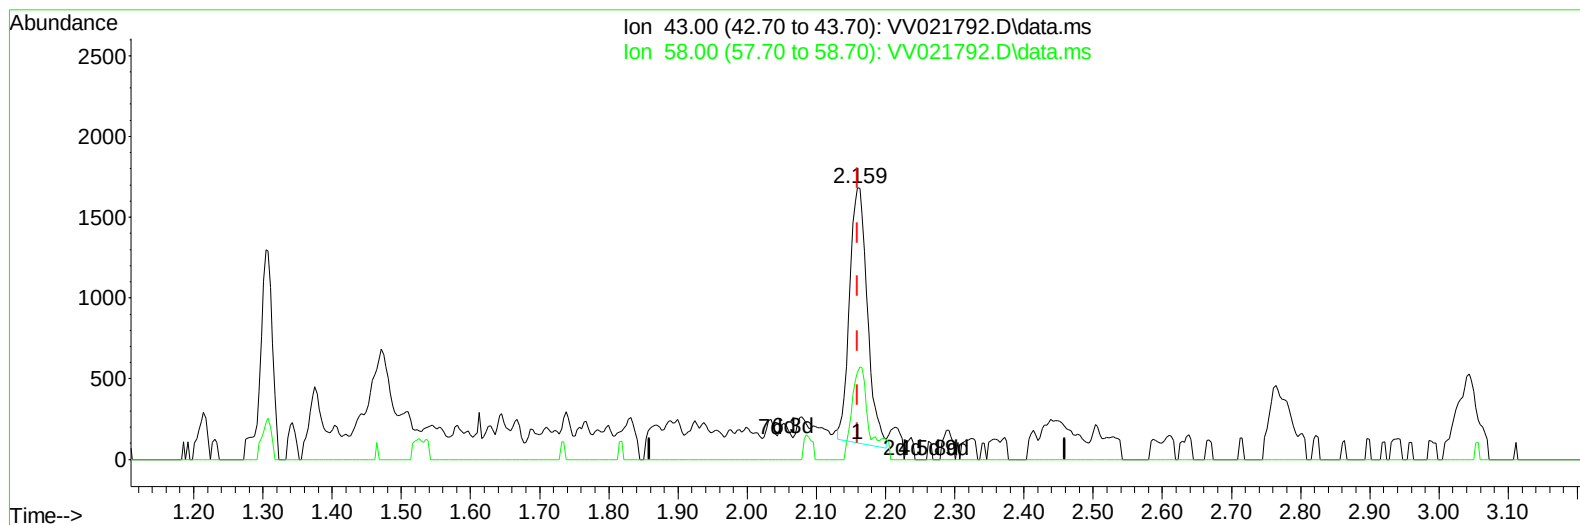

TIC: VV021792.D\data.ms

(13) Acetone (T)

2.159min (+ 0.000) 2.58 ug/L

response 2823

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	0.00	28.87#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081621\
 Data File : VV021792.D
 Acq On : 16 Aug 2021 15:41
 Operator : SY/MD
 Sample : M3364-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKC6

Manual Integrations
 APPROVED

MMDadoda
 8/19/2021 3:35:03 PM

Quant Time: Aug 17 04:30:31 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 17 04:08:59 2021
 Response via : Initial Calibration

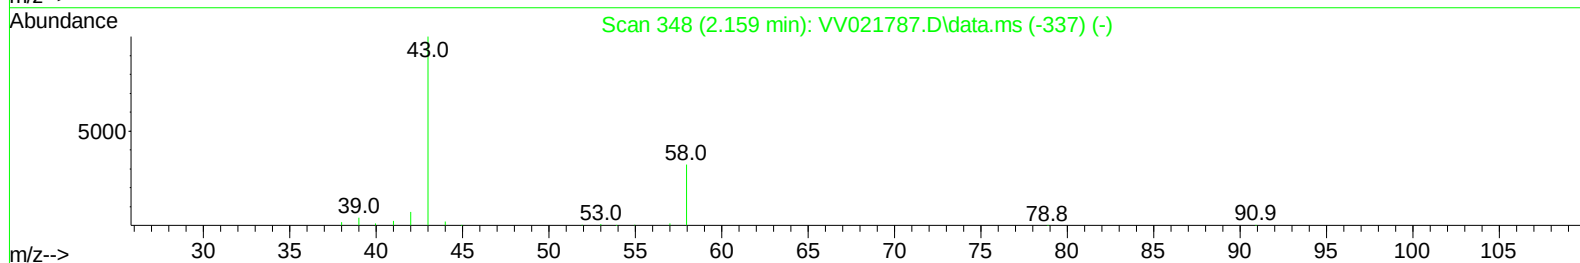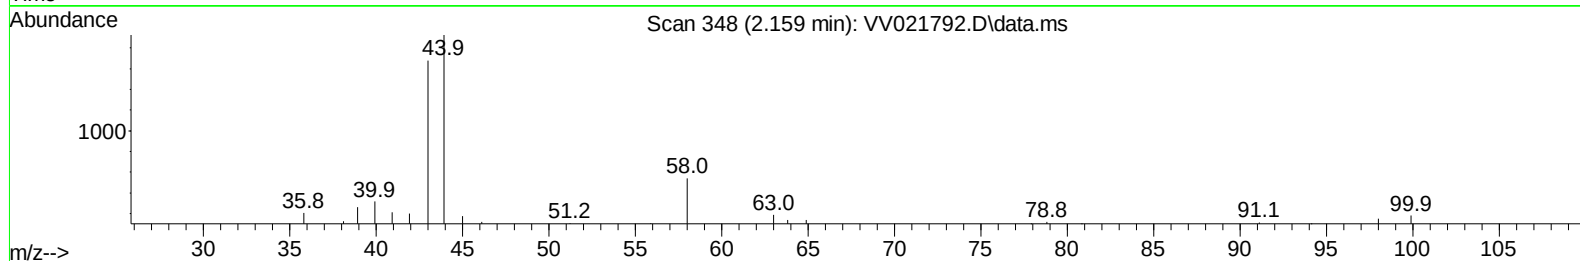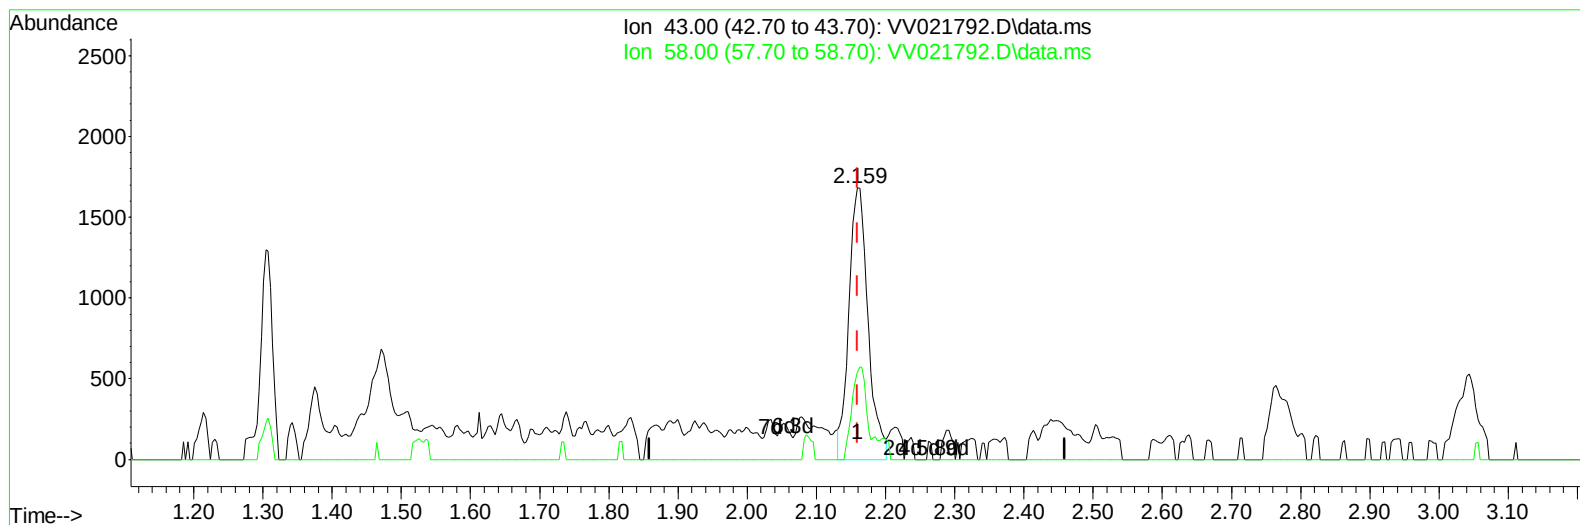

TIC: VV021792.D\data.ms

(13) Acetone (T)

2.159min (+ 0.000) 2.95 ug/L m

response 3233

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	0.00	25.21#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081621\
 Data File : VV021792.D
 Acq On : 16 Aug 2021 15:41
 Operator : SY/MD
 Sample : M3364-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKC6

Manual Integrations
 APPROVED

MMDadoda
 8/19/2021 3:35:03 PM

Quant Time: Aug 17 04:30:31 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 17 04:08:59 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	273553	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	250492	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	114867	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	102997	48.162	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	96.320%	
7) Chloroethane-d5	1.555	69	79595	49.321	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	98.640%	
11) 1,1-Dichloroethene-d2	2.102	63	125146	36.763	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	73.520%	
21) 2-Butanone-d5	3.876	46	181904	136.766	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	136.770%#	
24) Chloroform-d	4.349	84	176421	47.616	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	95.240%	
26) 1,2-Dichloroethane-d4	5.034	65	109568	51.411	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	102.820%	
32) Benzene-d6	5.050	84	373671	51.875	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	103.760%	
36) 1,2-Dichloropropane-d6	6.069	67	118048	52.626	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	105.260%	
41) Toluene-d8	7.317	98	333441	50.082	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	100.160%	
43) trans-1,3-Dichloroprop...	7.625	79	49268	44.628	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	89.260%	
47) 2-Hexanone-d5	8.088	63	93326	126.940	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	126.940%	
56) 1,1,2,2-Tetrachloroeth...	10.220	84	153933	55.376	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	110.760%	
66) 1,2-Dichlorobenzene-d4	11.625	152	125505	52.795	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	105.600%	
Target Compounds						
13) Acetone	2.159	43	3233m	2.954	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081621\
Data File : VV021792.D
Acq On : 16 Aug 2021 15:41
Operator : SY/MD
Sample : M3364-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKC6

Manual Integrations
APPROVED

MMDadoda
8/19/2021 3:35:03 PM

Quant Time: Aug 17 04:30:31 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 17 04:08:59 2021
Response via : Initial Calibration

