


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081621\
 Data File : VV021778.D
 Acq On : 16 Aug 2021 08:49
 Operator : SY/MD
 Sample : BFB215
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB215

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Title : VOC Analysis
 Last Update : Thu Aug 19 01:14:55 2021

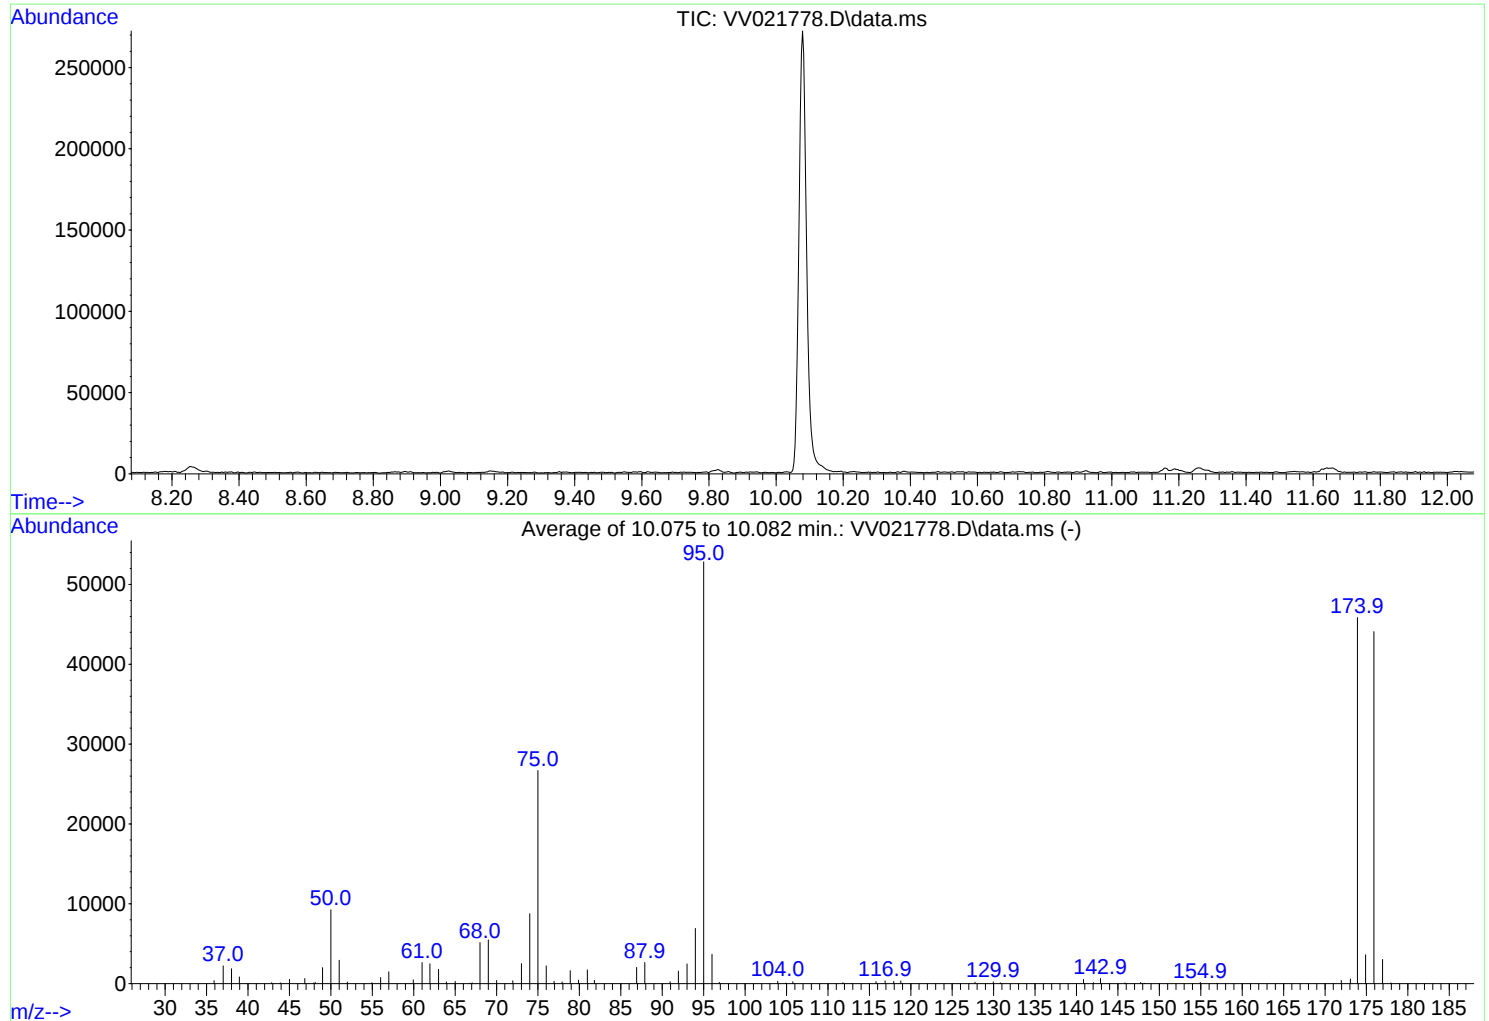

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	9244	PASS
75	95	30	80	50.5	26688	PASS
95	95	100	100	100.0	52827	PASS
96	95	5	9	7.0	3690	PASS
173	174	0.00	2	1.3	575	PASS
174	95	50	120	86.8	45848	PASS
175	174	5	9	7.9	3610	PASS
176	174	95	105	96.2	44091	PASS
177	176	5	10	6.9	3033	PASS

m/z	Abundance
39.90	217.0
41.10	162.0
44.00	599.0

Instrument :
MSVOA_V
ClientSampleId :
BFB215

m/z	Abundance
35.90	411.0
37.00	2319.0
38.00	1897.0
38.90	760.0
39.90	210.0
42.90	153.0
43.90	691.0
45.00	598.0
46.90	713.0
47.90	257.0
49.00	2113.0
50.00	9417.0
51.00	2919.0
51.90	231.0
55.00	115.0
56.00	702.0
57.00	1468.0
59.90	479.0
61.00	2566.0
62.00	2615.0
63.00	1892.0
63.90	218.0
65.00	299.0
66.80	196.0
68.00	5213.0
69.00	5638.0
70.00	394.0
71.90	354.0
73.00	2470.0
74.00	8924.0
75.00	26256.0
76.00	2368.0
76.90	277.0
77.90	218.0
78.90	1625.0
79.90	457.0
81.00	1704.0
81.80	399.0
86.90	2162.0
87.90	2516.0
90.90	225.0
91.90	1556.0
93.00	2379.0
94.00	6918.0
95.00	51624.0
96.00	3605.0
96.90	180.0
104.00	314.0
105.80	232.0
111.80	118.0
112.80	109.0
115.80	266.0
116.90	348.0
118.00	248.0
118.80	375.0
127.80	186.0
130.00	180.0
130.80	102.0
140.80	500.0
142.10	110.0
142.90	616.0
145.90	188.0
147.80	143.0
155.00	177.0
171.90	451.0
173.00	594.0
173.90	44128.0
174.90	3627.0
175.90	42552.0
176.90	2777.0
178.00	100.0

Instrument :
MSVOA_V
ClientSampleId :
BFB215

m/z	Abundance
35.90	405.0
37.00	2295.0
38.00	1925.0
39.00	901.0
39.80	215.0
42.90	130.0
43.90	734.0
45.00	539.0
46.90	674.0
48.10	277.0
49.00	2083.0
50.00	9614.0
51.00	3078.0
52.00	207.0
55.00	136.0
56.00	786.0
57.00	1556.0
60.00	479.0
61.00	2790.0
61.90	2552.0
63.00	1832.0
64.00	221.0
65.00	294.0
67.00	165.0
68.00	5307.0
69.00	5656.0
70.00	414.0
71.90	360.0
73.00	2632.0
74.00	9047.0
75.00	27712.0
76.00	2292.0
77.00	285.0
77.90	219.0
78.90	1676.0
79.90	419.0
81.00	1760.0
81.80	428.0
86.90	2053.0
87.90	2761.0
90.90	242.0
92.00	1648.0
93.00	2550.0
94.00	7169.0
95.00	54456.0
96.00	3828.0
96.90	182.0
104.00	308.0
104.90	103.0
105.70	241.0
111.80	134.0
115.80	263.0
116.90	352.0
117.90	295.0
118.80	359.0
127.70	204.0
129.90	210.0
130.80	118.0
140.90	539.0
142.10	120.0
142.90	684.0
145.80	146.0
147.70	126.0
148.20	104.0
155.00	162.0
172.00	412.0
173.00	611.0
173.90	47480.0
174.90	3801.0
175.90	45512.0
176.90	3118.0
178.00	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB215

m/z	Abundance
35.90	355.0
37.00	2081.0
38.00	1775.0
39.00	868.0
39.80	225.0
42.80	106.0
43.90	694.0
45.00	464.0
46.80	563.0
48.10	246.0
49.00	1822.0
50.00	8701.0
51.00	2772.0
52.10	137.0
54.90	140.0
56.00	831.0
57.00	1441.0
60.00	509.0
61.00	2603.0
61.90	2264.0
63.00	1629.0
64.00	228.0
65.00	252.0
67.10	139.0
68.00	4912.0
69.00	5126.0
70.00	377.0
72.00	356.0
73.00	2415.0
74.00	8277.0
75.00	26096.0
76.00	2026.0
77.00	280.0
77.90	219.0
78.90	1563.0
79.90	436.0
80.90	1682.0
81.80	402.0
86.90	1848.0
87.90	2652.0
91.00	244.0
92.00	1498.0
93.00	2490.0
94.00	6657.0
95.00	52400.0
96.00	3638.0
96.90	147.0
103.90	309.0
104.90	120.0
105.70	258.0
111.80	109.0
115.80	269.0
116.90	334.0
117.90	282.0
118.80	300.0
127.70	172.0
129.90	245.0
130.80	102.0
140.90	526.0
142.00	110.0
142.90	649.0
147.70	126.0
154.90	133.0
156.90	125.0
172.00	352.0
173.10	519.0
173.90	45936.0
174.90	3402.0
175.90	44208.0
177.00	3203.0
177.90	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB215