




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081622\
 Data File : VV027406.D
 Acq On : 16 Aug 2022 11:55
 Operator : SY/MD
 Sample : N4195-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CZ0

Manual IntegrationsAPPROVED

Quant Time: Aug 17 00:28:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Aug 16 00:24:20 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/19/2022
 Supervised By :Semsettin Yesilyurt 08/22/2022

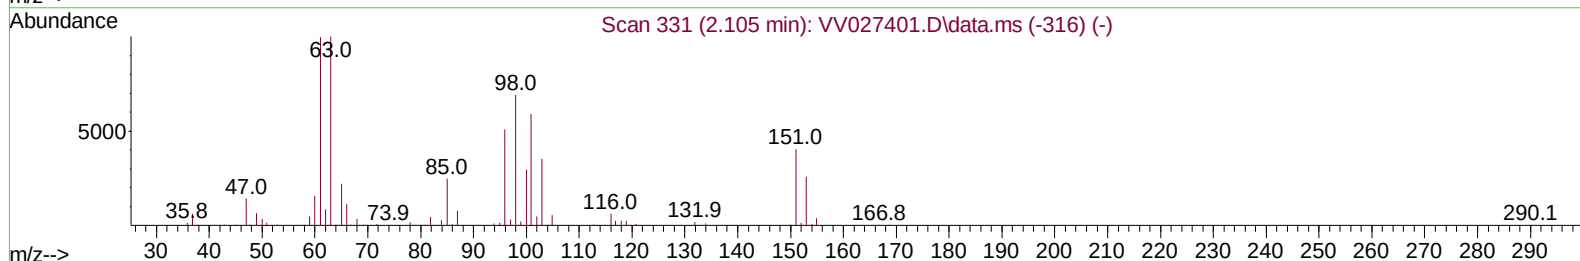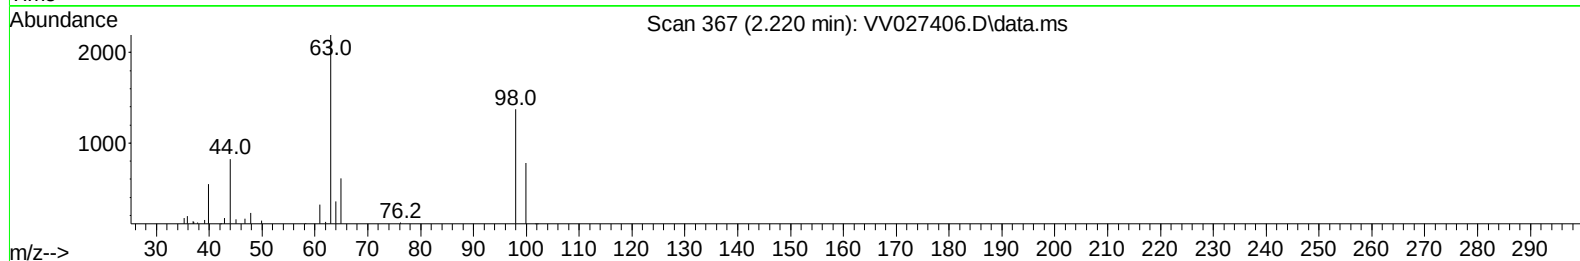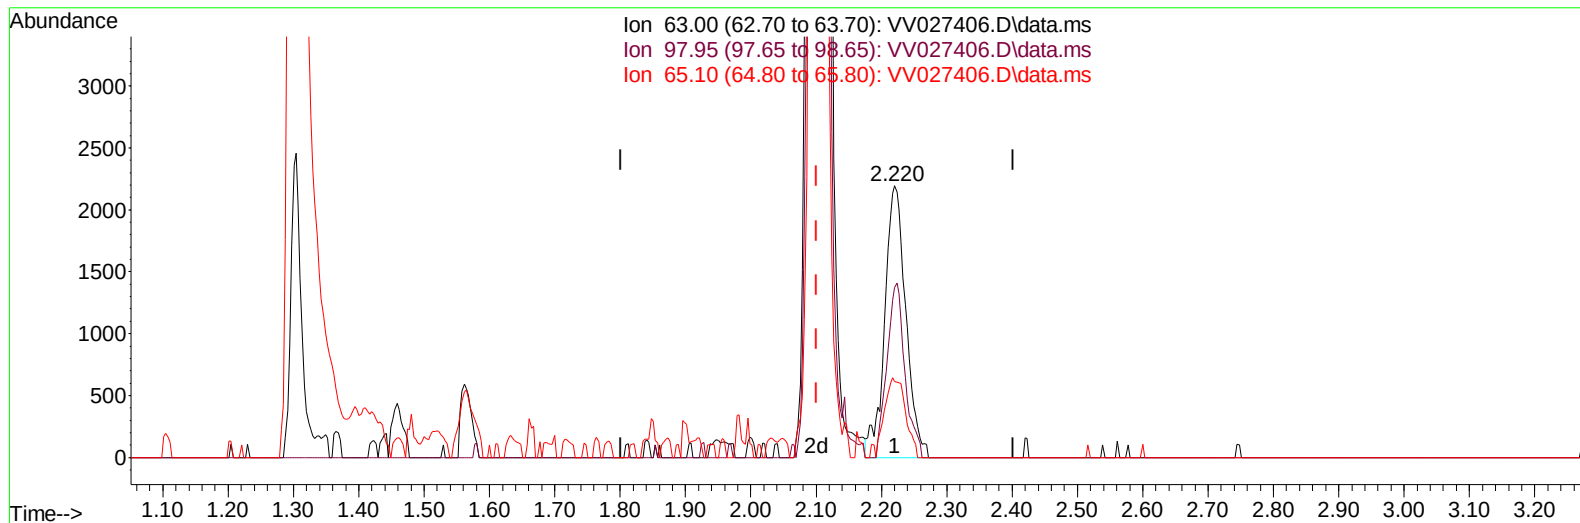

TIC: VV027406.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.220min (+ 0.119) 0.23 ug/L

response 4931

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	67.40	54.49
65.10	23.50	29.04
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081622\
Data File : VV027406.D
Acq On : 16 Aug 2022 11:55
Operator : SY/MD
Sample : N4195-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CZ0

Manual IntegrationsAPPROVED

Quant Time: Aug 17 00:28:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Aug 16 00:24:20 2022
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/19/2022
Supervised By :Semsettin Yesilyurt 08/22/2022

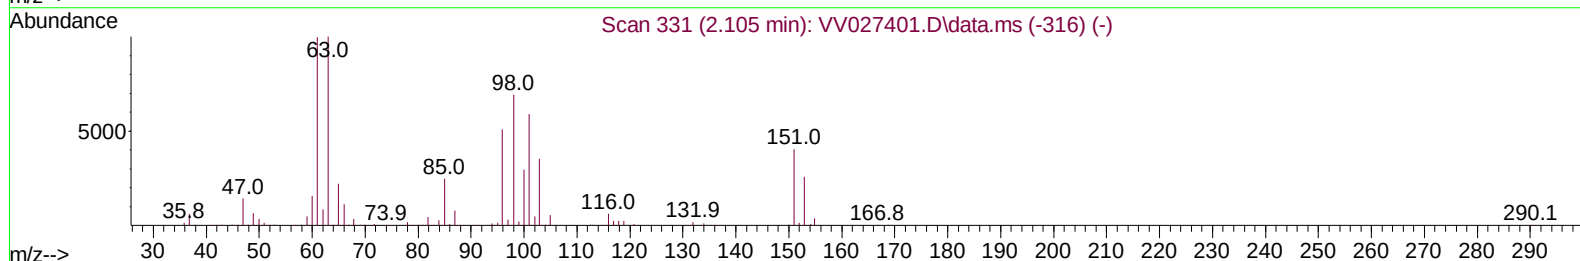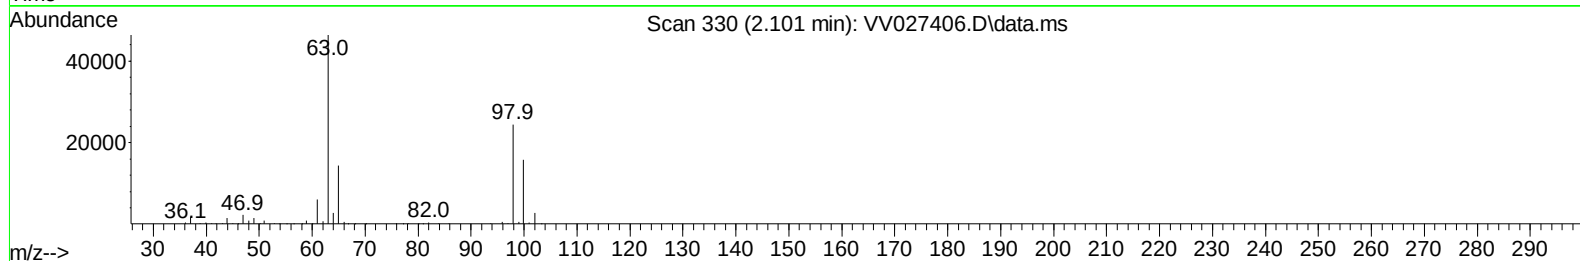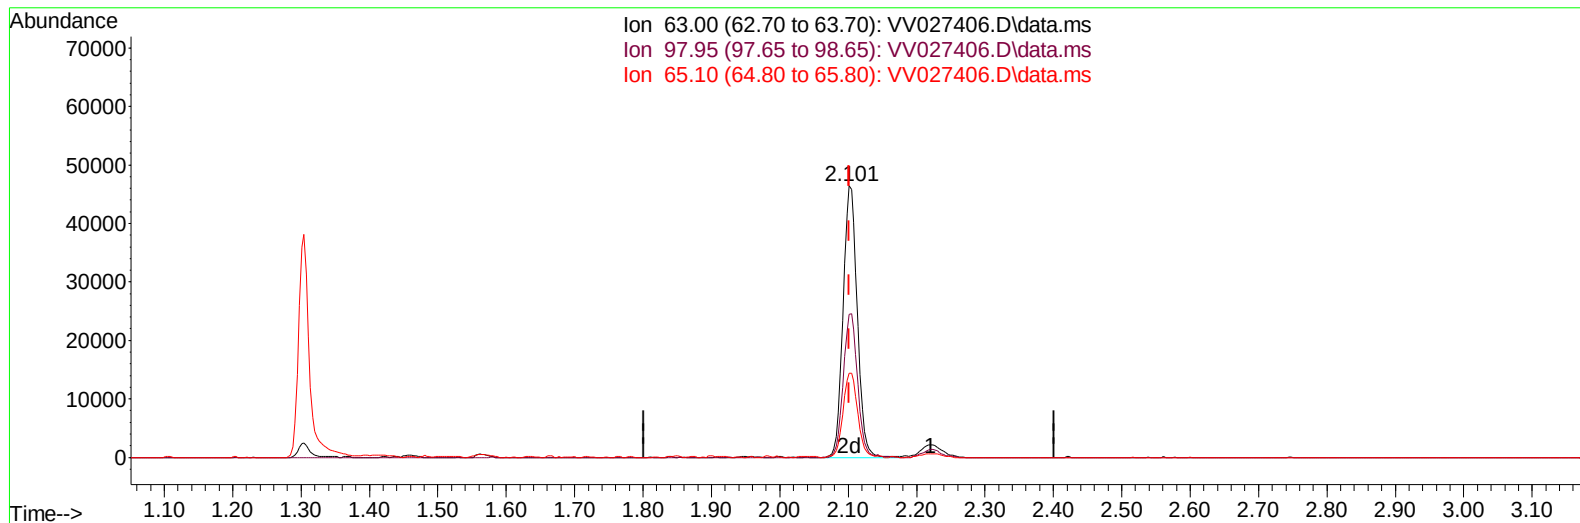

TIC: VV027406.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.101min (+ 0.000) 3.08 ug/L m

response 67005

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	67.40	4.01#
65.10	23.50	2.14#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081622\
 Data File : VV027406.D
 Acq On : 16 Aug 2022 11:55
 Operator : SY/MD
 Sample : N4195-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CZ0

Manual IntegrationsAPPROVED

Quant Time: Aug 17 00:28:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Aug 16 00:24:20 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/19/2022
 Supervised By :Semsettin Yesilyurt 08/22/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.613	114		137890	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		148320	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152		62301	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.304	65		42546	3.551	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	71.000%	
7) Chloroethane-d5	1.561	69		36870	4.238	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	84.800%	
11) 1,1-Dichloroethene-d2	2.101	63		67005m	3.084	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	61.600%	
20) 2-Butanone-d5	3.873	46		116834	57.586	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	115.180%	
24) Chloroform-d	4.342	84		106246	4.836	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	96.800%	
26) 1,2-Dichloroethane-d4	5.027	65		52416	5.008	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	100.200%	
32) Benzene-d6	5.047	84		175741	4.017	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	80.400%	
36) 1,2-Dichloropropane-d6	6.066	67		65652	4.853	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	97.000%	
41) Toluene-d8	7.313	98		140206	3.500	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	70.000%	
43) trans-1,3-Dichloroprop...	7.625	79		19681	4.200	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	84.000%	
46) 2-Hexanone-d5	8.085	63		80015	44.123	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	88.240%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84		46027	4.703	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	94.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152		56205	5.227	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	104.600%	
Target Compounds							
13) Acetone	2.159	43		14183	9.460	ug/L	Qvalue 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081622\
Data File : VV027406.D
Acq On : 16 Aug 2022 11:55
Operator : SY/MD
Sample : N4195-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CZ0

Manual IntegrationsAPPROVED

Quant Time: Aug 17 00:28:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Aug 16 00:24:20 2022
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/19/2022
Supervised By :Semsettin Yesilyurt 08/22/2022

