

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW081622\
 Data File : VW027406.D
 Acq On : 16 Aug 2022 11:55
 Operator : SY/MD
 Sample : N4195-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CZ0

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 08/19/2022
 Supervised By :Semsettin Yesilyurt 08/22/2022

Quant Time: Aug 17 00:28:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Aug 16 00:24:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	137890	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	148320	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	62301	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	42546	3.551	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	71.000%	
7) Chloroethane-d5	1.561	69	36870	4.238	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	84.800%	
11) 1,1-Dichloroethene-d2	2.101	63	67005m	3.084	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	61.600%	
20) 2-Butanone-d5	3.873	46	116834	57.586	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	115.180%	
24) Chloroform-d	4.342	84	106246	4.836	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.800%	
26) 1,2-Dichloroethane-d4	5.027	65	52416	5.008	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.200%	
32) Benzene-d6	5.047	84	175741	4.017	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	80.400%	
36) 1,2-Dichloropropane-d6	6.066	67	65652	4.853	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	97.000%	
41) Toluene-d8	7.313	98	140206	3.500	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	70.000%	
43) trans-1,3-Dichloroprop...	7.625	79	19681	4.200	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	84.000%	
46) 2-Hexanone-d5	8.085	63	80015	44.123	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	88.240%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	46027	4.703	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	94.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	56205	5.227	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	104.600%	
Target Compounds					Qvalue	
13) Acetone	2.159	43	14183	9.460	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081622\
Data File : VV027406.D
Acq On : 16 Aug 2022 11:55
Operator : SY/MD
Sample : N4195-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
C0CZ0

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 08/19/2022
Supervised By :Semsettin Yesilyurt 08/22/2022


Quant Time: Aug 17 00:28:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Aug 16 00:24:20 2022
Response via : Initial Calibration

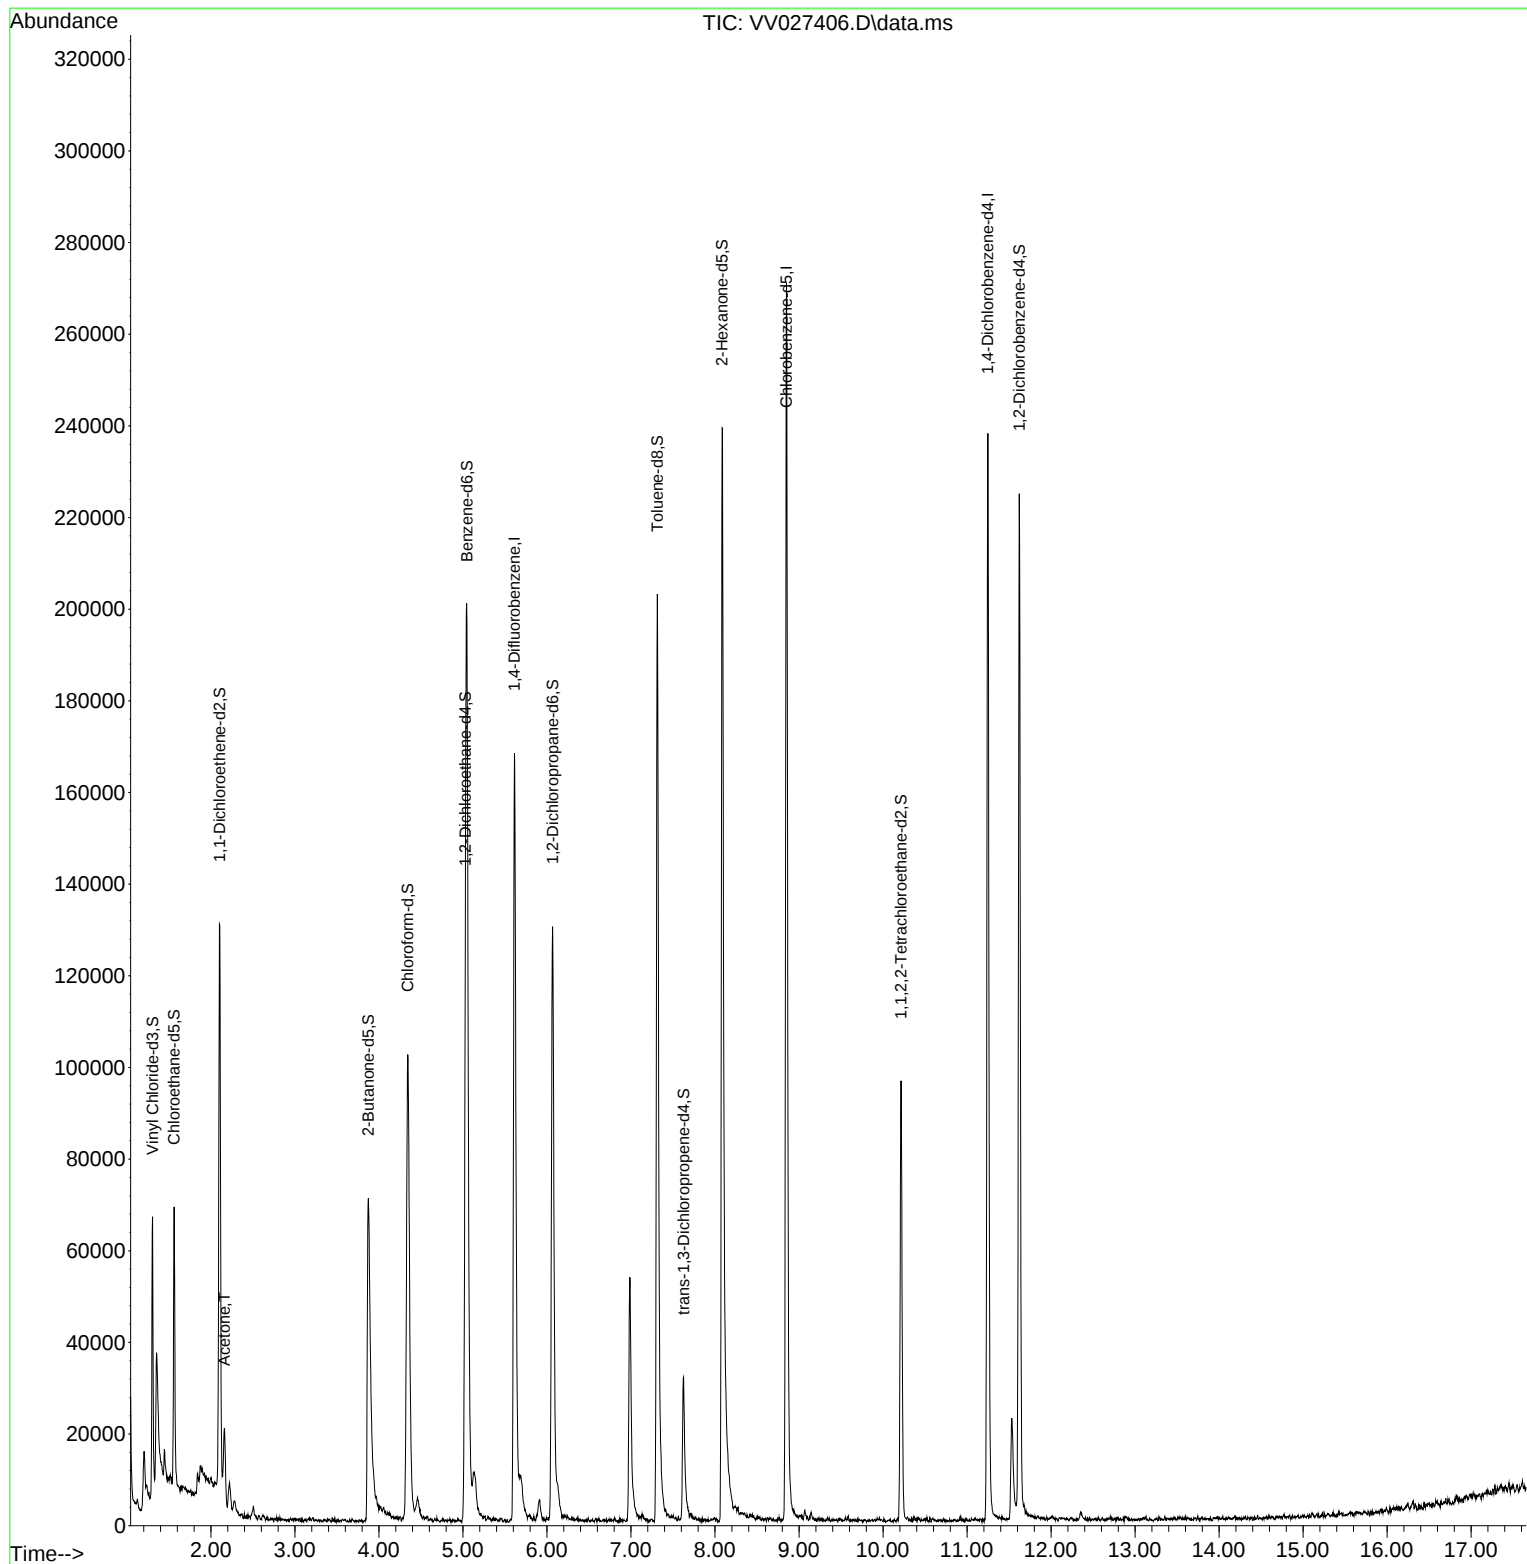

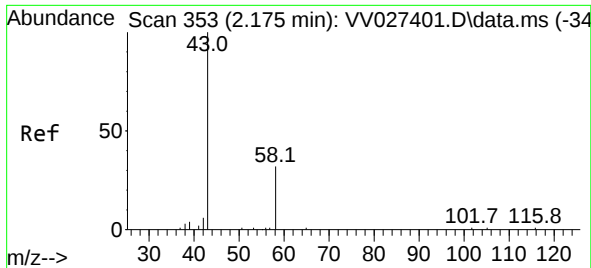

#13
 Acetone
 Concen: 9.460 ug/L
 RT: 2.159 min Scan# 34
 Delta R.T. -0.010 min
 Lab File: VV027406.D
 Acq: 16 Aug 2022 11:55

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CZ0

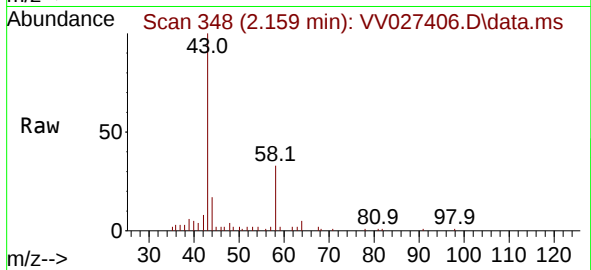

Tgt Ion: 43 Resp: 1418
 Ion Ratio Lower Upper
 43 100
 58 34.7 0.0 63.2

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 08/19/2022
 Supervised By :Semsettin Yesilyurt 08/22/2022

