

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081622\
 Data File : VV027407.D
 Acq On : 16 Aug 2022 12:20
 Operator : SY/MD
 Sample : N4195-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CZ1

Quant Time: Aug 17 00:29:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Aug 16 00:24:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	139193	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	150845	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	62348	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	40652	3.362	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	67.200%	
7) Chloroethane-d5	1.561	69	32708	3.724	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	74.400%	
11) 1,1-Dichloroethene-d2	2.101	63	66866	3.049	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	61.000%	
20) 2-Butanone-d5	3.879	46	118257	57.741	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	115.480%	
24) Chloroform-d	4.342	84	103037	4.646	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.000%	
26) 1,2-Dichloroethane-d4	5.027	65	52906	5.007	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.200%	
32) Benzene-d6	5.043	84	175003	3.933	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	78.600%	
36) 1,2-Dichloropropane-d6	6.066	67	65530	4.763	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	95.200%	
41) Toluene-d8	7.313	98	137776	3.382	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	67.600%#	
43) trans-1,3-Dichloroprop...	7.622	79	20202	4.239	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	84.800%	
46) 2-Hexanone-d5	8.088	63	80030	43.392	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	86.780%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	44992	4.520	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	90.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	53288	4.952	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	99.000%	
Target Compounds					Qvalue	
13) Acetone	2.169	43	11670	7.711	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081622\
Data File : VV027407.D
Acq On : 16 Aug 2022 12:20
Operator : SY/MD
Sample : N4195-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CZ1

Quant Time: Aug 17 00:29:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Aug 16 00:24:20 2022
Response via : Initial Calibration

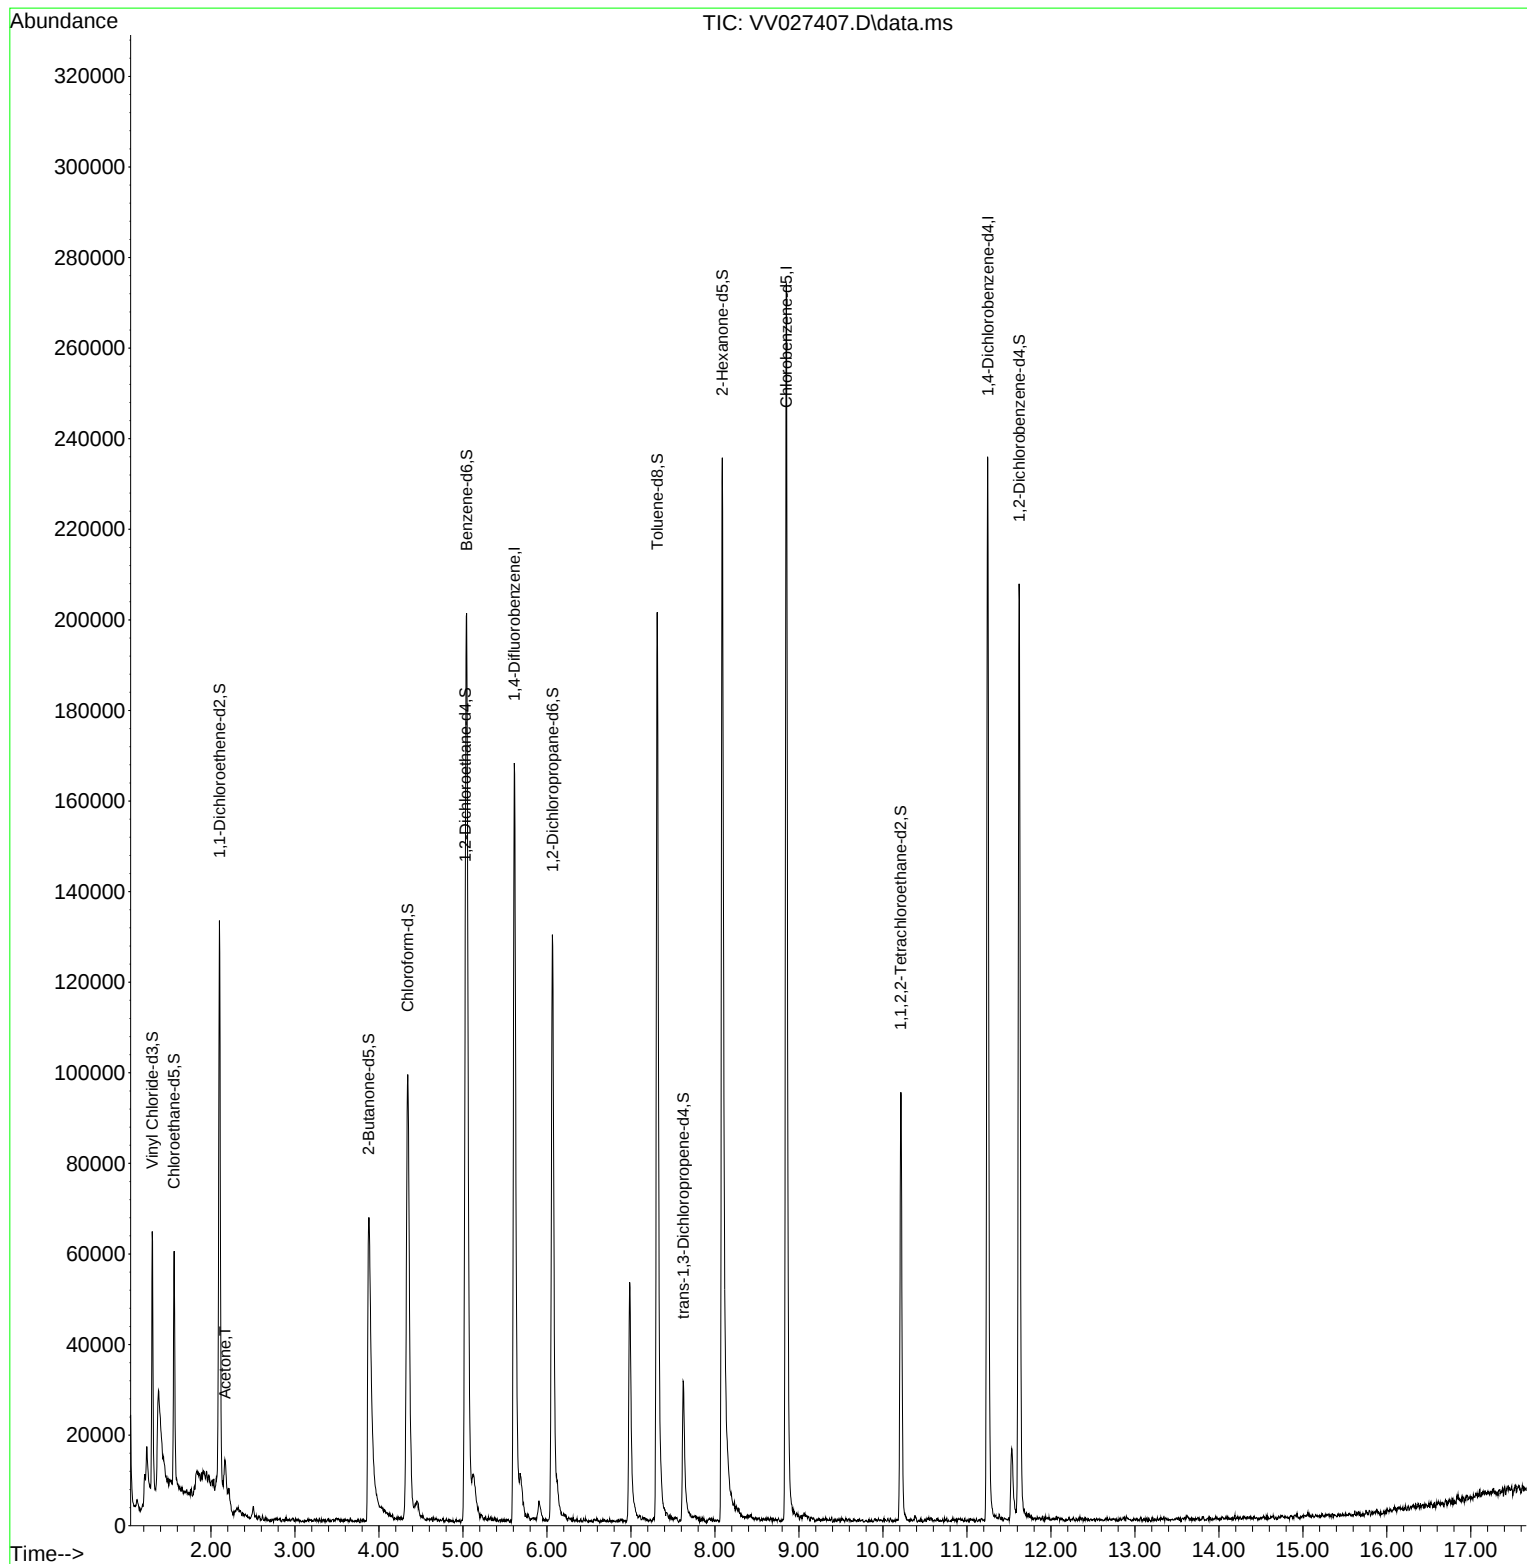

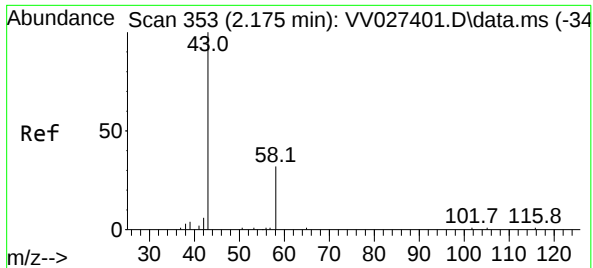

#13
 Acetone
 Concen: 7.711 ug/L
 RT: 2.169 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: VV027407.D
 Acq: 16 Aug 2022 12:20

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CZ1

Tgt Ion: 43 Resp: 11670
 Ion Ratio Lower Upper
 43 100
 58 32.9 0.0 63.2

