

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081622\
 Data File : VV027412.D
 Acq On : 16 Aug 2022 17:14
 Operator : SY/MD
 Sample : VSTDCCC005EC
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 LabSampleId :
 VSTDCCC005EC

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027412.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.127	21	27	37	rBV	144813	144232	11.87%	0.657%
2	1.236	55	61	75	rBV	78780	107120	8.81%	0.488%
3	1.304	75	82	102	rVB2	151765	176422	14.51%	0.804%
4	1.516	141	148	156	rBV	62958	72129	5.93%	0.329%
5	1.564	156	163	164	rBV	54875	49828	4.10%	0.227%
6	1.748	211	220	234	rVB	188051	244301	20.10%	1.114%
7	1.899	257	267	275	rBV3	12957	25007	2.06%	0.114%
8	2.108	320	332	343	rBV4	448644	748925	61.62%	3.414%
9	2.166	344	350	370	rVV	35091	64061	5.27%	0.292%
10	2.288	370	388	403	rVB	160128	276782	22.77%	1.262%
11	2.432	424	433	443	rBV2	14772	25706	2.11%	0.117%
12	2.500	443	454	471	rVB	200958	324987	26.74%	1.481%
13	2.757	519	534	563	rBV2	258337	554959	45.66%	2.529%
14	2.915	574	583	601	rVB5	10117	24794	2.04%	0.113%
15	3.185	651	667	687	rBV	121327	257908	21.22%	1.176%
16	3.902	871	890	903	rBV3	141014	425360	35.00%	1.939%
17	4.243	983	996	1014	rBV2	75574	183818	15.12%	0.838%
18	4.362	1014	1033	1057	rVB4	163502	564396	46.43%	2.572%
19	4.603	1092	1108	1118	rBV3	133324	332993	27.40%	1.518%
20	4.670	1119	1129	1154	rVB2	167964	425256	34.99%	1.938%
21	4.821	1159	1176	1197	rVB2	129460	324531	26.70%	1.479%
22	4.940	1203	1213	1226	rVB5	6262	14819	1.22%	0.068%
23	5.043	1229	1245	1253	rBV2	218023	525141	43.20%	2.394%
24	5.095	1254	1261	1289	rVB2	247836	678373	55.81%	3.092%
25	5.612	1410	1422	1443	rBV	174820	365611	30.08%	1.666%
26	5.702	1445	1450	1472	rVB3	9664	23911	1.97%	0.109%
27	5.911	1500	1515	1532	rBV	176879	359901	29.61%	1.640%
28	6.066	1550	1563	1572	rBV2	133115	267221	21.98%	1.218%
29	6.127	1572	1582	1589	rVV2	234553	485319	39.93%	2.212%
30	6.169	1590	1595	1615	rVB	169880	330755	27.21%	1.508%
31	6.506	1686	1700	1714	rBV	123136	241794	19.89%	1.102%
32	6.985	1835	1849	1854	rBV	61907	99711	8.20%	0.454%
33	7.027	1855	1862	1887	rVB	127469	248397	20.44%	1.132%
34	7.227	1911	1924	1942	rBV	424958	897967	73.88%	4.093%
35	7.313	1942	1951	1963	rVV	269256	495835	40.79%	2.260%
36	7.384	1963	1973	2000	rVB	379355	701446	57.71%	3.197%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081622\
 Data File : VV027412.D
 Acq On : 16 Aug 2022 17:14
 Operator : SY/MD
 Sample : VSTDCCC005EC
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 LabSampleId :
 VSTDCCC005EC

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Title : TRACE VOA SFAM1.0

37	7.651	2038	2056	2078	rBV3	119379	294120	24.20%	1.341%
38	7.837	2101	2114	2134	rBV	142870	263265	21.66%	1.200%
39	7.972	2144	2156	2182	rVB	235067	416868	34.30%	1.900%
40	8.088	2182	2192	2200	rBV	279930	521947	42.94%	2.379%
41	8.140	2201	2208	2229	rVV	348280	722253	59.42%	3.292%
42	8.243	2231	2240	2263	rVB	104987	202680	16.67%	0.924%
43	8.352	2263	2274	2291	rBV	56099	104860	8.63%	0.478%
44	8.850	2418	2429	2433	rBV	301637	447294	36.80%	2.039%
45	9.011	2468	2479	2497	rBV	397712	637431	52.44%	2.905%
46	9.136	2507	2518	2540	rBV	383851	643108	52.91%	2.931%
47	9.551	2629	2647	2669	rBV4	534046	1215480	100.00%	5.540%
48	9.731	2692	2703	2726	rVB2	59725	108181	8.90%	0.493%
49	9.931	2753	2765	2787	rBV	453394	713036	58.66%	3.250%
50	10.217	2840	2854	2857	rBV	121601	181440	14.93%	0.827%
51	10.271	2867	2871	2885	rVB	92445	139101	11.44%	0.634%
52	10.538	2939	2954	2974	rBV	134587	214170	17.62%	0.976%
53	10.914	3060	3071	3087	rBV	384089	591240	48.64%	2.695%
54	11.178	3142	3153	3165	rBV	347193	544576	44.80%	2.482%
55	11.249	3165	3175	3178	rBV	357572	519099	42.71%	2.366%
56	11.635	3278	3295	3322	rBV2	390480	931938	76.67%	4.248%
57	12.429	3532	3542	3552	rBV3	30476	48885	4.02%	0.223%
58	12.644	3598	3609	3624	rBV	320884	497225	40.91%	2.266%
59	13.258	3788	3800	3816	rBV	232421	360562	29.66%	1.643%
60	13.500	3860	3875	3893	rBV	117353	194776	16.02%	0.888%
61	13.741	3938	3950	3964	rBV	217622	336503	27.68%	1.534%




Sum of corrected areas: 21939754

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081622\
Data File : VV027412.D
Acq On : 16 Aug 2022 17:14
Operator : SY/MD
Sample : VSTDCCC005EC
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
LabSampleId :
VSTDCCC005EC

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

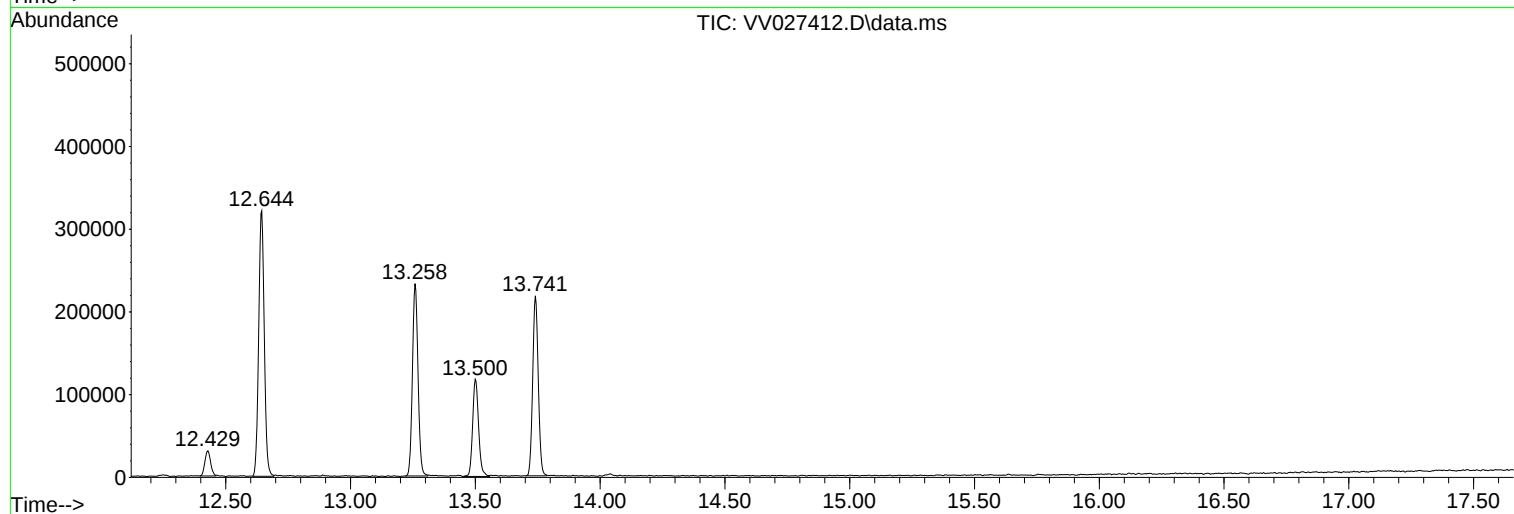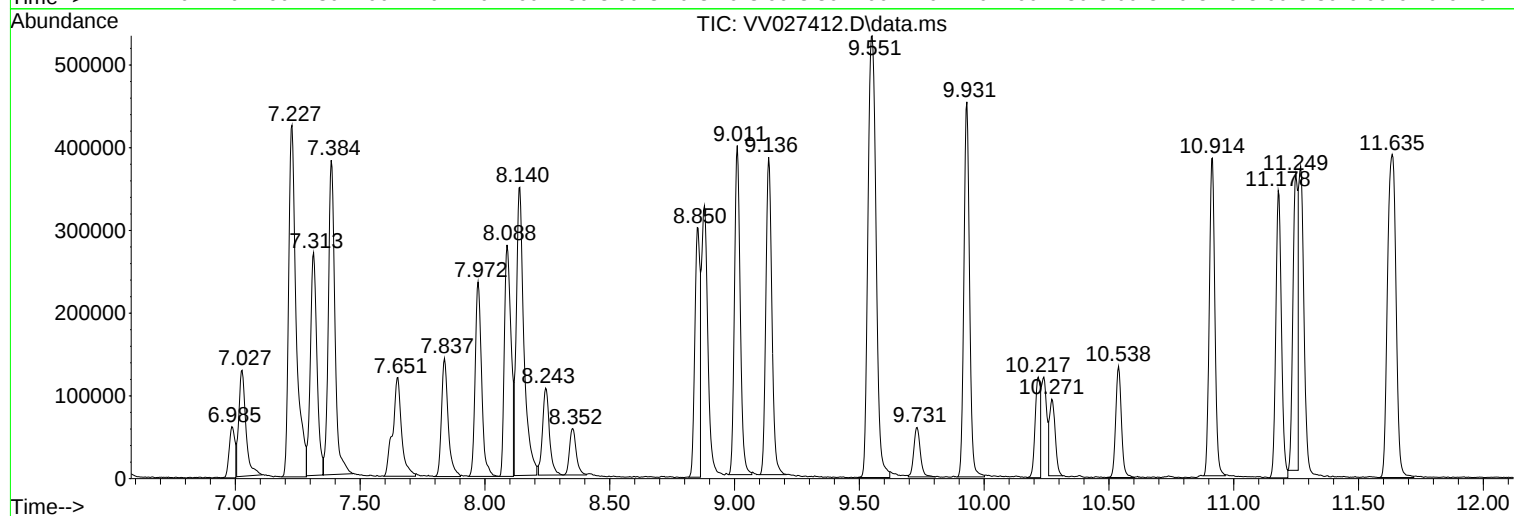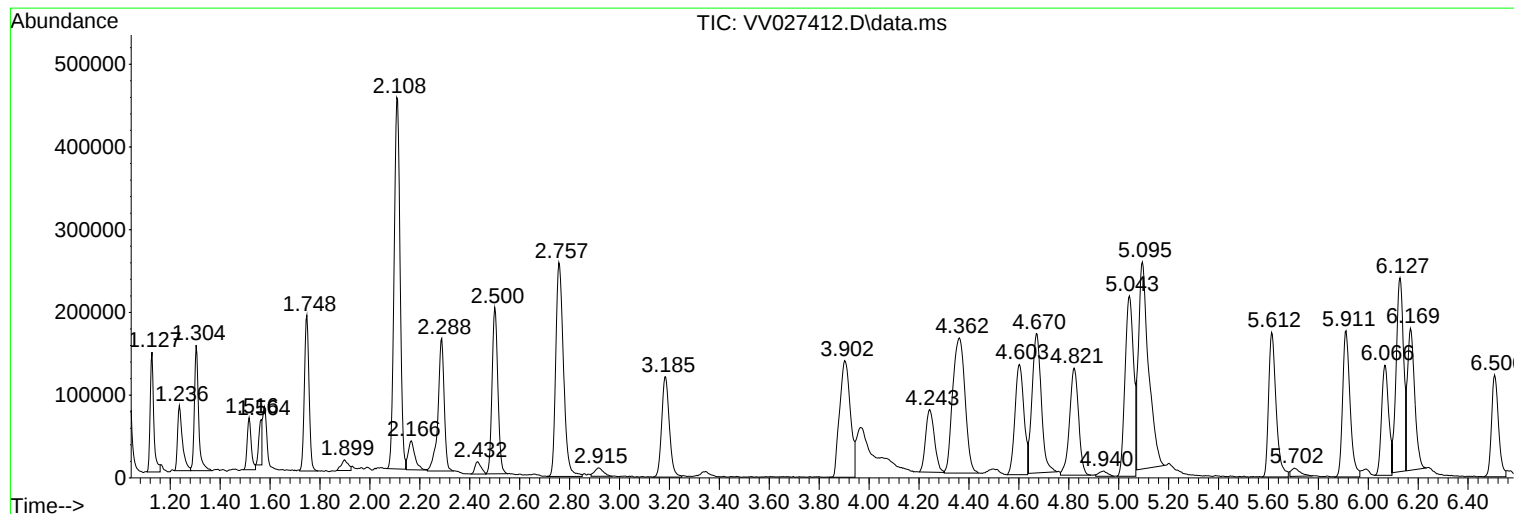

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081622\
Data File : VV027412.D
Acq On : 16 Aug 2022 17:14
Operator : SY/MD
Sample : VSTDCCC005EC
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
LabSampleId :
VSTDCCC005EC

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081622\
Data File : VV027412.D
Acq On : 16 Aug 2022 17:14
Operator : SY/MD
Sample : VSTDCCC005EC
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
LabSampleId :
VSTDCCC005EC

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc