
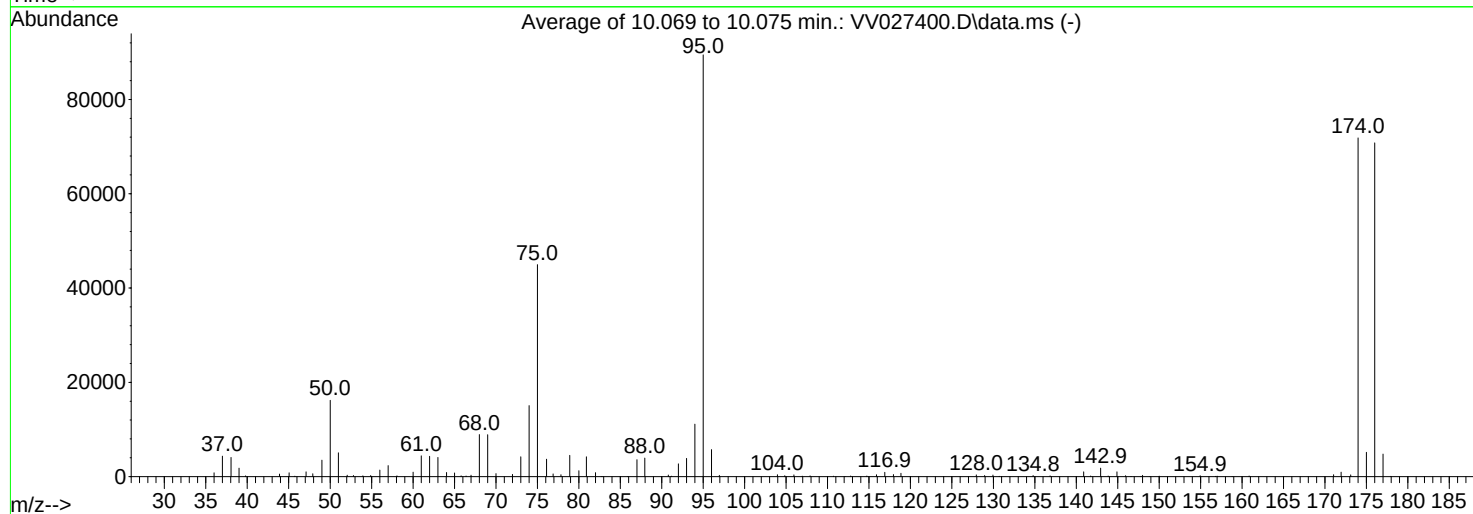


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081622\
 Data File : VV027400.D
 Acq On : 16 Aug 2022 08:22
 Operator : SY/MD
 Sample : BFB354
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB354

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Aug 16 00:24:20 2022

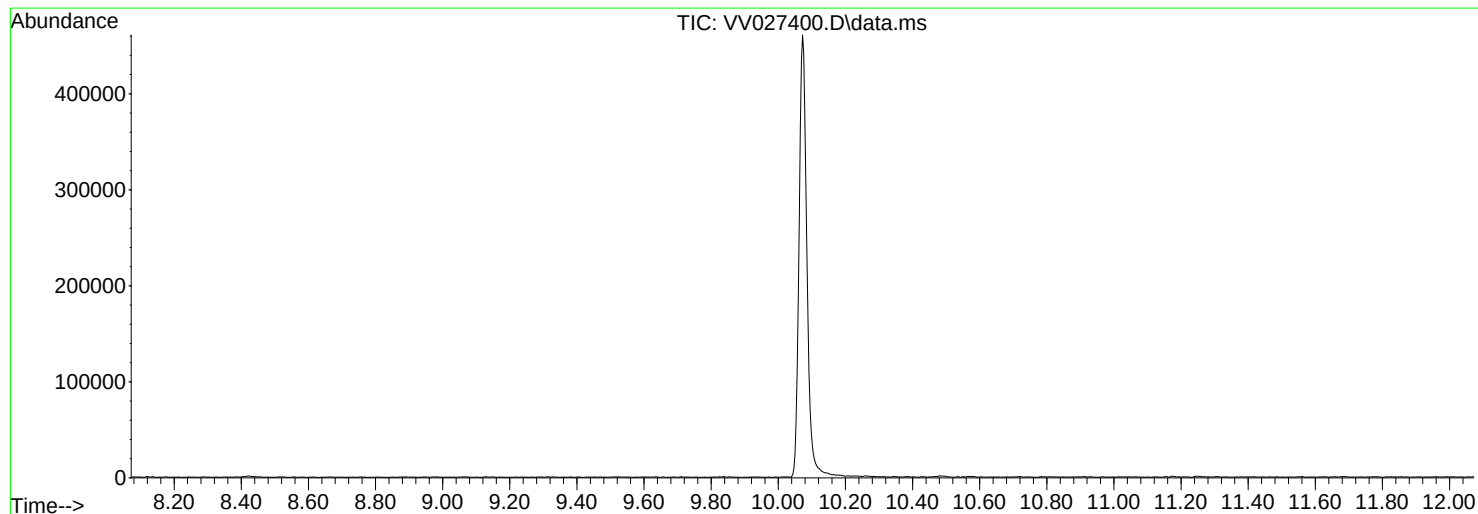

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	16199	PASS
75	95	30	80	50.3	44963	PASS
95	95	100	100	100.0	89464	PASS
96	95	5	9	6.4	5740	PASS
173	174	0.00	2	0.5	373	PASS
174	95	50	120	80.3	71845	PASS
175	174	5	9	7.2	5174	PASS
176	174	95	105	98.5	70789	PASS
177	176	5	10	6.8	4791	PASS

m/z	Abundance
37.60	104.0
40.10	334.0
42.70	109.0
43.90	309.0
45.70	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB354

m/z	Abundance
35.90	842.0
37.00	4396.0
38.00	3973.0
39.00	1724.0
39.80	469.0
44.00	806.0
45.10	758.0
45.90	205.0
47.10	960.0
47.90	619.0
49.00	3534.0
50.00	15898.0
51.00	5174.0
52.00	281.0
52.80	213.0
53.90	129.0
54.90	252.0
56.00	1516.0
57.00	2447.0
58.10	139.0
60.00	979.0
61.00	4565.0
62.00	4174.0
63.00	3866.0
64.10	890.0
65.00	714.0
65.80	153.0
66.40	142.0
67.00	305.0
68.00	8651.0
69.00	8866.0
70.00	620.0
72.00	477.0
73.00	4167.0
74.00	15236.0
75.00	44160.0
76.10	3588.0
76.90	576.0
77.80	353.0
78.90	4332.0
80.00	1094.0
80.90	3938.0
82.00	775.0
82.70	135.0
85.90	118.0
87.00	3718.0
87.90	4113.0
90.80	345.0
92.00	2548.0
93.00	3788.0
94.00	10726.0
95.00	87984.0
96.00	5796.0
97.00	281.0
103.90	412.0
104.90	173.0
105.90	402.0
107.90	130.0
110.70	115.0
112.10	102.0
112.90	144.0
114.70	107.0
115.90	449.0
116.80	865.0
118.00	373.0
118.80	642.0
128.00	367.0
129.00	232.0
129.90	335.0
130.70	133.0
134.80	221.0
136.80	179.0
140.90	1034.0
141.80	191.0
142.90	1714.0
143.80	141.0
144.90	913.0
145.90	223.0
147.80	238.0
148.00	244.0
150.00	114.0
155.00	215.0
156.80	157.0
160.80	110.0
171.00	406.0
171.90	895.0
174.00	67600.0
175.00	5086.0
176.00	67416.0
177.00	4545.0
178.00	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB354

m/z	Abundance
36.00	828.0
37.00	4481.0
38.10	4216.0
39.00	1906.0
40.20	332.0
44.00	825.0
45.00	840.0
45.80	211.0
47.10	1064.0
47.90	653.0
49.00	3632.0
50.00	16808.0
51.00	5268.0
52.00	332.0
52.80	239.0
54.00	177.0
54.90	249.0
56.00	1465.0
57.00	2401.0
58.10	165.0
60.00	956.0
61.00	4577.0
62.00	4418.0
63.00	4173.0
64.10	871.0
65.00	794.0
65.80	190.0
66.40	132.0
67.00	301.0
68.00	9183.0
69.00	9244.0
70.00	680.0
72.00	487.0
73.00	4349.0
74.00	15582.0
75.00	46560.0
76.10	3786.0
76.90	576.0
77.80	416.0
78.90	4641.0
80.00	1301.0
80.90	4391.0
82.00	876.0
82.90	113.0
87.00	3641.0
88.00	4062.0
90.80	349.0
91.20	269.0
92.00	2761.0
93.00	4051.0
94.00	11546.0
95.00	92576.0
96.00	5978.0
97.00	264.0
104.00	426.0
104.90	205.0
105.90	397.0
107.00	118.0
107.90	169.0
110.70	116.0
112.80	121.0
114.80	127.0
115.90	450.0
116.90	967.0
117.90	473.0
118.90	708.0
128.00	387.0
128.90	231.0
130.00	349.0
130.70	128.0
134.80	258.0
136.80	197.0
140.90	1050.0
141.70	182.0
143.00	1814.0
143.90	156.0
144.90	1082.0
146.00	221.0
146.60	102.0
148.00	271.0
148.90	100.0
150.00	110.0
154.90	221.0
157.00	148.0
160.90	120.0
171.00	435.0
171.90	1001.0
174.00	74488.0
175.00	5278.0
176.00	73336.0
177.00	5002.0
177.90	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB354

m/z	Abundance
36.10	791.0
37.00	4144.0
38.10	4052.0
39.00	1827.0
40.30	358.0
43.90	881.0
45.00	838.0
45.80	209.0
47.10	1027.0
47.90	605.0
49.00	3342.0
50.00	15890.0
51.00	4694.0
52.10	334.0
52.80	225.0
54.00	181.0
54.90	235.0
56.00	1201.0
57.00	2139.0
58.00	169.0
60.00	895.0
61.00	4116.0
62.00	4322.0
63.00	4203.0
64.00	874.0
65.00	807.0
65.80	198.0
66.40	103.0
67.00	279.0
68.00	8926.0
69.00	8612.0
70.00	674.0
72.00	497.0
73.00	4102.0
74.00	14391.0
75.00	44168.0
76.10	3689.0
76.90	591.0
77.90	512.0
78.90	4527.0
80.00	1363.0
80.90	4326.0
82.00	900.0
87.00	3483.0
88.00	3656.0
90.80	323.0
92.00	2818.0
93.00	3823.0
94.00	11091.0
95.00	87832.0
96.00	5446.0
96.90	237.0
104.00	411.0
104.80	191.0
106.00	346.0
106.90	171.0
107.90	189.0
110.70	106.0
112.70	115.0
114.80	160.0
115.90	369.0
117.00	931.0
117.90	507.0
118.90	756.0
124.00	110.0
127.90	361.0
128.90	209.0
129.90	339.0
131.00	126.0
134.80	235.0
136.90	172.0
140.90	967.0
143.00	1833.0
143.90	155.0
144.90	1112.0
146.00	179.0
148.00	256.0
150.00	107.0
154.90	209.0
157.00	121.0
158.80	108.0
160.90	133.0
171.10	412.0
172.00	946.0
173.10	1118.0
174.00	73448.0
175.00	5157.0
176.00	71616.0
177.00	4827.0

Instrument :
MSVOA_V
ClientSampleId :
BFB354