

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081623\
 Data File : VV031818.D
 Acq On : 16 Aug 2023 13:26
 Operator : SY/MD
 Sample : VV0816WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK378

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

Signal : TIC: VV031818.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	328835	349936	16.23%	2.357%
2	1.532	146	153	166	rVB	268206	322001	14.94%	2.169%
3	2.060	308	317	334	rBV	514450	741675	34.41%	4.995%
4	2.381	415	417	421	rBV4	1569	1114	0.05%	0.008%
5	2.503	453	455	464	rVB5	1978	2110	0.10%	0.014%
6	2.774	537	539	542	rVB4	1273	731	0.03%	0.005%
7	2.796	542	546	548	rBV4	1304	1016	0.05%	0.007%
8	2.870	565	569	571	rBV4	1980	1135	0.05%	0.008%
9	2.944	588	592	596	rVB6	1224	1181	0.05%	0.008%
10	2.970	596	600	603	rBV4	971	851	0.04%	0.006%
11	3.021	614	616	621	rVB3	1339	921	0.04%	0.006%
12	3.047	621	624	628	rBV5	939	791	0.04%	0.005%
13	3.079	632	634	638	rVB3	1171	563	0.03%	0.004%
14	3.108	638	643	644	rBV3	1154	890	0.04%	0.006%
15	3.204	671	673	681	rVB5	1169	1245	0.06%	0.008%
16	3.240	681	684	688	rBV5	1115	760	0.04%	0.005%
17	3.330	710	712	718	rVB4	914	727	0.03%	0.005%
18	3.388	725	730	736	rVB7	1415	1826	0.08%	0.012%
19	3.503	763	766	767	rBV2	873	549	0.03%	0.004%
20	3.532	774	775	779	rVB3	1342	644	0.03%	0.004%
21	3.568	783	786	789	rBV2	984	611	0.03%	0.004%
22	3.597	793	795	797	rVB2	1163	580	0.03%	0.004%
23	3.616	797	801	803	rBV2	1588	929	0.04%	0.006%
24	3.667	816	817	821	rVV3	1102	653	0.03%	0.004%
25	3.687	821	823	828	rVB3	1180	848	0.04%	0.006%
26	3.725	833	835	838	rBV4	1007	484	0.02%	0.003%
27	3.793	846	856	881	rBV2	133373	362870	16.83%	2.444%
28	4.256	983	1000	1027	rBV	344346	902127	41.85%	6.076%
29	4.526	1082	1084	1088	rBV4	1486	1362	0.06%	0.009%
30	4.661	1124	1126	1127	rBV2	1409	620	0.03%	0.004%
31	4.783	1161	1164	1168	rVB3	1080	770	0.04%	0.005%
32	4.806	1168	1171	1172	rBV2	1544	788	0.04%	0.005%
33	4.960	1203	1219	1249	rBV2	812876	2155609	100.00%	14.519%
34	5.539	1387	1399	1422	rBV	462879	973627	45.17%	6.558%
35	5.831	1480	1490	1505	rBV2	45223	93504	4.34%	0.630%
36	5.995	1528	1541	1562	rBV	467236	982984	45.60%	6.621%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081623\
 Data File : VV031818.D
 Acq On : 16 Aug 2023 13:26
 Operator : SY/MD
 Sample : VV0816WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK378

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

37	6.407	1665	1669	1670	rBV3	849	511	0.02%	0.003%
38	6.416	1670	1672	1676	rBV5	1502	940	0.04%	0.006%
39	6.484	1690	1693	1697	rBV5	1324	1107	0.05%	0.007%
40	6.574	1718	1721	1723	rBV4	1381	935	0.04%	0.006%
41	6.600	1727	1729	1733	rBV5	1408	930	0.04%	0.006%
42	6.670	1749	1751	1754	rBV4	932	516	0.02%	0.003%
43	6.738	1770	1772	1776	rBV4	771	578	0.03%	0.004%
44	6.828	1797	1800	1802	rBV3	908	590	0.03%	0.004%
45	6.870	1810	1813	1815	rBV3	999	646	0.03%	0.004%
46	6.918	1816	1828	1847	rBV	231731	434472	20.16%	2.926%
47	7.249	1920	1931	1966	rBV	892588	1583271	73.45%	10.664%
48	7.558	2017	2027	2053	rBV2	168131	316982	14.70%	2.135%
49	7.822	2106	2109	2111	rBV4	1258	725	0.03%	0.005%
50	8.031	2165	2174	2220	rBV	273737	598734	27.78%	4.033%
51	8.436	2295	2300	2302	rBV7	1609	1432	0.07%	0.010%
52	8.641	2362	2364	2368	rVB4	1845	1012	0.05%	0.007%
53	8.686	2374	2378	2381	rBV5	1194	976	0.05%	0.007%
54	8.744	2394	2396	2398	rBV2	1565	731	0.03%	0.005%
55	8.789	2398	2410	2430	rBV	761415	1247201	57.86%	8.400%
56	9.223	2541	2545	2549	rVB5	1368	1274	0.06%	0.009%
57	9.246	2550	2552	2556	rVB4	1384	806	0.04%	0.005%
58	9.268	2557	2559	2562	rBV4	1410	775	0.04%	0.005%
59	9.349	2577	2584	2588	rBV6	2002	2486	0.12%	0.017%
60	9.471	2619	2622	2624	rBV2	962	585	0.03%	0.004%
61	9.497	2624	2630	2633	rBV6	2263	2956	0.14%	0.020%
62	9.580	2653	2656	2657	rBV3	843	451	0.02%	0.003%
63	9.677	2683	2686	2691	rBV5	1258	1004	0.05%	0.007%
64	9.715	2694	2698	2699	rBV4	989	576	0.03%	0.004%
65	9.879	2742	2749	2752	rBV6	2994	3175	0.15%	0.021%
66	9.915	2758	2760	2771	rVB9	1900	1961	0.09%	0.013%
67	9.960	2771	2774	2775	rBV4	1191	605	0.03%	0.004%
68	10.088	2811	2814	2816	rBV3	1239	825	0.04%	0.006%
69	10.156	2824	2835	2855	rBV	610264	978625	45.40%	6.591%
70	10.288	2873	2876	2878	rBV4	1326	884	0.04%	0.006%
71	10.323	2883	2887	2888	rBV2	1642	1095	0.05%	0.007%
72	10.583	2964	2968	2970	rVB4	1324	976	0.05%	0.007%
73	10.600	2970	2973	2976	rBV3	1491	1253	0.06%	0.008%
74	10.661	2990	2992	2995	rVB4	1369	626	0.03%	0.004%
75	10.844	3044	3049	3051	rBV4	1873	1992	0.09%	0.013%
76	10.973	3085	3089	3093	rBV3	1305	1135	0.05%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081623\
 Data File : VV031818.D
 Acq On : 16 Aug 2023 13:26
 Operator : SY/MD
 Sample : VV0816WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK378

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

77	10.998	3093	3097	3100	rVB4	1467	1083	0.05%	0.007%
78	11.027	3100	3106	3109	rBV7	1314	1457	0.07%	0.010%
79	11.092	3122	3126	3129	rBV3	1222	867	0.04%	0.006%
80	11.117	3129	3134	3136	rBV5	3774	3490	0.16%	0.024%
81	11.191	3146	3157	3182	rBV	773700	1208283	56.05%	8.138%
82	11.384	3212	3217	3219	rBV3	1532	1255	0.06%	0.008%
83	11.493	3249	3251	3254	rVB3	1763	950	0.04%	0.006%
84	11.567	3262	3274	3294	rBV	915016	1443144	66.95%	9.720%
85	11.834	3354	3357	3358	rBV3	1074	506	0.02%	0.003%
86	11.960	3393	3396	3398	rBV4	1559	1028	0.05%	0.007%
87	12.108	3439	3442	3447	rBV6	1139	837	0.04%	0.006%
88	12.159	3456	3458	3461	rBV4	1303	783	0.04%	0.005%
89	12.281	3492	3496	3498	rBV5	901	744	0.03%	0.005%
90	12.432	3539	3543	3545	rBV5	1140	941	0.04%	0.006%
91	12.590	3585	3592	3603	rBV5	5662	9794	0.45%	0.066%
92	12.632	3603	3605	3609	rBV4	1110	748	0.03%	0.005%
93	13.165	3768	3771	3773	rBV3	1569	1047	0.05%	0.007%
94	13.214	3777	3786	3793	rBV9	8278	13981	0.65%	0.094%
95	13.448	3851	3859	3875	rVB2	18066	29993	1.39%	0.202%
96	13.580	3898	3900	3902	rBV3	1615	644	0.03%	0.004%
97	13.628	3913	3915	3918	rBV3	1119	646	0.03%	0.004%
98	13.686	3926	3933	3944	rVB9	9652	16086	0.75%	0.108%
99	14.397	4152	4154	4157	rBV4	1765	1225	0.06%	0.008%
100	14.792	4272	4277	4279	rBV3	2690	2394	0.11%	0.016%




Sum of corrected areas: 14847312

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081623\
Data File : VV031818.D
Acq On : 16 Aug 2023 13:26
Operator : SY/MD
Sample : VV0816WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK378

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

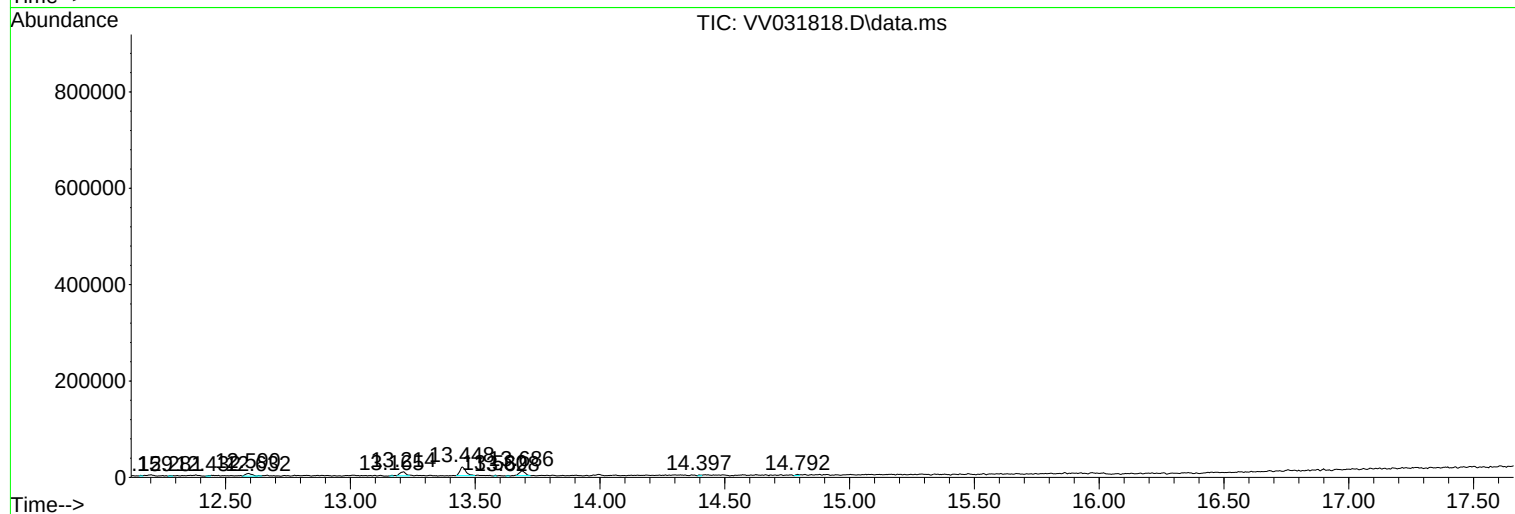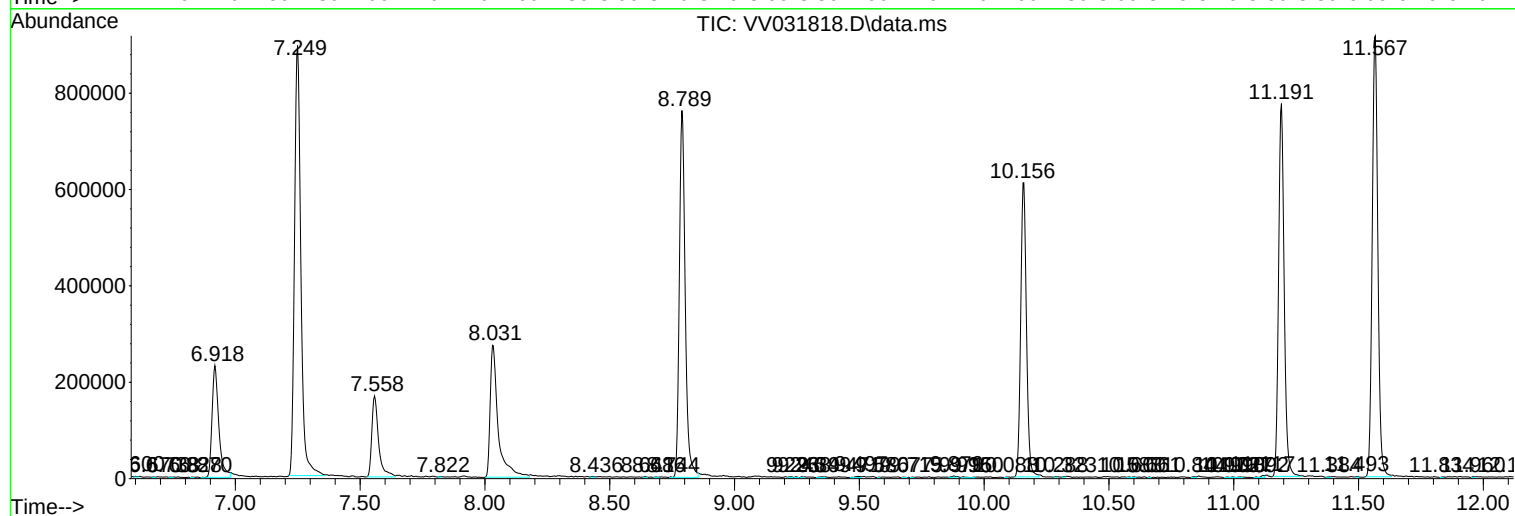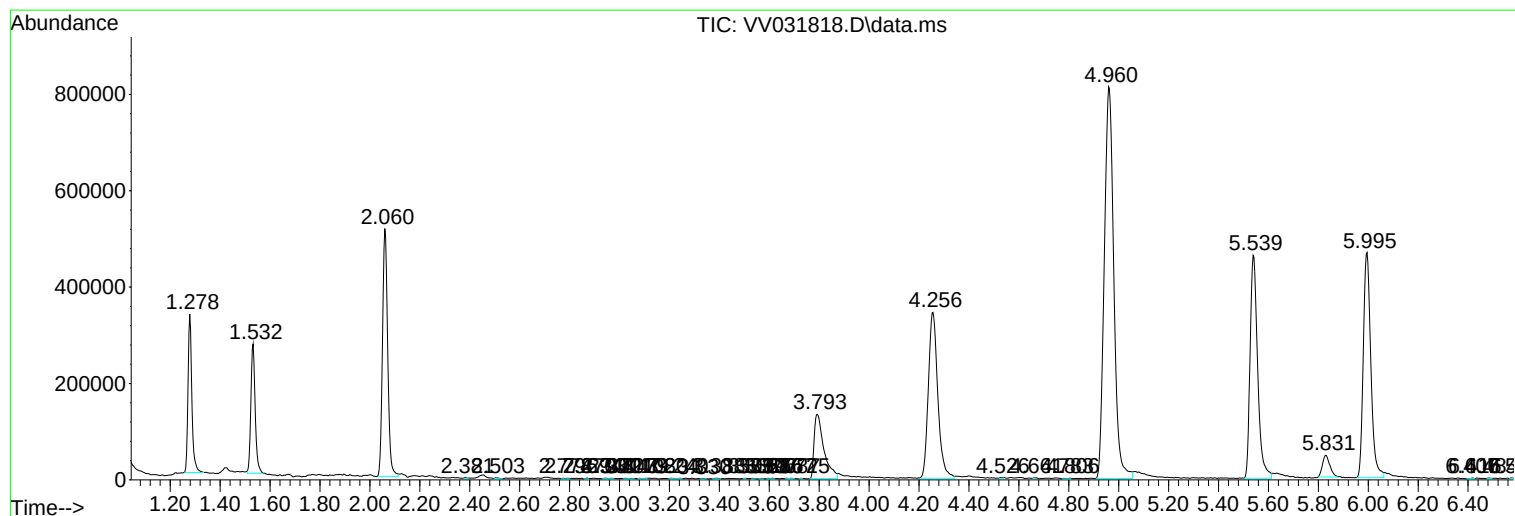

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081623\
Data File : VV031818.D
Acq On : 16 Aug 2023 13:26
Operator : SY/MD
Sample : VV0816WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK378

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081623\
Data File : VV031818.D
Acq On : 16 Aug 2023 13:26
Operator : SY/MD
Sample : VV0816WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK378

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------