

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081623\
 Data File : VV031819.D
 Acq On : 16 Aug 2023 13:50
 Operator : SY/MD
 Sample : 03965-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

Signal : TIC: VV031819.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	318885	339092	15.91%	2.351%
2	1.532	146	153	168	rVB	272013	331042	15.54%	2.296%
3	2.060	308	317	330	rVB	518958	729410	34.23%	5.058%
4	2.805	545	549	551	rBV4	1326	1097	0.05%	0.008%
5	2.931	585	588	589	rBV	796	356	0.02%	0.002%
6	2.969	598	600	602	rVB3	963	453	0.02%	0.003%
7	2.989	604	606	609	rVB4	1141	676	0.03%	0.005%
8	3.088	633	637	638	rBV3	833	508	0.02%	0.004%
9	3.127	646	649	652	rVB5	1439	921	0.04%	0.006%
10	3.182	665	666	667	rBV	506	156	0.01%	0.001%
11	3.246	684	686	688	rBV2	1231	627	0.03%	0.004%
12	3.275	693	695	697	rVV3	1016	412	0.02%	0.003%
13	3.288	697	699	701	rVB3	926	331	0.02%	0.002%
14	3.304	701	704	709	rVB5	1069	845	0.04%	0.006%
15	3.326	709	711	712	rBV2	708	198	0.01%	0.001%
16	3.339	712	715	716	rBV3	734	426	0.02%	0.003%
17	3.362	719	722	724	rVB4	1272	526	0.02%	0.004%
18	3.400	730	734	735	rBV4	1235	746	0.04%	0.005%
19	3.436	742	745	747	rVB4	897	511	0.02%	0.004%
20	3.449	747	749	752	rBV3	903	460	0.02%	0.003%
21	3.516	768	770	772	rVB3	1036	369	0.02%	0.003%
22	3.529	772	774	776	rVB3	628	273	0.01%	0.002%
23	3.558	780	783	784	rBV2	1037	577	0.03%	0.004%
24	3.590	792	793	794	rBV	520	147	0.01%	0.001%
25	3.632	804	806	807	rBV	500	186	0.01%	0.001%
26	3.680	819	821	824	rBV2	1228	632	0.03%	0.004%
27	3.735	837	838	840	rVB2	685	210	0.01%	0.001%
28	3.748	840	842	843	rBV2	1068	410	0.02%	0.003%
29	3.793	847	856	888	rBV2	138352	376393	17.66%	2.610%
30	4.256	986	1000	1029	rVB	338354	859114	40.32%	5.958%
31	4.571	1096	1098	1101	rBV3	1700	1186	0.06%	0.008%
32	4.674	1127	1130	1132	rVB2	911	542	0.03%	0.004%
33	4.963	1203	1220	1247	rBV2	792403	2130939	100.00%	14.777%
34	5.426	1362	1364	1368	rBV3	1455	688	0.03%	0.005%
35	5.542	1388	1400	1426	rBV	436321	924671	43.39%	6.412%
36	5.831	1481	1490	1507	rVB3	47967	98425	4.62%	0.683%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081623\
 Data File : VV031819.D
 Acq On : 16 Aug 2023 13:50
 Operator : SY/MD
 Sample : 03965-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

37	5.995	1529	1541	1562	rBV	472056	967614	45.41%	6.710%
38	6.249	1617	1620	1622	rBV3	1537	1040	0.05%	0.007%
39	6.841	1800	1804	1807	rVB5	1383	815	0.04%	0.006%
40	6.870	1811	1813	1817	rBV3	1175	1131	0.05%	0.008%
41	6.918	1817	1828	1851	rBV	220371	427319	20.05%	2.963%
42	7.249	1920	1931	1955	rBV	860535	1532682	71.93%	10.629%
43	7.558	2018	2027	2049	rBV	164028	298566	14.01%	2.070%
44	8.034	2165	2175	2212	rBV	275771	584932	27.45%	4.056%
45	8.789	2399	2410	2434	rBV	709310	1192572	55.96%	8.270%
46	9.435	2607	2611	2615	rBV3	860	664	0.03%	0.005%
47	9.458	2615	2618	2620	rBV3	1067	787	0.04%	0.005%
48	9.487	2622	2627	2629	rBV5	2018	1917	0.09%	0.013%
49	9.567	2650	2652	2656	rBV5	1446	1081	0.05%	0.007%
50	9.625	2668	2670	2673	rBV4	810	538	0.03%	0.004%
51	9.712	2695	2697	2702	rBV4	1043	845	0.04%	0.006%
52	9.744	2704	2707	2710	rBV4	1518	1337	0.06%	0.009%
53	9.789	2717	2721	2724	rBV7	1170	1222	0.06%	0.008%
54	9.863	2737	2744	2747	rBV5	1495	2245	0.11%	0.016%
55	9.882	2747	2750	2751	rVV2	1433	669	0.03%	0.005%
56	9.956	2769	2773	2775	rBV3	980	690	0.03%	0.005%
57	10.075	2806	2810	2811	rBV3	1429	868	0.04%	0.006%
58	10.159	2824	2836	2859	rBV	607045	974079	45.71%	6.755%
59	10.307	2880	2882	2884	rBV3	1391	824	0.04%	0.006%
60	10.394	2906	2909	2913	rBV3	1002	718	0.03%	0.005%
61	10.490	2931	2939	2943	rBV9	2772	3781	0.18%	0.026%
62	10.558	2958	2960	2963	rBV2	871	533	0.03%	0.004%
63	10.606	2973	2975	2977	rBV3	1291	446	0.02%	0.003%
64	10.660	2989	2992	2994	rBV5	844	493	0.02%	0.003%
65	10.673	2994	2996	2998	rVB2	818	312	0.01%	0.002%
66	10.686	2998	3000	3002	rBV2	914	548	0.03%	0.004%
67	10.789	3030	3032	3036	rVB4	1409	906	0.04%	0.006%
68	10.812	3036	3039	3042	rBV2	840	737	0.03%	0.005%
69	10.863	3048	3055	3058	rBV6	2752	3030	0.14%	0.021%
70	10.889	3061	3063	3065	rBV2	853	449	0.02%	0.003%
71	11.027	3104	3106	3109	rVB2	1663	688	0.03%	0.005%
72	11.046	3110	3112	3116	rBV5	712	497	0.02%	0.003%
73	11.191	3146	3157	3178	rBV	743633	1155814	54.24%	8.015%
74	11.567	3262	3274	3297	rBV	890807	1420746	66.67%	9.852%
75	11.959	3394	3396	3397	rBV	742	268	0.01%	0.002%
76	11.969	3397	3399	3400	rVV2	1257	397	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081623\
Data File : VV031819.D
Acq On : 16 Aug 2023 13:50
Operator : SY/MD
Sample : 03965-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M

Title : VOC Analysis

77	12.673	3615	3618	3619	rBV2	1186	601	0.03%	0.004%
78	12.767	3646	3647	3648	rBV	868	279	0.01%	0.002%
79	13.210	3777	3785	3791	rBV10	5374	8884	0.42%	0.062%
80	13.648	3919	3921	3924	rBV4	1405	826	0.04%	0.006%
81	13.689	3928	3934	3949	rVV4	6747	10879	0.51%	0.075%
82	13.773	3957	3960	3965	rVB	14401	9181	0.43%	0.064%
83	14.220	4096	4099	4101	rBV3	1913	1275	0.06%	0.009%




Sum of corrected areas: 14420280

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081623\
Data File : VV031819.D
Acq On : 16 Aug 2023 13:50
Operator : SY/MD
Sample : 03965-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

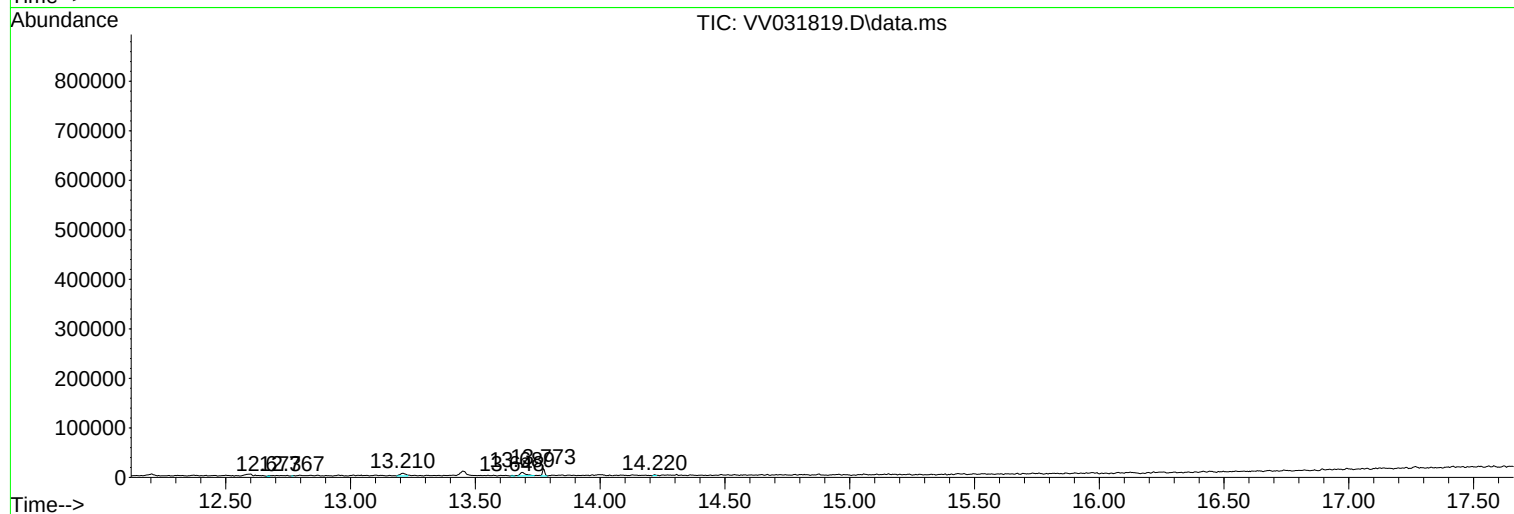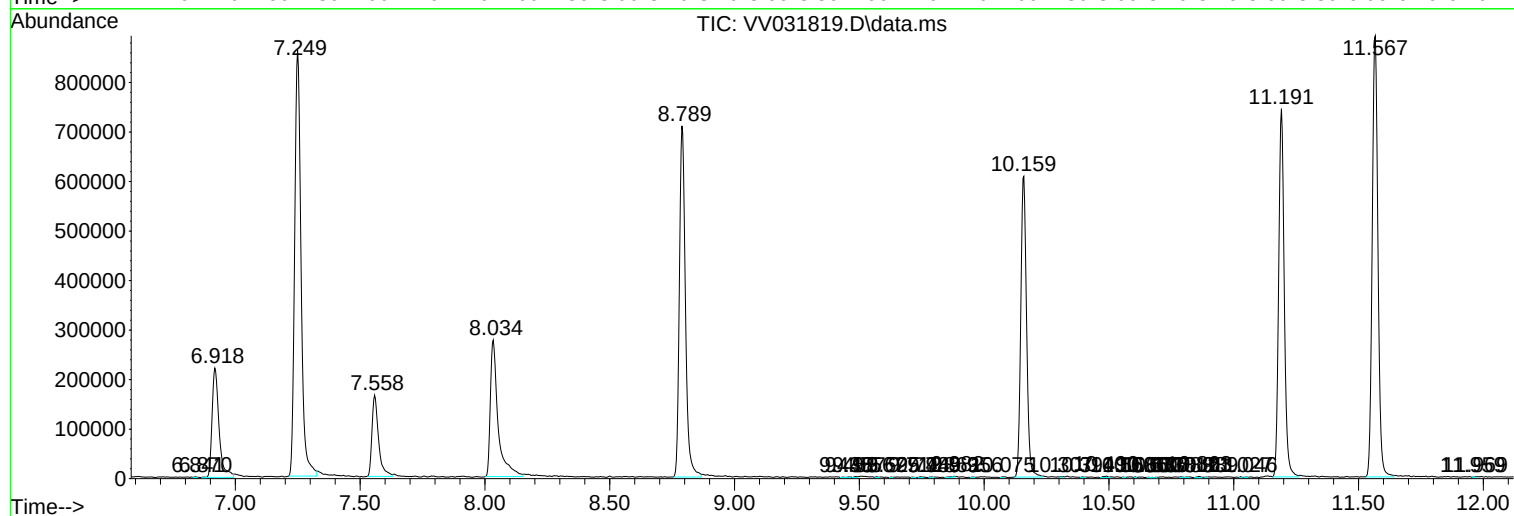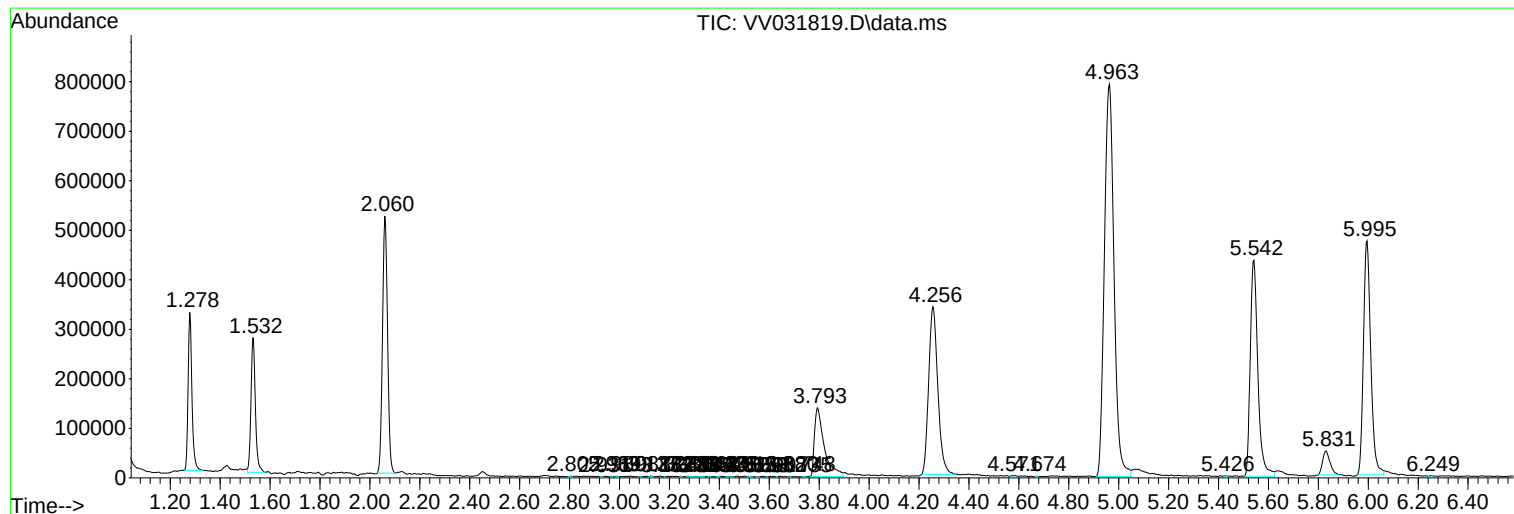

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081623\
Data File : VV031819.D
Acq On : 16 Aug 2023 13:50
Operator : SY/MD
Sample : 03965-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081623\
Data File : VV031819.D
Acq On : 16 Aug 2023 13:50
Operator : SY/MD
Sample : 03965-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------