

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081623\
 Data File : VV031821.D
 Acq On : 16 Aug 2023 14:59
 Operator : SY/MD
 Sample : 03968-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

Signal : TIC: VV031821.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	309257	325271	15.67%	2.326%
2	1.532	146	153	172	rVB	230656	290387	13.99%	2.077%
3	2.060	308	317	336	rVB	510067	757824	36.51%	5.420%
4	2.687	509	512	513	rBV2	1285	581	0.03%	0.004%
5	2.764	534	536	539	rVB2	1012	449	0.02%	0.003%
6	2.777	539	540	541	rBV	605	203	0.01%	0.001%
7	2.950	592	594	596	rVB2	1169	550	0.03%	0.004%
8	3.095	636	639	641	rVB3	1048	589	0.03%	0.004%
9	3.121	645	647	653	rVB5	1540	1323	0.06%	0.009%
10	3.233	676	682	684	rBV6	1797	1886	0.09%	0.013%
11	3.294	700	701	702	rBB	305	150	0.01%	0.001%
12	3.339	713	715	716	rBV2	735	366	0.02%	0.003%
13	3.439	744	746	750	rBV4	1487	810	0.04%	0.006%
14	3.503	764	766	768	rBV	512	206	0.01%	0.001%
15	3.580	784	790	792	rBV4	1127	1114	0.05%	0.008%
16	3.642	802	809	811	rBV4	1317	1465	0.07%	0.010%
17	3.690	823	824	826	rVB3	932	317	0.02%	0.002%
18	3.703	826	828	831	rBV3	1433	661	0.03%	0.005%
19	3.719	831	833	836	rBV4	846	534	0.03%	0.004%
20	3.751	841	843	844	rBV	700	247	0.01%	0.002%
21	3.796	848	857	887	rBV	122102	343847	16.57%	2.459%
22	4.098	949	951	952	rBV	1706	718	0.03%	0.005%
23	4.256	985	1000	1027	rBV	330450	857596	41.32%	6.133%
24	4.674	1129	1130	1133	rBV3	894	477	0.02%	0.003%
25	4.719	1141	1144	1147	rBV4	1471	1097	0.05%	0.008%
26	4.963	1203	1220	1250	rBV2	782222	2075553	100.00%	14.843%
27	5.426	1362	1364	1366	rBV3	1351	630	0.03%	0.005%
28	5.478	1378	1380	1386	rBV4	1405	1000	0.05%	0.007%
29	5.542	1388	1400	1423	rBV	429066	915240	44.10%	6.545%
30	5.831	1481	1490	1506	rVB2	43901	88757	4.28%	0.635%
31	5.995	1529	1541	1560	rBV	452036	938693	45.23%	6.713%
32	6.272	1625	1627	1629	rBV2	1332	699	0.03%	0.005%
33	6.400	1665	1667	1672	rVB5	1514	878	0.04%	0.006%
34	6.503	1696	1699	1701	rVB4	1287	606	0.03%	0.004%
35	6.516	1701	1703	1705	rBV4	947	490	0.02%	0.004%
36	6.548	1712	1713	1715	rBV3	915	449	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081623\
 Data File : VV031821.D
 Acq On : 16 Aug 2023 14:59
 Operator : SY/MD
 Sample : 03968-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

37	6.580	1721	1723	1726	rVB4	1308	545	0.03%	0.004%
38	6.725	1766	1768	1771	rBV4	1100	682	0.03%	0.005%
39	6.789	1786	1788	1790	rBV3	1384	736	0.04%	0.005%
40	6.831	1798	1801	1803	rBV4	1427	687	0.03%	0.005%
41	6.918	1816	1828	1850	rBV	210923	411884	19.84%	2.946%
42	7.249	1920	1931	1971	rBV	825401	1492724	71.92%	10.675%
43	7.558	2018	2027	2042	rBV	156871	277113	13.35%	1.982%
44	7.838	2111	2114	2119	rVB6	1425	1219	0.06%	0.009%
45	7.973	2153	2156	2160	rVB5	1781	1146	0.06%	0.008%
46	8.034	2163	2175	2203	rBV	255712	546606	26.34%	3.909%
47	8.445	2301	2303	2307	rBV4	1293	1031	0.05%	0.007%
48	8.519	2322	2326	2331	rBV5	1412	1308	0.06%	0.009%
49	8.612	2354	2355	2358	rBV3	958	553	0.03%	0.004%
50	8.789	2400	2410	2437	rBV	711018	1189403	57.31%	8.506%
51	9.233	2545	2548	2550	rBV4	1520	794	0.04%	0.006%
52	9.246	2550	2552	2555	rVB4	1272	369	0.02%	0.003%
53	9.474	2615	2623	2624	rBV4	1832	1684	0.08%	0.012%
54	9.641	2673	2675	2677	rBV2	1143	487	0.02%	0.003%
55	9.654	2677	2679	2682	rVB3	1294	583	0.03%	0.004%
56	9.702	2692	2694	2697	rBV4	1145	606	0.03%	0.004%
57	9.870	2741	2746	2748	rBV5	2576	1974	0.10%	0.014%
58	10.030	2790	2796	2798	rBV6	1884	1594	0.08%	0.011%
59	10.079	2809	2811	2814	rBV3	658	471	0.02%	0.003%
60	10.098	2814	2817	2819	rVV4	1235	802	0.04%	0.006%
61	10.159	2824	2836	2855	rBV	592596	945781	45.57%	6.764%
62	10.403	2909	2912	2915	rBV4	1721	1265	0.06%	0.009%
63	10.567	2962	2963	2964	rBV	523	149	0.01%	0.001%
64	10.645	2984	2987	2989	rBV3	687	426	0.02%	0.003%
65	10.706	3005	3006	3015	rVB6	1353	1571	0.08%	0.011%
66	10.738	3015	3016	3017	rBV	286	65	0.00%	0.000%
67	10.747	3017	3019	3022	rBV4	1379	895	0.04%	0.006%
68	10.760	3022	3023	3024	rBV	835	304	0.01%	0.002%
69	10.808	3035	3038	3040	rBV2	784	458	0.02%	0.003%
70	10.921	3069	3073	3074	rBV3	888	536	0.03%	0.004%
71	10.947	3079	3081	3083	rBV2	1112	680	0.03%	0.005%
72	11.021	3102	3104	3107	rBV3	1063	547	0.03%	0.004%
73	11.050	3111	3113	3118	rBV4	718	568	0.03%	0.004%
74	11.191	3146	3157	3179	rBV	722447	1129989	54.44%	8.081%
75	11.567	3262	3274	3294	rBV	849495	1345724	64.84%	9.624%
76	11.786	3340	3342	3343	rBV2	1152	566	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081623\
Data File : VV031821.D
Acq On : 16 Aug 2023 14:59
Operator : SY/MD
Sample : 03968-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M

Title : VOC Analysis

77	11.841	3357	3359	3365	rBV5	1848	1228	0.06%	0.009%
78	11.953	3392	3394	3395	rBV2	1831	746	0.04%	0.005%
79	12.175	3461	3463	3464	rBV	1275	468	0.02%	0.003%
80	12.741	3637	3639	3641	rBV3	1567	794	0.04%	0.006%
81	12.796	3654	3656	3659	rBV3	1828	1420	0.07%	0.010%
82	12.927	3694	3697	3699	rBV4	1402	913	0.04%	0.007%
83	12.969	3708	3710	3713	rBV3	1478	750	0.04%	0.005%
84	13.140	3761	3763	3765	rBV3	1241	630	0.03%	0.005%




Sum of corrected areas: 13983137

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081623\
Data File : VV031821.D
Acq On : 16 Aug 2023 14:59
Operator : SY/MD
Sample : 03968-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

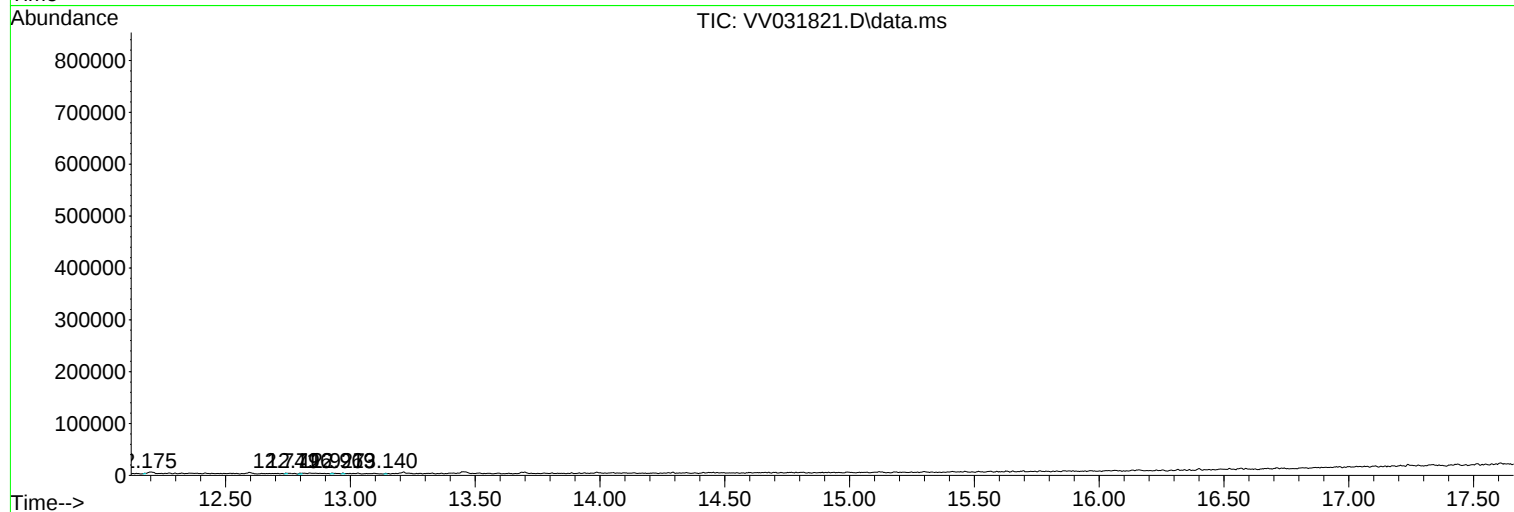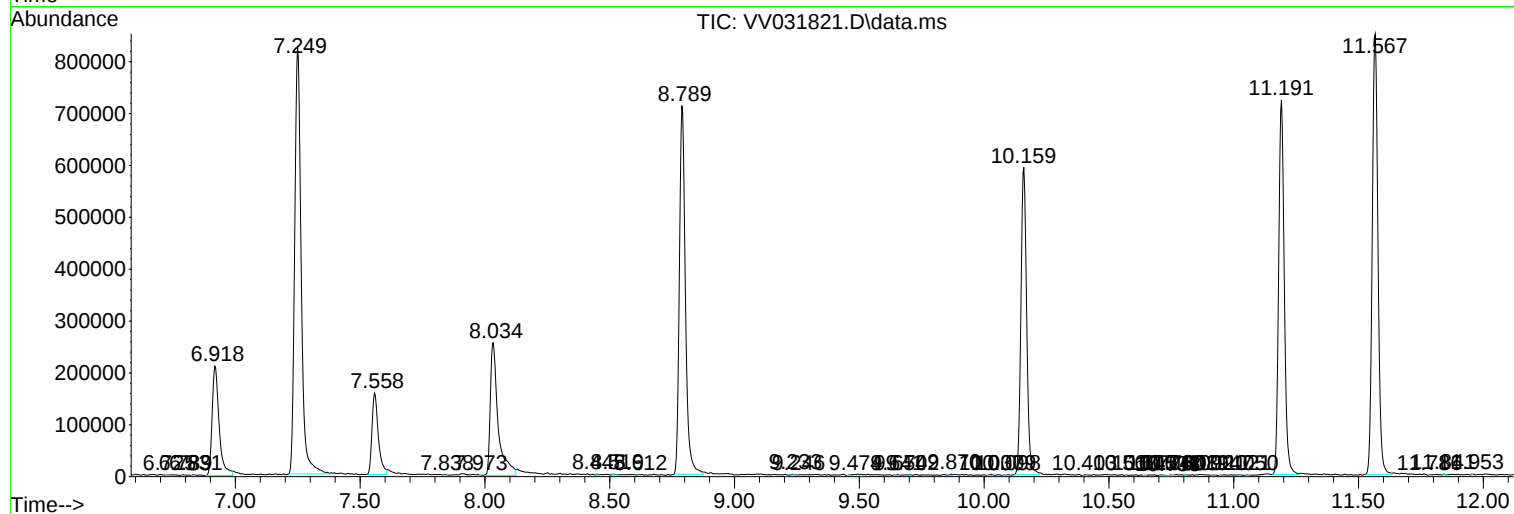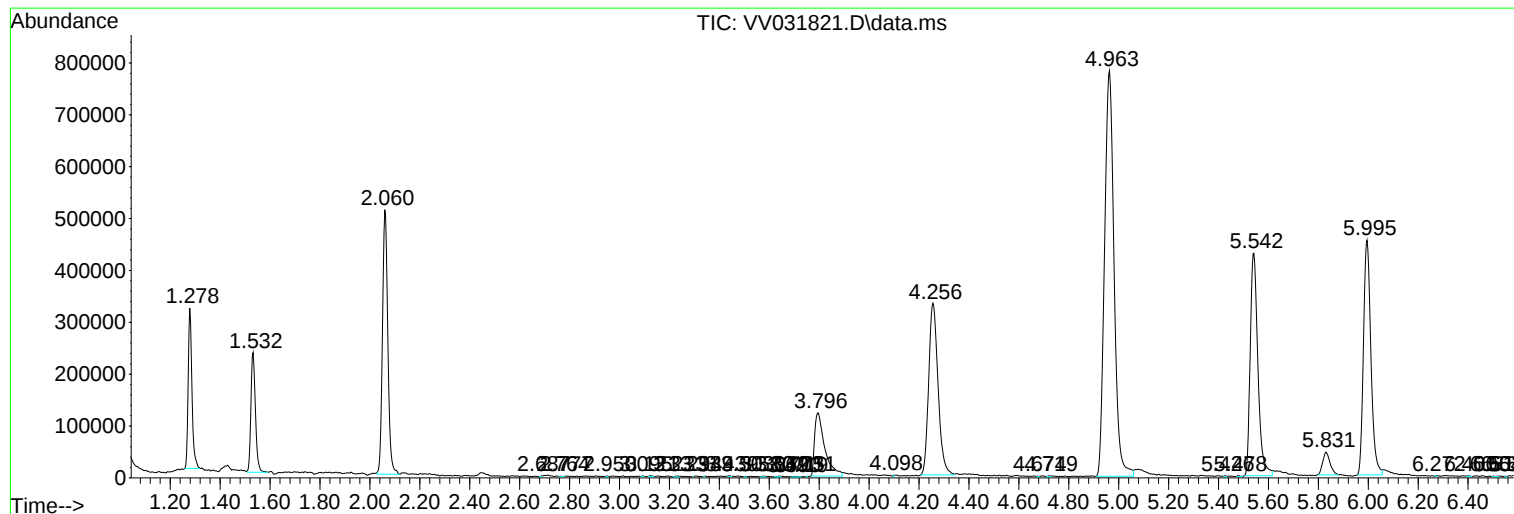

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081623\
Data File : VV031821.D
Acq On : 16 Aug 2023 14:59
Operator : SY/MD
Sample : 03968-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081623\
Data File : VV031821.D
Acq On : 16 Aug 2023 14:59
Operator : SY/MD
Sample : 03968-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------