
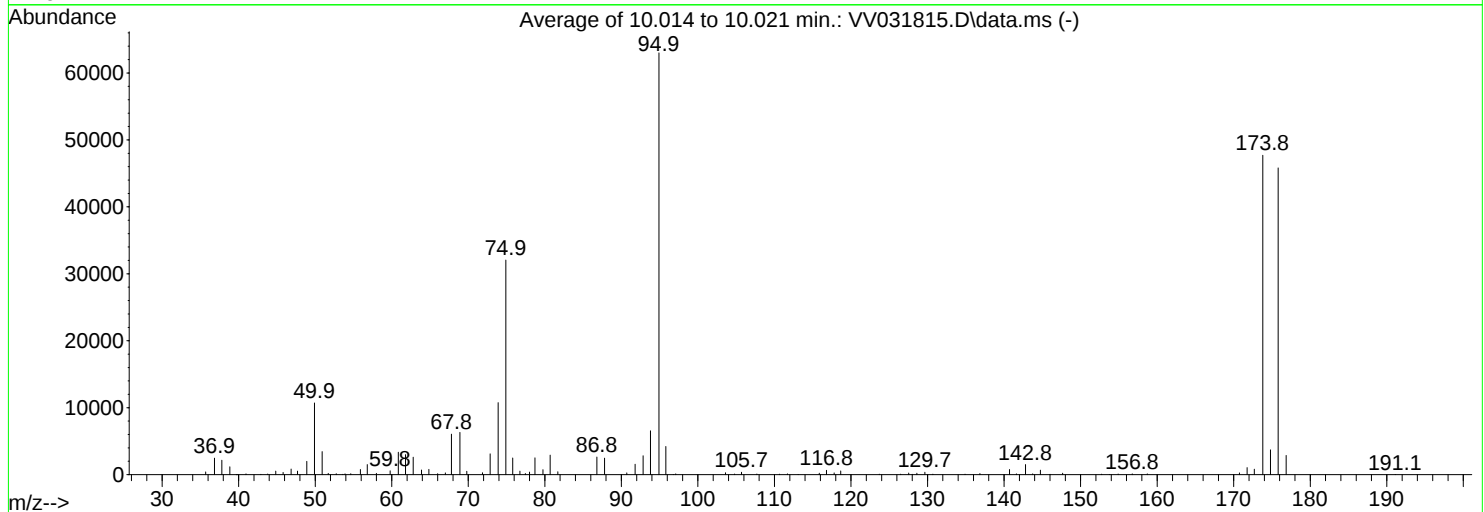


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081623\
Data File : VV031815.D
Acq On : 16 Aug 2023 09:02
Operator : SY/MD
Sample : BFB203
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB203

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Title : VOC Analysis
Last Update : Thu Aug 17 01:59:38 2023

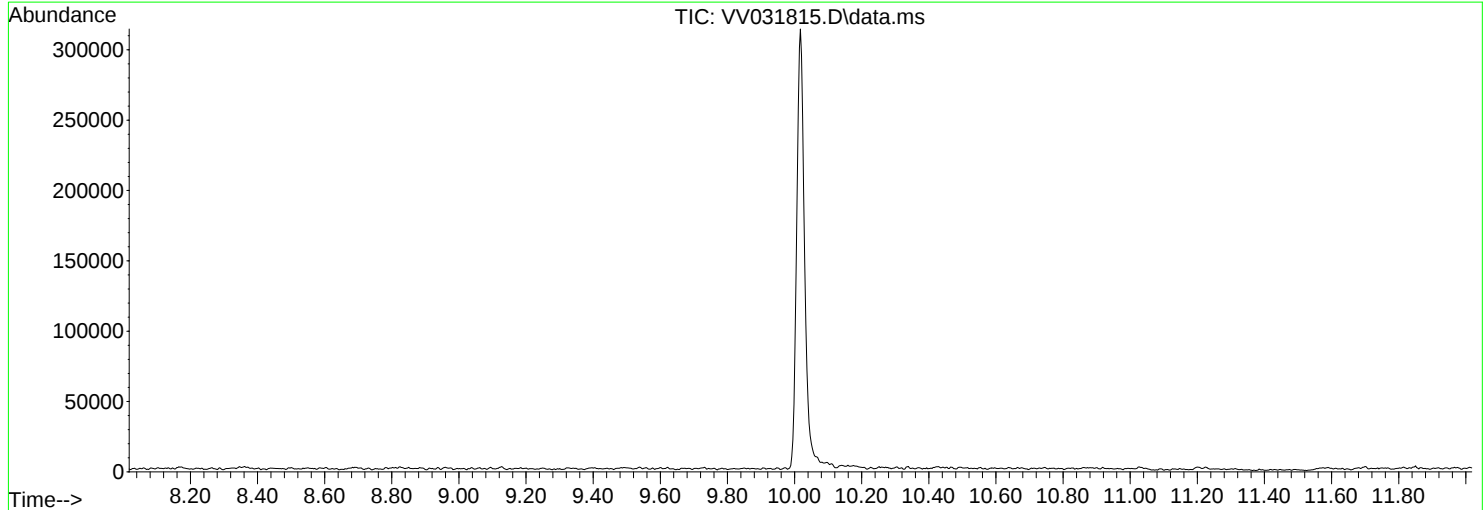

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2780

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	10722	PASS
75	95	30	80	50.9	32061	PASS
95	95	100	100	100.0	63008	PASS
96	95	5	9	6.7	4217	PASS
173	174	0.00	2	1.7	821	PASS
174	95	50	120	75.7	47704	PASS
175	174	5	9	7.8	3719	PASS
176	174	95	105	96.1	45827	PASS
177	176	5	10	6.2	2860	PASS

m/z	Abundance
37.90	108.0
39.80	393.0
43.90	936.0
48.30	134.0
53.10	115.0
54.90	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

m/z	Abundance
35.70	403.0
36.90	2574.0
37.80	2255.0
38.90	1201.0
39.70	360.0
41.10	136.0
43.80	1085.0
44.80	545.0
45.80	471.0
46.90	824.0
47.70	509.0
48.90	2191.0
49.90	10686.0
50.90	3577.0
51.70	241.0
52.70	191.0
53.90	171.0
54.70	143.0
55.90	779.0
56.80	1407.0
58.00	164.0
59.80	554.0
60.90	3539.0
61.80	2819.0
62.80	2659.0
63.90	792.0
64.80	686.0
66.00	114.0
67.00	247.0
67.80	6226.0
68.90	6417.0
69.80	492.0
71.90	229.0
72.90	3217.0
73.90	10584.0
74.90	32360.0
75.80	2525.0
76.80	516.0
78.00	475.0
78.70	2689.0
79.80	750.0
80.70	2878.0
81.70	422.0
86.80	2772.0
87.80	2442.0
90.80	328.0
91.80	1512.0
92.90	2796.0
93.80	6601.0
94.90	62672.0
95.80	4347.0
96.80	118.0
103.60	274.0
104.80	157.0
105.70	380.0
107.70	129.0
110.70	103.0
111.70	129.0
113.10	106.0
115.80	206.0
116.80	658.0
117.80	301.0
118.60	546.0
126.50	118.0
127.70	293.0
128.60	187.0
129.60	378.0
130.70	105.0
136.90	218.0
140.80	714.0
141.60	107.0
142.80	1514.0
143.70	107.0
144.80	732.0
146.00	124.0
147.70	147.0
156.80	113.0
158.70	178.0
170.80	291.0
171.80	1048.0
172.70	896.0
173.80	45680.0
174.80	3771.0
175.80	44232.0
176.80	2825.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

m/z	Abundance
35.70	406.0
36.90	2503.0
37.80	2270.0
38.90	1182.0
39.60	410.0
40.90	121.0
43.80	1003.0
44.90	562.0
45.80	354.0
46.80	875.0
47.70	588.0
48.90	2053.0
49.90	11179.0
50.90	3576.0
51.70	197.0
52.80	163.0
53.90	217.0
54.60	163.0
55.90	802.0
56.80	1542.0
58.00	212.0
59.80	600.0
60.80	3454.0
61.80	3137.0
62.80	2673.0
63.90	713.0
64.80	773.0
66.00	144.0
67.00	275.0
67.80	6278.0
68.90	6495.0
69.80	478.0
71.90	291.0
72.90	3247.0
73.90	11381.0
74.90	33080.0
75.80	2503.0
76.70	557.0
77.40	263.0
78.00	417.0
78.70	2487.0
79.80	780.0
80.70	2979.0
81.70	431.0
86.80	2712.0
87.80	2559.0
90.70	282.0
91.80	1588.0
92.80	3010.0
93.80	6698.0
94.90	65304.0
95.80	4328.0
97.10	152.0
103.60	322.0
104.80	138.0
105.70	360.0
107.70	148.0
111.70	149.0
115.90	219.0
116.80	655.0
117.80	295.0
118.70	583.0
123.70	111.0
126.50	126.0
127.50	251.0
128.60	231.0
129.70	351.0
130.70	111.0
134.90	114.0
136.90	171.0
140.70	766.0
141.60	113.0
142.80	1536.0
143.80	126.0
144.80	690.0
147.70	224.0
152.70	137.0
154.90	126.0
156.70	140.0
158.70	170.0
170.80	276.0
171.70	1059.0
172.70	844.0
173.80	49472.0
174.80	3840.0
175.80	47520.0
176.90	2964.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

m/z	Abundance
35.70	428.0
36.80	2298.0
37.80	2240.0
38.80	1103.0
39.60	434.0
40.80	131.0
42.90	158.0
43.80	1001.0
44.90	459.0
45.90	185.0
46.80	833.0
47.70	493.0
48.90	1722.0
49.90	10301.0
50.90	3142.0
51.60	120.0
52.80	120.0
53.60	176.0
54.70	157.0
55.10	138.0
55.90	721.0
56.80	1597.0
58.00	182.0
59.80	579.0
60.80	3045.0
61.80	3037.0
62.80	2521.0
63.90	574.0
64.90	881.0
66.00	169.0
67.00	253.0
67.80	5647.0
68.90	5997.0
69.80	507.0
71.80	314.0
72.80	2858.0
73.90	10332.0
74.90	30744.0
75.80	2434.0
76.70	487.0
77.50	245.0
77.90	276.0
78.70	2333.0
79.70	729.0
80.70	2903.0
81.70	413.0
86.80	2388.0
87.80	2396.0
90.60	195.0
91.80	1547.0
92.80	2641.0
93.80	6343.0
94.90	61048.0
95.80	3977.0
97.10	243.0
103.60	302.0
105.70	331.0
110.60	109.0
111.70	107.0
115.80	203.0
116.80	633.0
117.80	215.0
118.70	532.0
123.70	132.0
127.50	201.0
128.00	131.0
128.60	249.0
129.70	325.0
134.90	114.0
136.80	133.0
140.60	797.0
141.60	115.0
142.80	1473.0
143.80	133.0
144.70	582.0
147.60	241.0
152.80	115.0
153.80	104.0
154.90	142.0
156.70	107.0
170.70	223.0
171.70	1054.0
172.70	723.0
173.80	47960.0
174.80	3547.0
175.80	45728.0
176.90	2791.0
191.10	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203