
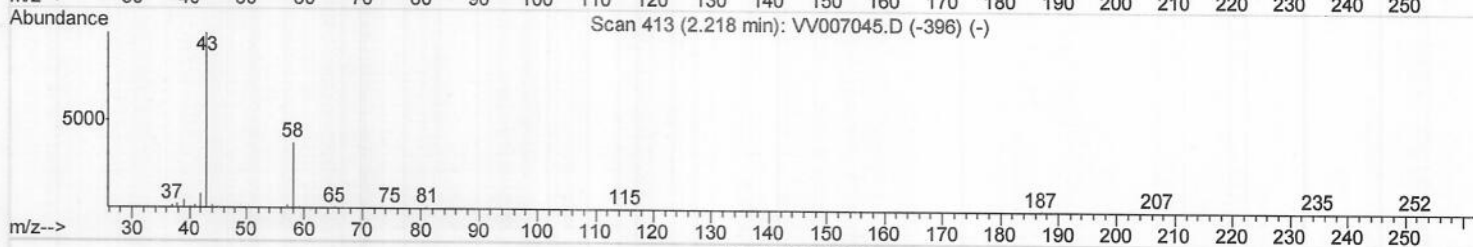
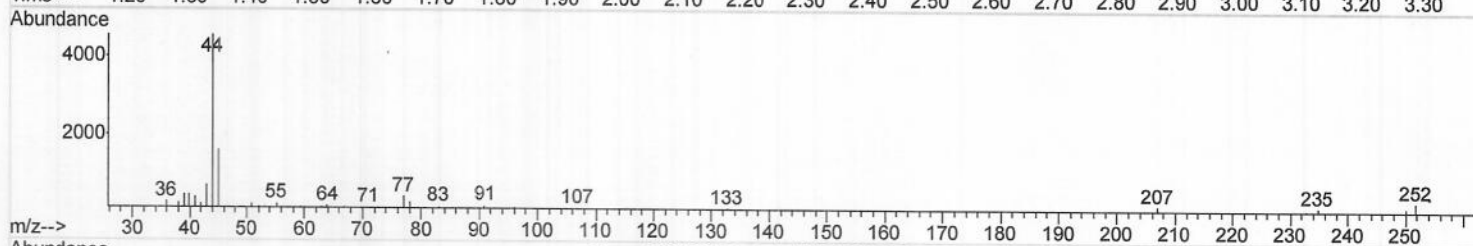


Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081718\
 Data File : VV007050.D
 Acq On : 17 Aug 2018 13:16
 Operator : SY/MD
 Sample : J4487-02
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Quant Time: Aug 18 03:38:05 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 18 03:36:46 2018
 Response via : Initial Calibration

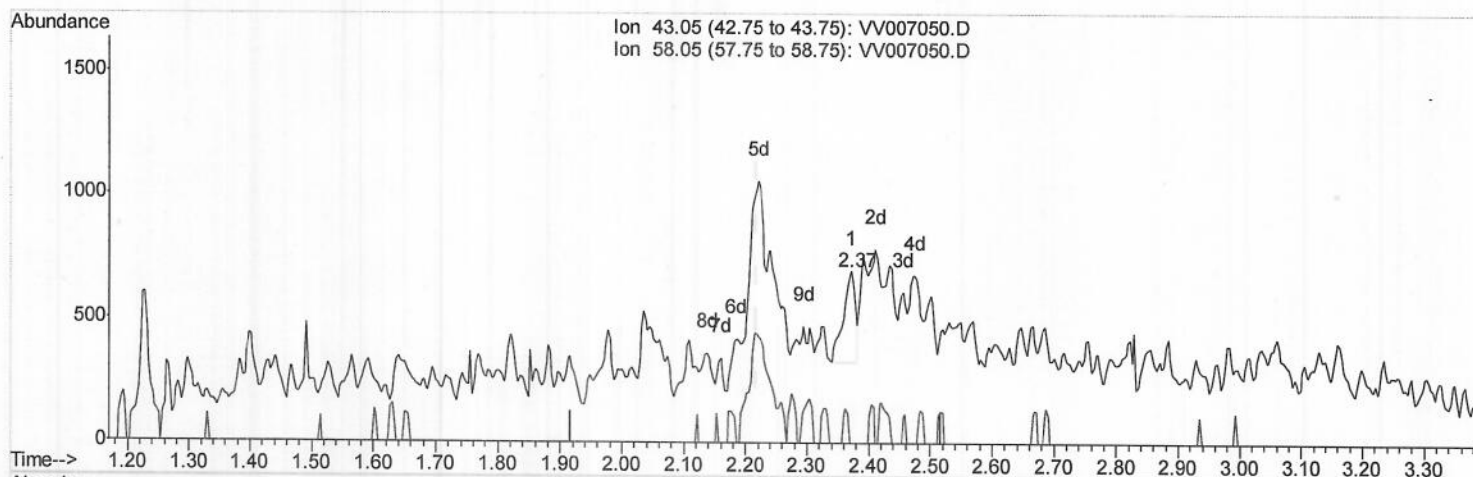

(13) Acetone (T)

2.373min (+0.154) 0.25ug/L




response 498

Ion	Exp%	Act%
43.05	100	100
58.05	35.70	14.26
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081718\
 Data File : VV007050.D
 Acq On : 17 Aug 2018 13:16
 Operator : SY/MD
 Sample : J4487-02
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Quant Time: Aug 18 03:38:05 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 18 03:36:46 2018
 Response via : Initial Calibration

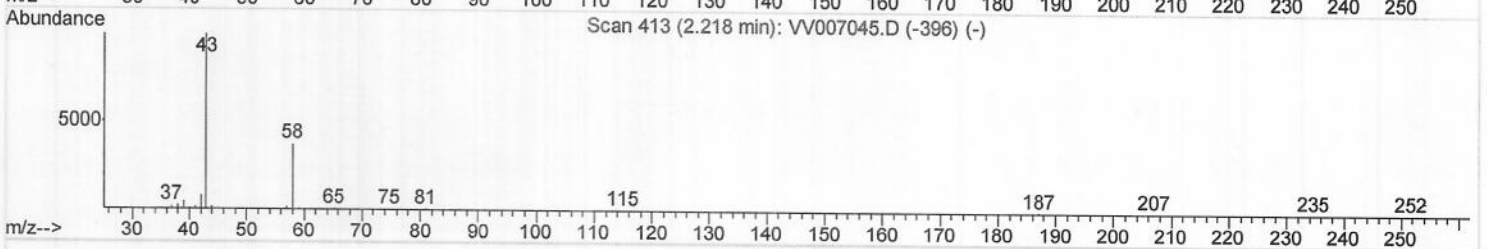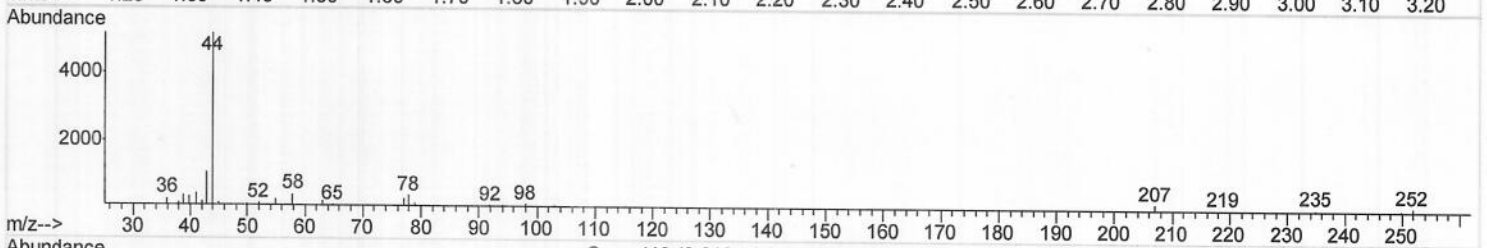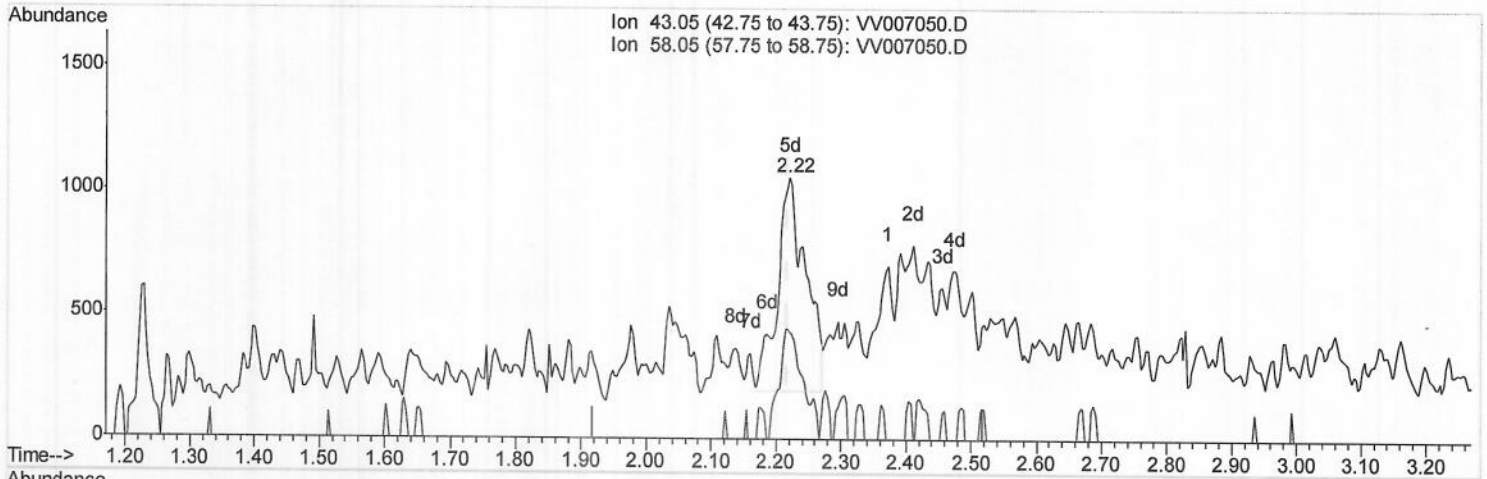

TIC: VV007050.D

(13) Acetone (T)

2.221min (+0.003) 1.30ug/L m) MD08124118

response 2584

Ion	Exp%	Act%
43.05	100	100
58.05	35.70	2.75
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081718\
 Data File : VV007050.D
 Acq On : 17 Aug 2018 13:16
 Operator : SY/MD
 Sample : J4487-02
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Quant Time: Aug 18 04:07:06 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 18 03:36:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	208062	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	202213	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	78358	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	74047	5.51	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	110.20%	
7) Chloroethane-d5	1.58	69	65710	5.77	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	115.40%	
11) 1,1-Dichloroethene-d2	2.13	63	104611	4.15	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	83.00%	
20) 2-Butanone-d5	3.98	46	178324	46.17	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	92.34%	
24) Chloroform-d	4.41	84	153614	5.64	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	112.80%	
26) 1,2-Dichloroethane-d4	5.09	65	77625	5.64	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	112.80%	
32) Benzene-d6	5.10	84	296644	5.71	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	114.20%	
36) 1,2-Dichloropropane-d6	6.12	67	98898	5.57	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	111.40%	
41) Toluene-d8	7.37	98	220351	4.99	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	99.80%	
43) trans-1,3-Dichloropropene-	7.67	79	30362	4.91	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	98.20%	
46) 2-Hexanone-d5	8.15	63	85870	33.99	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	67.98%	
57) 1,1,2,2-Tetrachloroethane-	10.27	84	70149	5.07	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	101.40%	
64) 1,2-Dichlorobenzene-d4	11.68	152	76907	5.64	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	112.80%	

Target Compounds

13) Acetone	2.22	43	2584m)	1.299	ug/L	Ovalue
-------------	------	----	---------	-------	------	--------

>M008/24/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081718\
 Data File : VV007050.D
 Acq On : 17 Aug 2018 13:16
 Operator : SY/MD
 Sample : J4487-02
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Quant Time: Aug 18 04:07:06 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 18 03:36:46 2018
 Response via : Initial Calibration

