

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081718\
 Data File : VV007063.D
 Acq On : 17 Aug 2018 19:03
 Operator : SY/MD
 Sample : J4488-11
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0306

Quant Time: Aug 18 04:57:17 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 18 03:36:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	227105	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	222613	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	86383	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	87009	5.94	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	118.80%
7) Chloroethane-d5	1.58	69	77238	6.21	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	124.20%
11) 1,1-Dichloroethene-d2	2.13	63	118622	4.31	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.20%
20) 2-Butanone-d5	3.97	46	224733	53.31	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.62%
24) Chloroform-d	4.41	84	180250	6.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	121.20%
26) 1,2-Dichloroethane-d4	5.09	65	90484	6.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	120.60%
32) Benzene-d6	5.10	84	339331	5.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	118.60%
36) 1,2-Dichloropropane-d6	6.12	67	115990	5.93	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	118.60%
41) Toluene-d8	7.37	98	252187	5.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.60%
43) trans-1,3-Dichloropropene-	7.67	79	32901	4.84	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.80%
46) 2-Hexanone-d5	8.15	63	93055	33.46	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	66.92%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	81958	5.38	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	88232	5.87	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	117.40%


Target Compounds					Ovalue
13) Acetone	2.21	43	4651	2.14 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081718\
Data File : VV007063.D
Acq On : 17 Aug 2018 19:03
Operator : SY/MD
Sample : J4488-11
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0306

Quant Time: Aug 18 04:57:17 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 18 03:36:46 2018
Response via : Initial Calibration

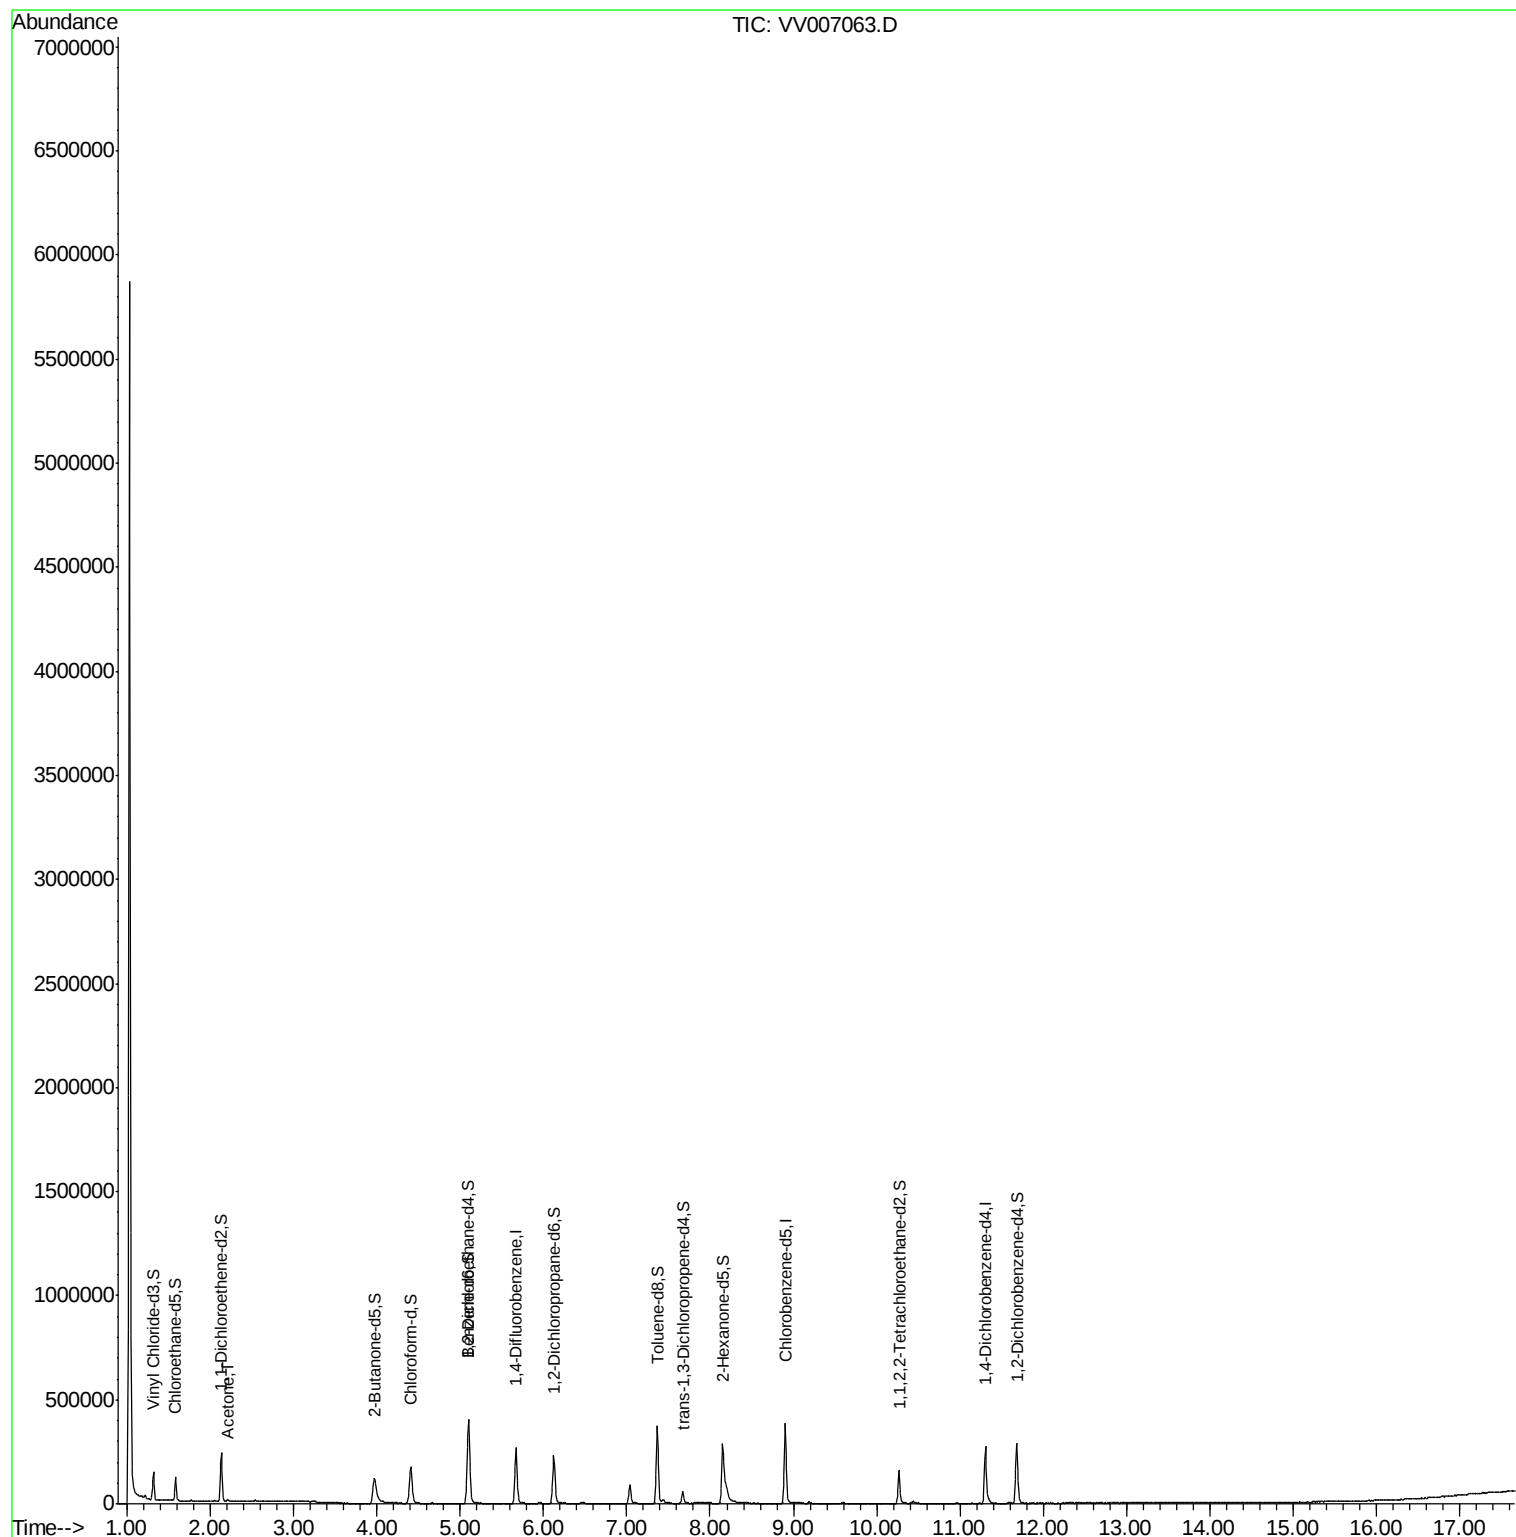

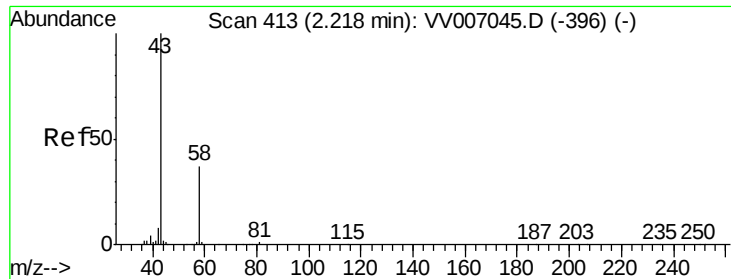

#13

Acetone

Concen: 2.14 ug/L

RT: 2.21 min Scan# 410

Delta R.T. -0.01 min

Lab File: VV007063.D

Acq: 17 Aug 2018 19:03

Instrument :
MSVOA_V
ClientSampleId :
C0306

Tot Ion: 43 Resp: 4651

Ion Ratio Lower Upper

43 100

58 39.6 0.0 71.4

