


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081718\
 Data File : VV007044.D
 Acq On : 17 Aug 2018 08:54
 Operator : SY/MD
 Sample : BFB86
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB86

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Aug 18 03:36:46 2018

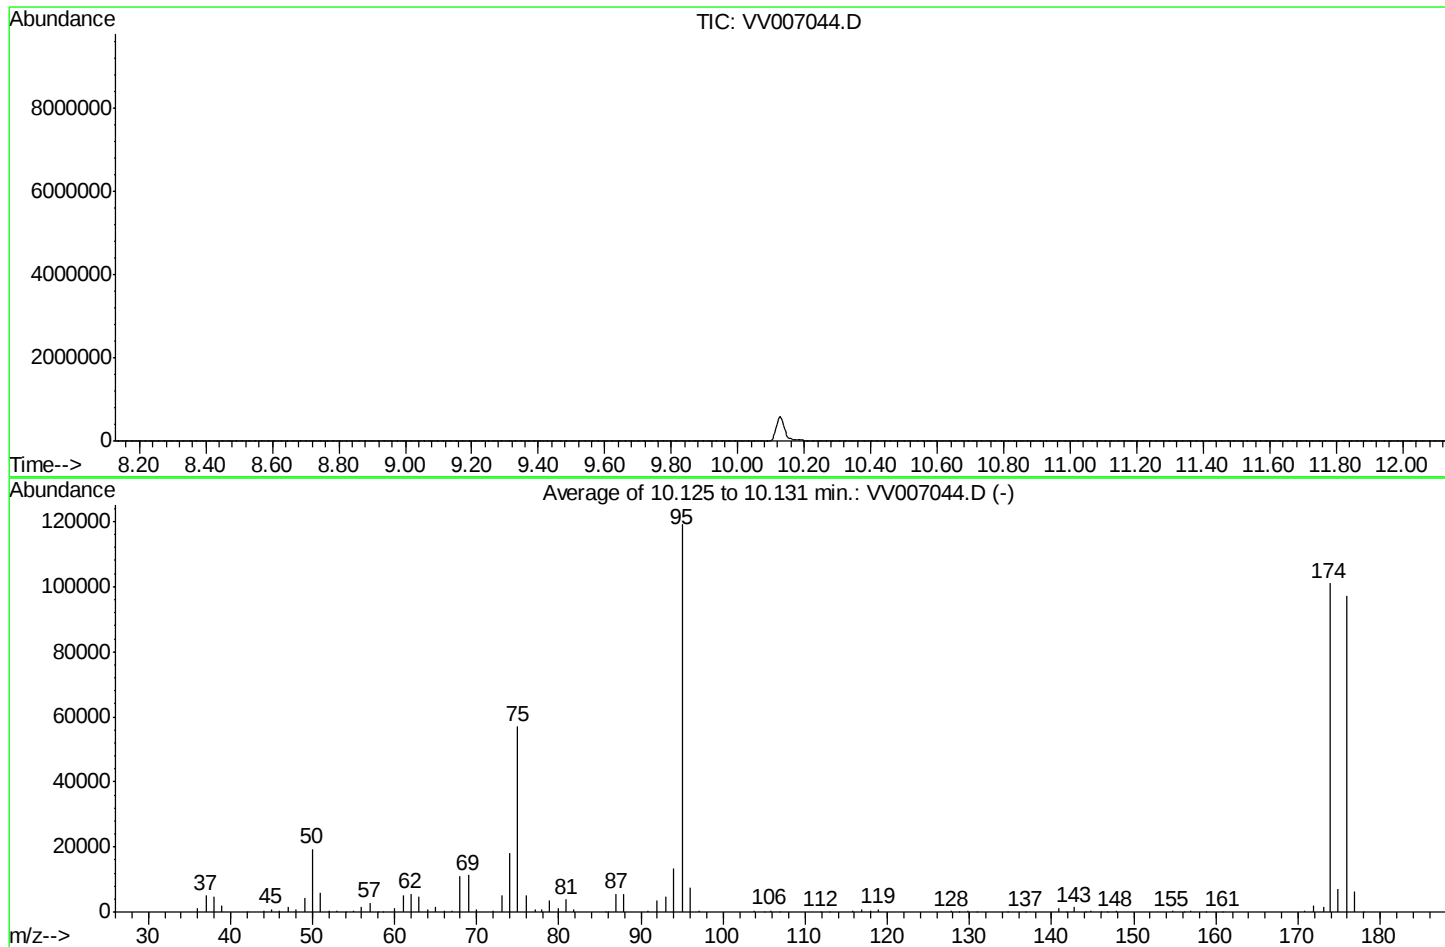

AutoFind: Scans 2872, 2873, 2874; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	19442	PASS
75	95	30	80	47.8	57002	PASS
95	95	100	100	100.0	119146	PASS
96	95	5	9	6.4	7672	PASS
173	174	0.00	2	1.5	1494	PASS
174	95	50	120	84.7	100952	PASS
175	174	5	9	7.2	7241	PASS
176	174	95	101	96.3	97242	PASS
177	176	5	9	6.3	6147	PASS

Scan 2858 (10.080 min): VV007044.D
BFB86

m/z	Abundance
39.90	497.0
44.00	1040.0
206.90	169.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
36.00	970.0
37.00	5163.0
38.00	4877.0
39.00	2202.0
40.00	480.0
44.00	1593.0
44.90	1028.0
45.80	263.0
47.00	1748.0
48.00	751.0
49.00	4330.0
50.00	19968.0
51.00	6067.0
52.00	397.0
52.90	270.0
54.10	151.0
55.00	384.0
55.90	1654.0
57.00	2845.0
57.90	123.0
58.50	110.0
59.90	1062.0
61.00	5350.0
62.00	5701.0
63.00	4814.0
64.00	940.0
65.00	1438.0
66.00	245.0
66.90	419.0
68.00	11480.0
69.00	11607.0
70.00	791.0
71.90	609.0
73.00	4988.0
74.00	18432.0
75.00	58216.0
76.00	4871.0
77.10	684.0
77.80	651.0
78.90	3580.0
79.90	1053.0
80.90	3758.0
81.90	817.0
85.70	207.0
86.90	5548.0
87.90	5386.0
90.80	396.0
92.00	3316.0
93.00	4743.0
94.00	13670.0
95.00	119384.0
96.00	7796.0
97.10	208.0
103.80	452.0
105.00	150.0
105.80	365.0
112.90	104.0
115.80	346.0
116.90	798.0
117.90	422.0
118.90	743.0
127.80	411.0
128.70	148.0
129.70	355.0
130.90	176.0
134.70	193.0
136.90	225.0
140.90	1011.0
142.80	1382.0
144.80	654.0
146.00	166.0
146.80	146.0
147.90	250.0
154.70	238.0
156.90	254.0
158.70	126.0
170.80	224.0
171.90	1994.0
173.10	1535.0
173.90	98528.0
174.90	7113.0
175.90	95808.0
176.90	6003.0
178.00	184.0
207.00	164.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
36.00	1027.0
37.00	5278.0
38.00	4699.0
39.00	2225.0
40.00	459.0
44.00	1587.0
45.00	1003.0
45.90	319.0
47.00	1836.0
48.00	736.0
49.00	4312.0
50.00	19968.0
51.00	6128.0
52.10	399.0
52.90	218.0
54.10	188.0
55.00	407.0
56.00	1664.0
57.00	3003.0
57.90	102.0
59.90	1051.0
61.00	5363.0
62.00	5900.0
63.00	4753.0
64.00	881.0
65.00	1482.0
66.00	251.0
67.00	405.0
68.00	11396.0
69.00	11720.0
70.00	850.0
72.00	620.0
73.00	5078.0
74.00	18904.0
75.00	58784.0
76.00	5159.0
77.10	696.0
77.80	625.0
78.90	3777.0
79.90	1176.0
80.90	3984.0
81.90	907.0
85.90	193.0
87.00	5799.0
87.90	5684.0
90.90	402.0
92.00	3439.0
93.00	5017.0
94.00	13967.0
95.00	122912.0
96.00	7972.0
97.00	226.0
103.80	401.0
104.90	179.0
105.80	433.0
106.90	135.0
115.80	400.0
116.90	762.0
117.90	411.0
118.90	859.0
127.90	389.0
128.80	192.0
129.80	369.0
130.90	170.0
134.70	173.0
136.80	199.0
140.90	1035.0
142.80	1520.0
144.20	109.0
144.80	602.0
146.00	171.0
146.80	109.0
147.80	207.0
154.70	298.0
156.10	102.0
156.90	228.0
158.80	207.0
160.90	120.0
170.70	257.0
171.90	2046.0
173.10	1571.0
173.90	104056.0
174.90	7508.0
175.90	100296.0
176.90	6333.0
178.00	217.0
206.90	156.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
36.00	1001.0
37.00	4792.0
38.00	4084.0
39.00	2078.0
40.00	523.0
42.10	117.0
44.00	1467.0
45.00	868.0
46.00	337.0
47.00	1638.0
48.00	700.0
49.00	3852.0
50.00	18392.0
51.00	5638.0
52.10	330.0
53.00	171.0
54.00	153.0
55.10	412.0
56.00	1522.0
57.00	2819.0
60.00	1023.0
61.00	4907.0
62.00	5549.0
63.00	4195.0
64.00	828.0
65.00	1372.0
66.00	205.0
67.00	325.0
68.00	10549.0
69.00	10784.0
70.00	788.0
72.00	579.0
73.00	4779.0
74.00	17248.0
75.00	54008.0
76.00	4930.0
77.10	674.0
77.90	579.0
78.90	3732.0
79.90	1125.0
80.90	3996.0
81.80	868.0
86.00	199.0
87.00	5726.0
87.90	5327.0
91.00	358.0
92.00	3455.0
93.00	5020.0
94.00	12821.0
95.00	115144.0
96.00	7249.0
97.10	239.0
103.90	325.0
104.90	201.0
105.80	497.0
106.90	122.0
111.90	164.0
115.90	366.0
116.80	638.0
117.90	392.0
118.90	846.0
127.90	340.0
128.80	190.0
129.90	375.0
130.90	131.0
134.70	179.0
136.80	157.0
140.90	944.0
141.80	125.0
142.80	1439.0
144.00	140.0
144.80	511.0
146.00	161.0
147.80	224.0
154.70	293.0
156.90	176.0
158.80	240.0
160.90	180.0
170.70	330.0
171.90	1985.0
173.10	1377.0
173.90	100272.0
174.90	7103.0
175.90	95624.0
176.90	6105.0
177.90	189.0
206.90	173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86