

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081720\
 Data File : VV018022.D
 Acq On : 17 Aug 2020 13:38
 Operator : SY/MD
 Sample : L3709-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFSH9

Quant Time: Aug 18 02:21:32 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 18 01:23:44 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	243167	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	239991	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	116322	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	89674	48.33	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	96.66%
7) Chloroethane-d5	1.58	69	77687	51.18	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	102.36%
11) 1,1-Dichloroethene-d2	2.12	63	135897	38.29	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.58%
21) 2-Butanone-d5	3.91	46	116283	95.69	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	95.69%
24) Chloroform-d	4.38	84	167706	49.66	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.32%
26) 1,2-Dichloroethane-d4	5.06	65	115919	52.84	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.68%
32) Benzene-d6	5.08	84	336953	50.95	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.90%
36) 1,2-Dichloropropane-d6	6.09	67	110465	51.09	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.18%
41) Toluene-d8	7.34	98	297834	50.07	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.14%
43) trans-1,3-Dichloropropene-	7.64	79	49522	50.49	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	100.98%
47) 2-Hexanone-d5	8.11	63	58291	84.01	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	84.01%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	132745	47.14	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.28%
64) 1,2-Dichlorobenzene-d4	11.65	152	124938	54.57	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	109.14%


Target Compounds					Ovalue
13) Acetone	2.19	43	12258	9.766 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081720\
Data File : VV018022.D
Acq On : 17 Aug 2020 13:38
Operator : SY/MD
Sample : L3709-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFSH9

Quant Time: Aug 18 02:21:32 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 18 01:23:44 2020
Response via : Initial Calibration

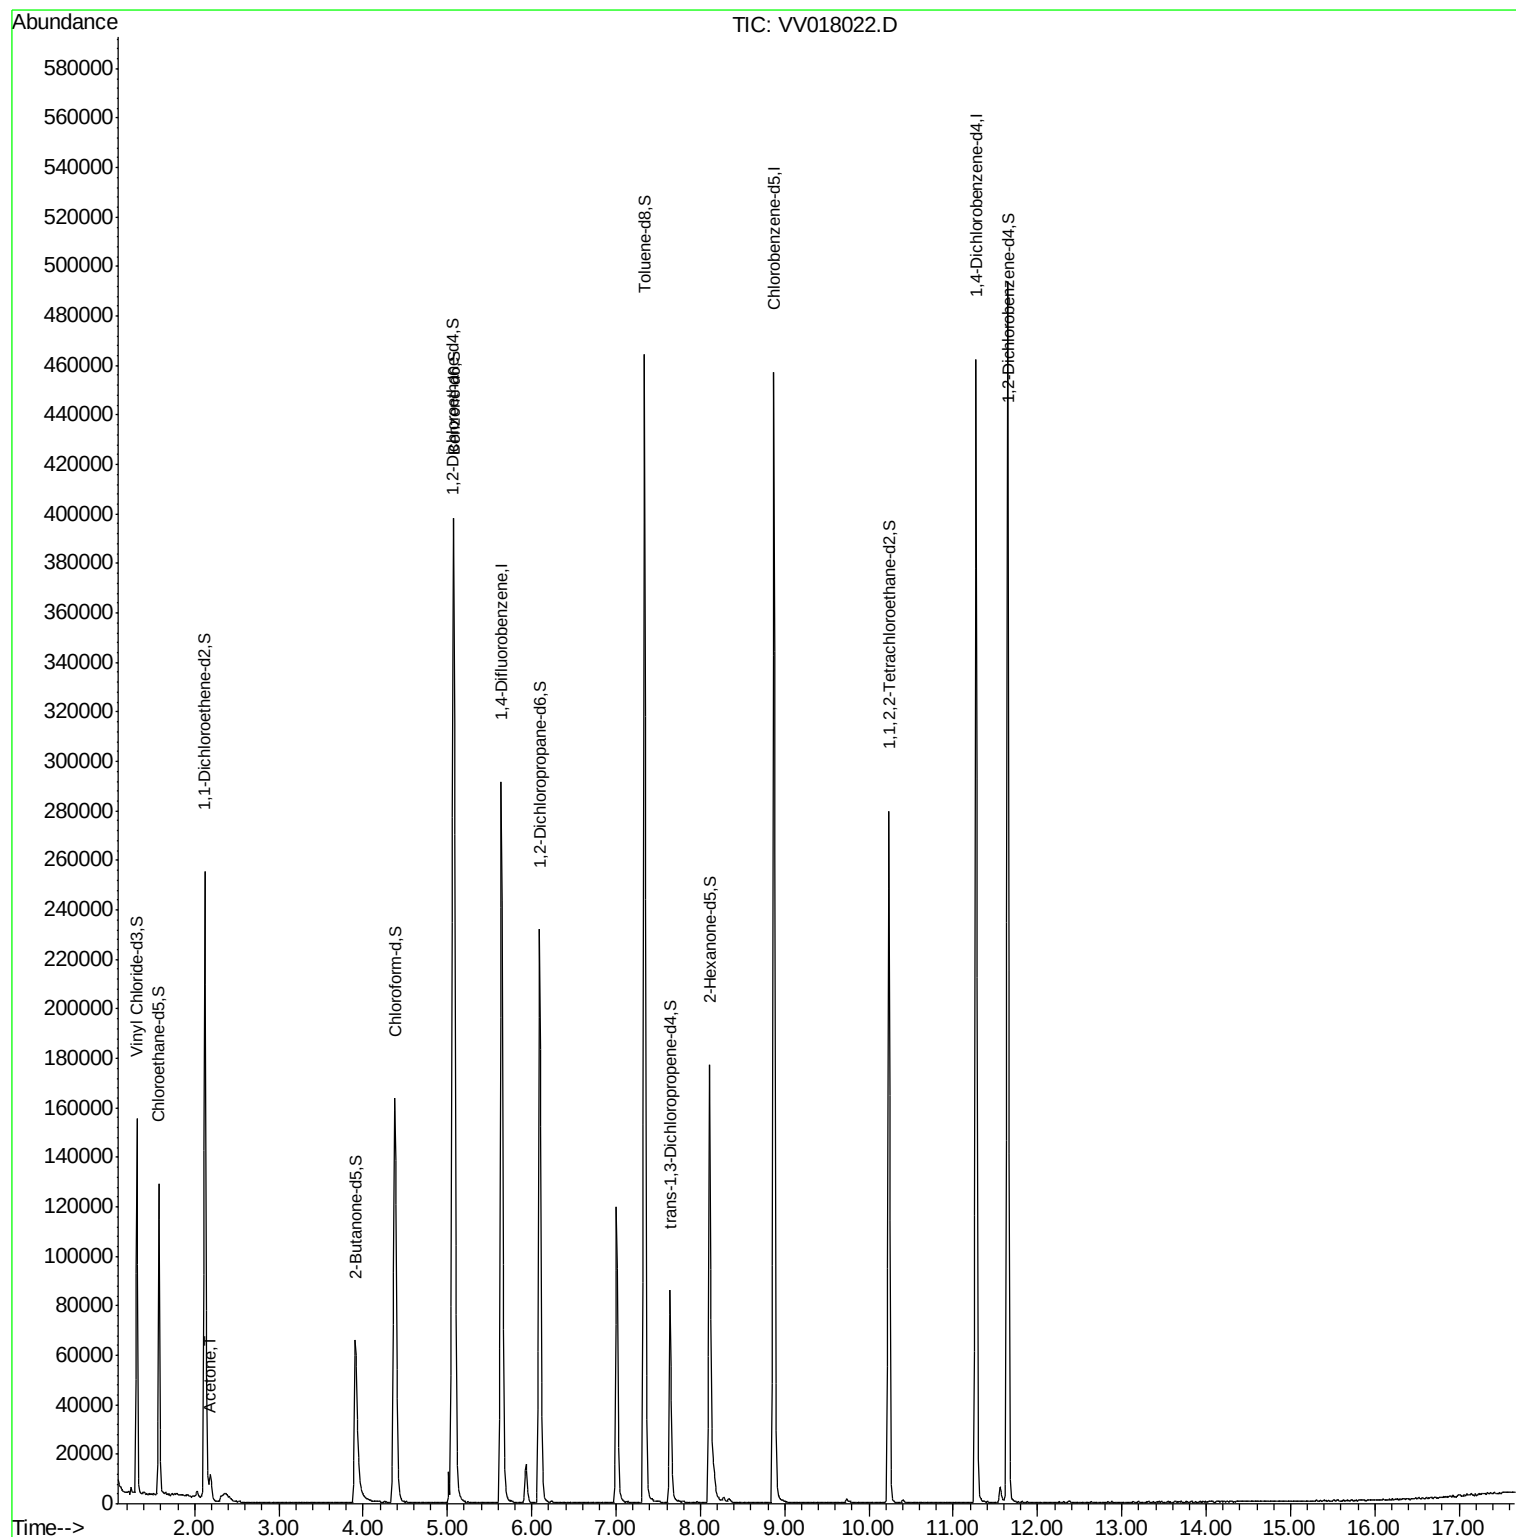

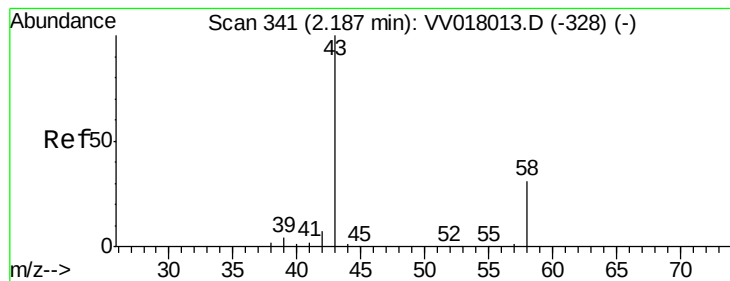

#13
 Acetone
 Concen: 9.766 ug/L
 RT: 2.19 min Scan# 342
 Delta R.T. 0.00 min
 Lab File: VV018022.D
 Acq: 17 Aug 2020 13:38

Instrument :
 MSVOA_V
 ClientSampleId :
 BFSH9

Tot Ion: 43 Resp: 12258
 Ion Ratio Lower Upper
 43 100
 58 34.1 0.0 63.6

