

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081721\
 Data File : VV021821.D
 Acq On : 17 Aug 2021 18:11
 Operator : SY/MD
 Sample : M3365-14ME
 Misc : 11.82g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKCOME

Quant Time: Aug 18 02:10:54 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 18 02:05:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	444053	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	404076	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	195695	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	114301	32.926	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	65.860%
7) Chloroethane-d5	1.558	69	97695	37.293	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	74.580%
11) 1,1-Dichloroethene-d2	2.101	63	137056	24.803	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	49.600%#
21) 2-Butanone-d5	3.873	46	223494	103.516	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	103.520%
24) Chloroform-d	4.349	84	247568	41.162	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.320%
26) 1,2-Dichloroethane-d4	5.034	65	154568	44.678	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.360%
32) Benzene-d6	5.050	84	488133	42.009	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.020%
36) 1,2-Dichloropropane-d6	6.069	67	161490	44.629	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	89.260%
41) Toluene-d8	7.320	98	424403	39.516	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	79.040%#
43) trans-1,3-Dichloroprop...	7.625	79	71709	40.267	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.540%
47) 2-Hexanone-d5	8.088	63	120039	101.216	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	101.220%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	213548	47.623	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.240%
66) 1,2-Dichlorobenzene-d4	11.625	152	184651	45.593	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.180%
Target Compounds						Qvalue
16) Methylene chloride	2.506	84	6360	1.742	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081721\
Data File : VV021821.D
Acq On : 17 Aug 2021 18:11
Operator : SY/MD
Sample : M3365-14ME
Misc : 11.82g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKCOME


Quant Time: Aug 18 02:10:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 18 02:05:23 2021
Response via : Initial Calibration

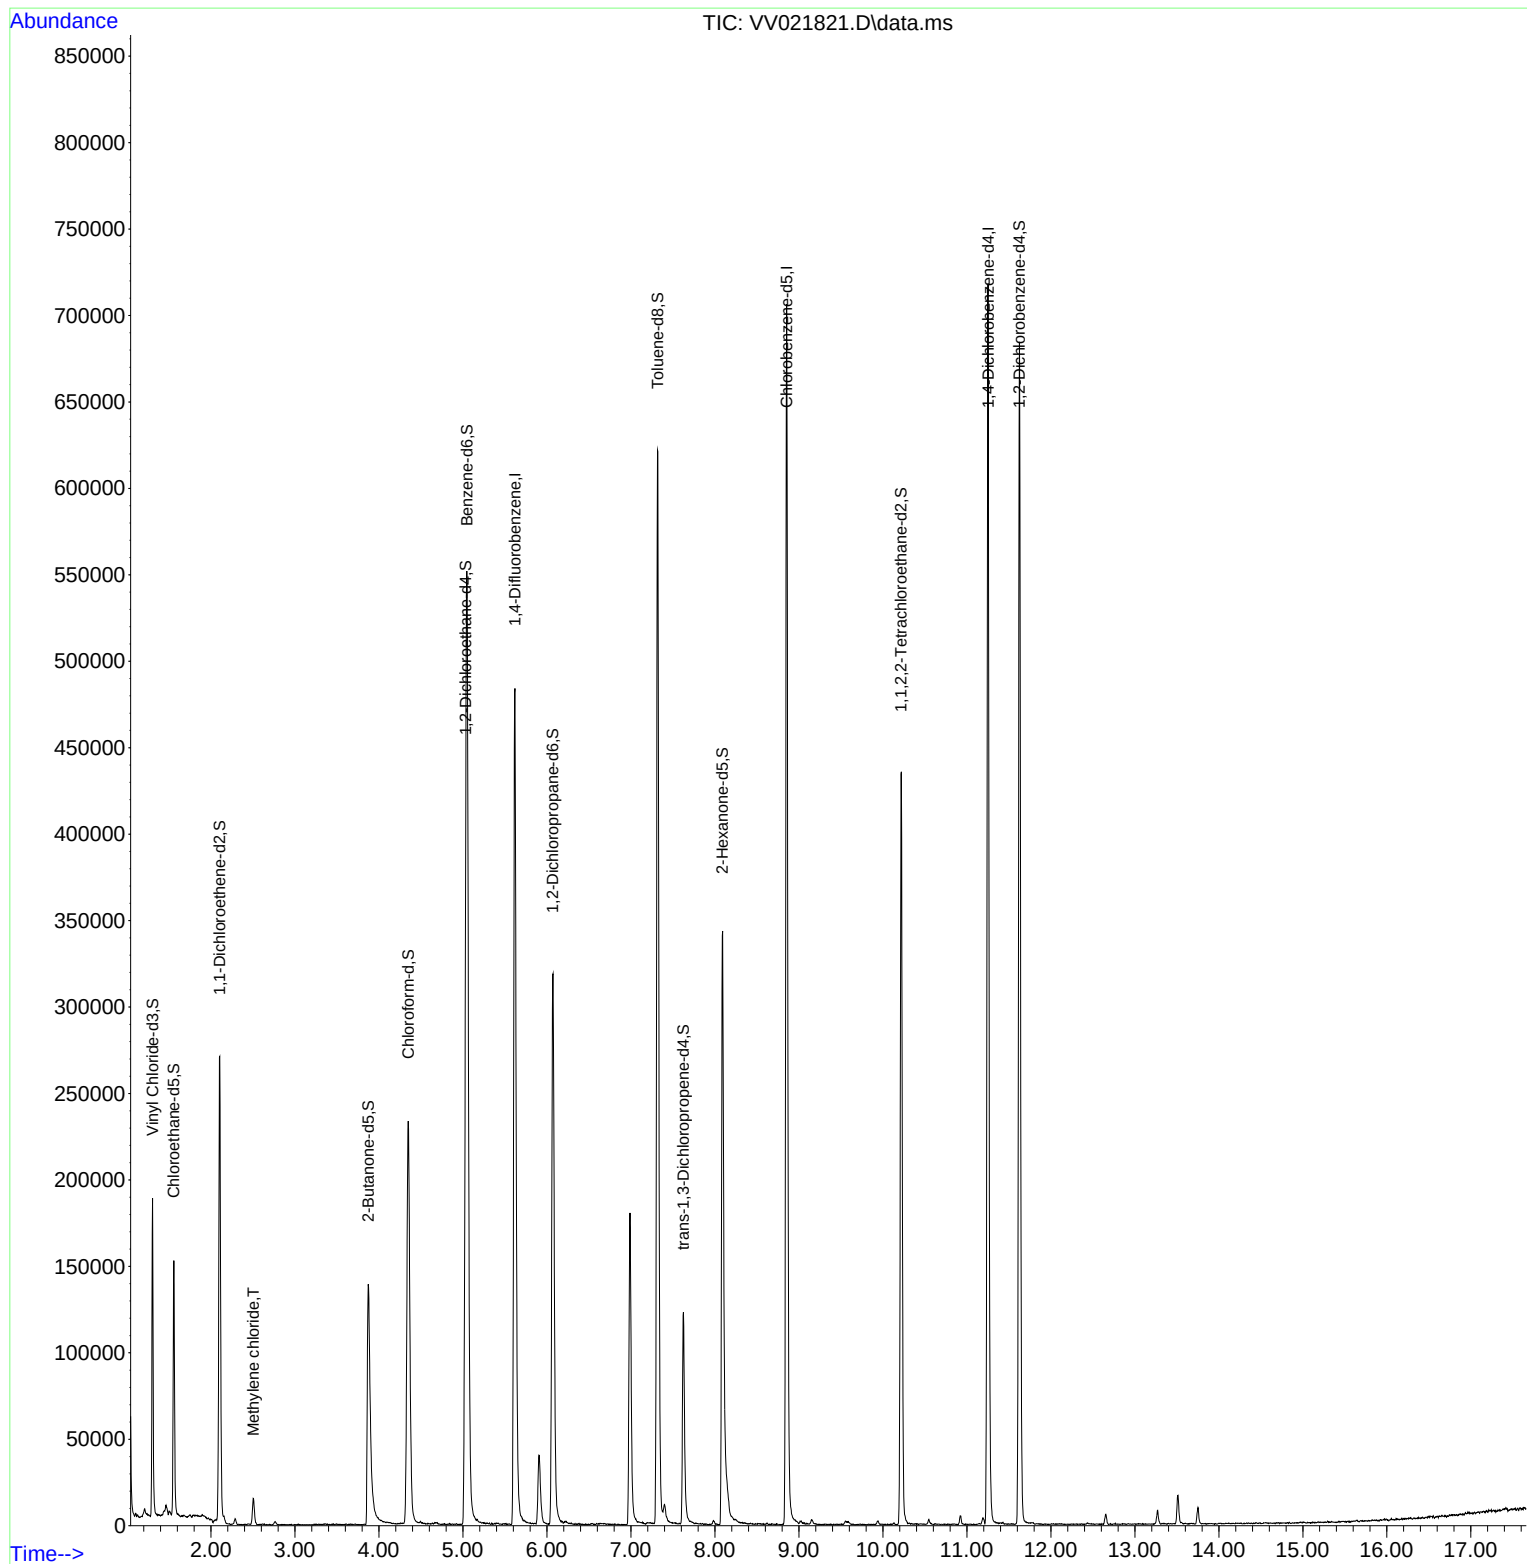

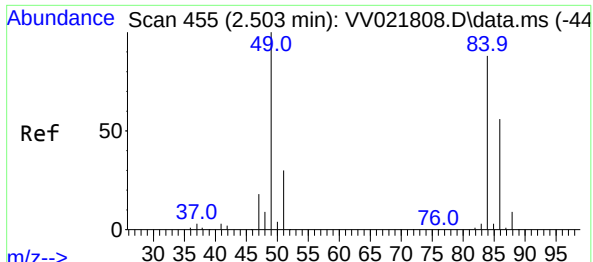

#16
Methylene chloride
Concen: 1.742 ug/L
RT: 2.506 min Scan# 456
Delta R.T. 0.003 min
Lab File: VV021821.D
Acq: 17 Aug 2021 18:11

Instrument :
MSVOA_V
ClientSampleId :
DBKCOME

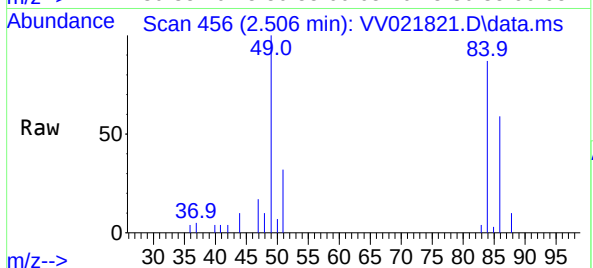

Tgt Ion:	84	Resp:	6360
Ion	Ratio	Lower	Upper
84	100		
86	67.8	44.7	83.1
49	114.4	82.5	153.3

