

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081721\
 Data File : VV021825.D
 Acq On : 17 Aug 2021 19:47
 Operator : SY/MD
 Sample : VV0817MBL02
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK234

Quant Time: Aug 18 03:35:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 18 03:33:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	413221	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	384610	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	186871	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	140364	43.451	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	86.900%		
7) Chloroethane-d5	1.558	69	117078	48.027	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	96.060%		
11) 1,1-Dichloroethene-d2	2.105	63	167452	32.565	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	65.120%		
21) 2-Butanone-d5	3.873	46	228158	113.561	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	113.560%		
24) Chloroform-d	4.349	84	281285	50.258	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.520%		
26) 1,2-Dichloroethane-d4	5.034	65	177553	55.151	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	110.300%		
32) Benzene-d6	5.050	84	585502	52.939	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	105.880%		
36) 1,2-Dichloropropane-d6	6.072	67	188943	54.858	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	109.720%		
41) Toluene-d8	7.317	98	527235	51.575	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	103.160%		
43) trans-1,3-Dichloroprop...	7.622	79	85341	50.347	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	100.700%		
47) 2-Hexanone-d5	8.088	63	127044	112.544	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	112.540%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	231674	54.280	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	108.560%		
66) 1,2-Dichlorobenzene-d4	11.625	152	205883	53.236	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	106.480%		
Target Compounds						Qvalue
16) Methylene chloride	2.507	84	6994	2.058	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081721\
Data File : VV021825.D
Acq On : 17 Aug 2021 19:47
Operator : SY/MD
Sample : VV0817MBL02
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK234


Quant Time: Aug 18 03:35:30 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 18 03:33:12 2021
Response via : Initial Calibration

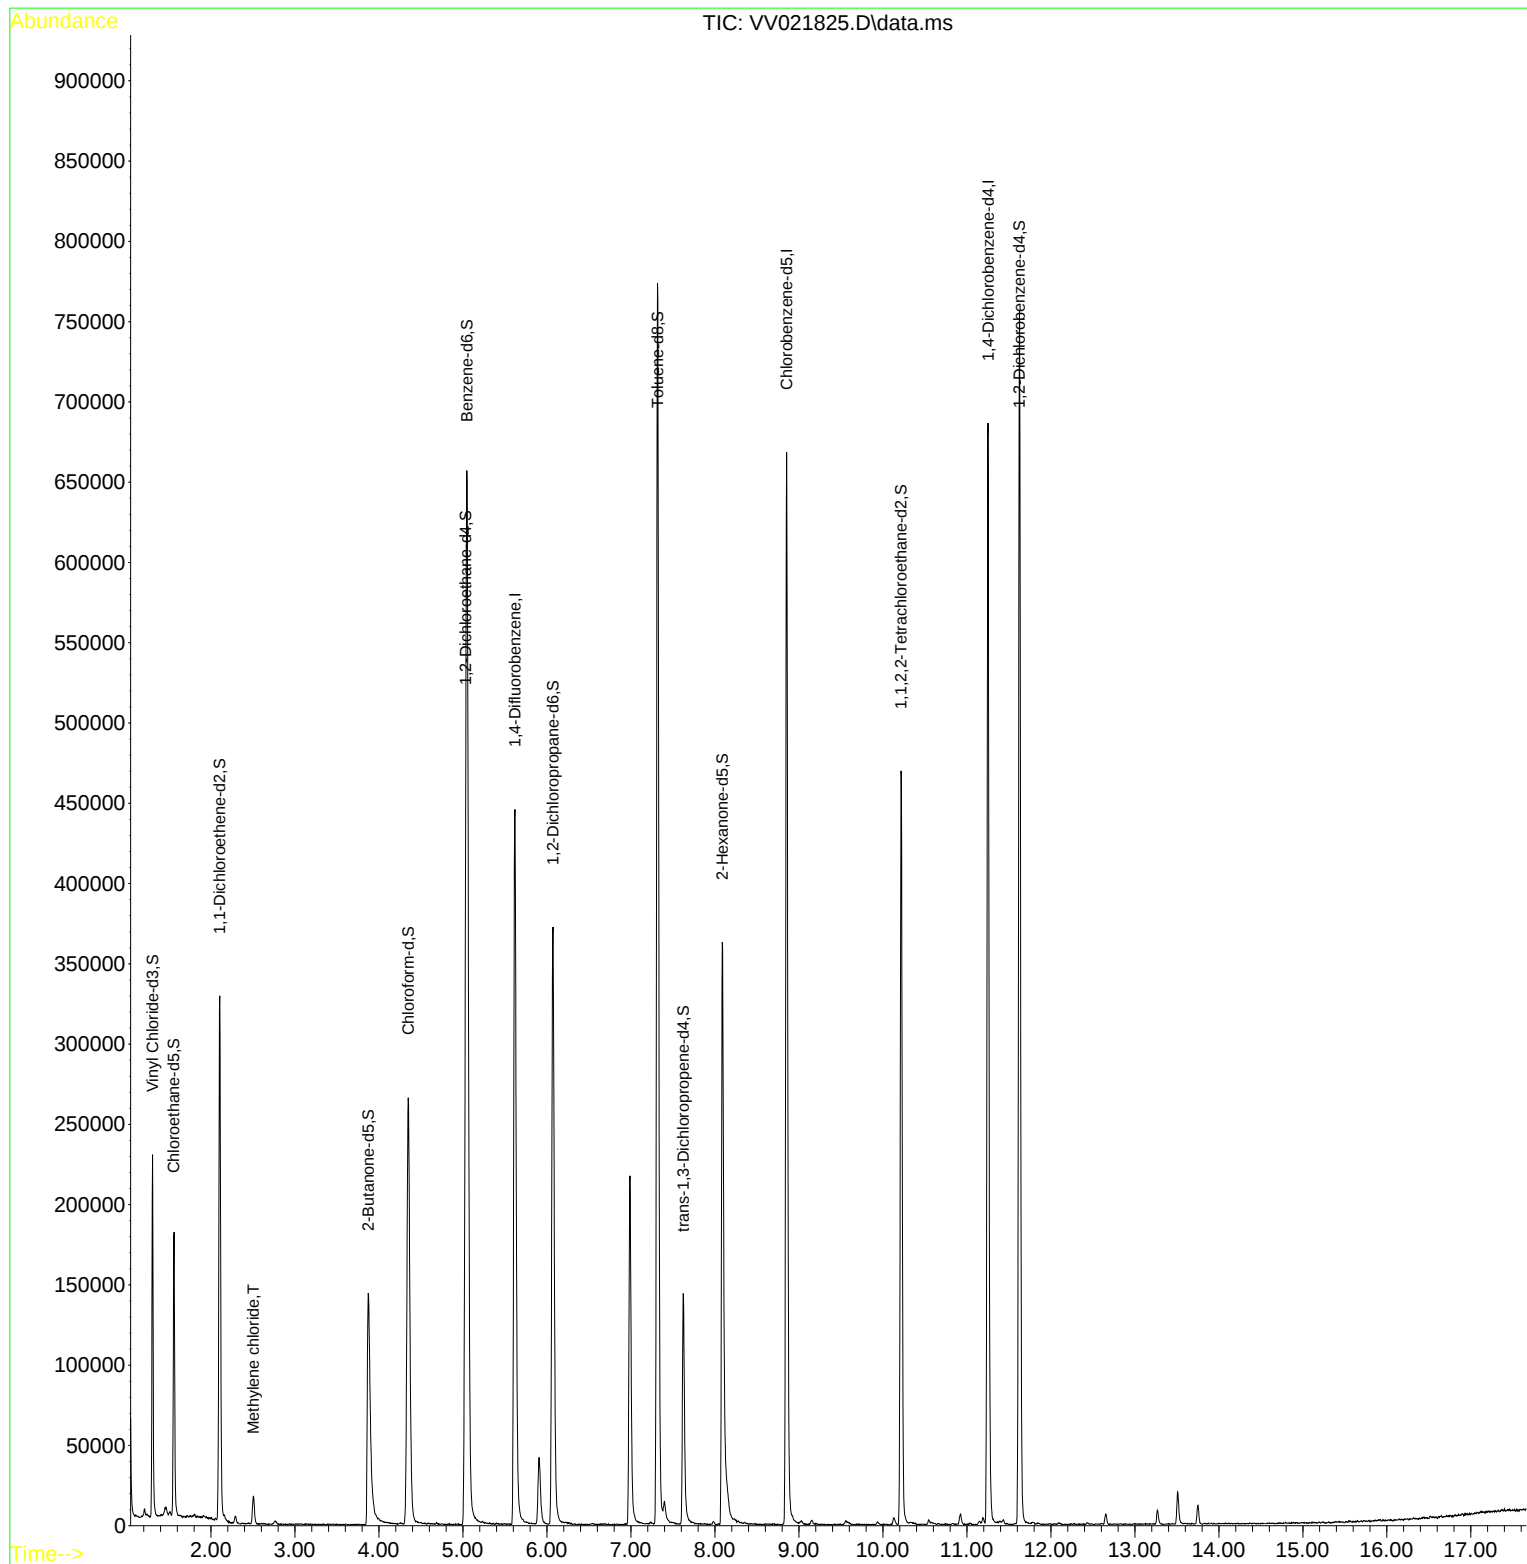

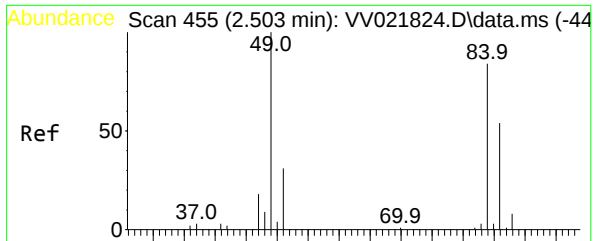

#16
Methylene chloride
Concen: 2.058 ug/L
RT: 2.507 min Scan# 456
Delta R.T. 0.003 min
Lab File: VV021825.D
Acq: 17 Aug 2021 19:47

Instrument :
MSVOA_V
ClientSampleId :
VBLK234

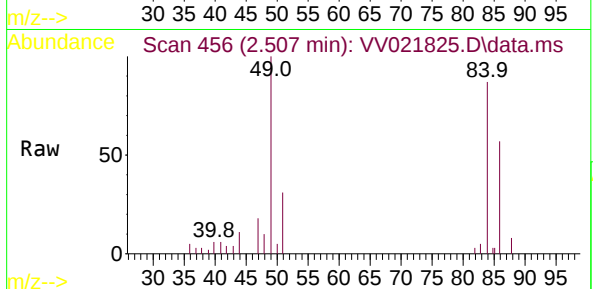

Tgt Ion:	84	Resp:	6994
Ion	Ratio	Lower	Upper
84	100		
86	66.0	44.7	83.1
49	115.0	82.5	153.3

