


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081721\
 Data File : VV021807.D
 Acq On : 17 Aug 2021 09:18
 Operator : SY/MD
 Sample : BFB216
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB216

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Title : VOC Analysis
 Last Update : Thu Aug 19 01:14:55 2021

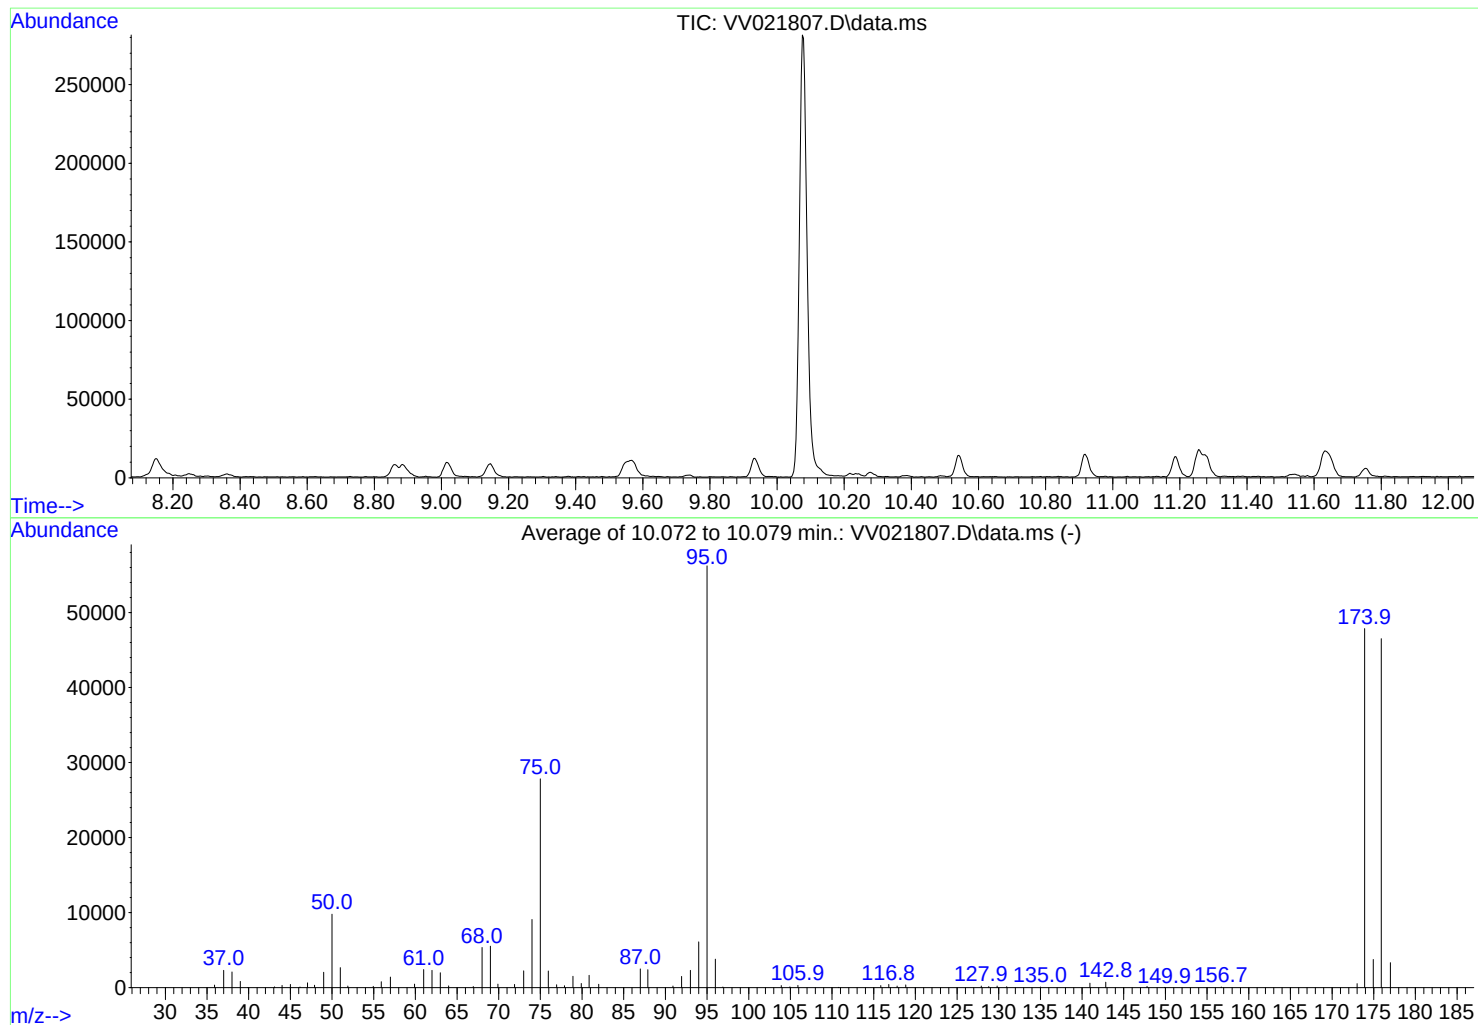

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	9797	PASS
75	95	30	80	49.5	27824	PASS
95	95	100	100	100.0	56221	PASS
96	95	5	9	6.7	3793	PASS
173	174	0.00	2	1.1	535	PASS
174	95	50	120	85.1	47853	PASS
175	174	5	9	7.8	3746	PASS
176	174	95	105	97.2	46515	PASS
177	176	5	10	7.2	3331	PASS

m/z	Abundance
35.90	339.0
37.00	2455.0
38.00	2151.0
39.00	858.0
39.90	244.0
43.10	131.0
44.00	640.0
45.00	443.0
46.20	121.0
47.10	628.0
47.90	331.0
49.00	2111.0
50.00	10120.0
51.00	2721.0
51.90	217.0
55.00	188.0
55.90	808.0
57.00	1466.0
59.90	478.0
61.00	2498.0
62.00	2385.0
63.00	2076.0
64.00	256.0
66.90	157.0
68.00	5540.0
69.00	5760.0
69.90	513.0
71.90	435.0
73.00	2303.0
74.00	9352.0
75.00	28832.0
76.00	2250.0
77.00	411.0
77.90	258.0
78.90	1583.0
79.90	570.0
80.90	1676.0
82.00	463.0
87.00	2582.0
87.90	2486.0
90.90	200.0
91.90	1517.0
93.00	2349.0
94.00	6240.0
95.00	58240.0
96.00	3908.0
96.90	117.0
103.90	298.0
105.00	104.0
105.90	322.0
115.80	298.0
116.80	447.0
117.80	236.0
118.80	380.0
127.90	239.0
128.80	145.0
129.80	204.0
131.00	133.0
135.00	121.0
141.00	632.0
142.80	758.0
147.80	165.0
156.70	121.0
173.00	566.0
173.90	49544.0
174.90	3916.0
175.90	48048.0
177.00	3474.0

Instrument :
MSVOA_V
ClientSampleId :
BFB216

Scan 2798 (10.037 min): VV021807.D\data.ms
BFB216

m/z	Abundance
39.90	227.0
44.00	342.0

Instrument :
MSVOA_V
ClientSampleId :
BFB216

m/z	Abundance
35.90	321.0
37.00	2215.0
38.00	1903.0
39.00	840.0
40.00	257.0
44.00	732.0
45.00	420.0
47.00	616.0
48.00	299.0
49.00	2209.0
50.00	9508.0
51.00	2523.0
51.90	189.0
55.00	200.0
55.90	843.0
57.00	1289.0
59.90	514.0
61.00	2215.0
62.00	2224.0
63.00	1905.0
64.00	233.0
67.00	144.0
68.00	5095.0
69.00	5276.0
69.90	446.0
71.90	367.0
73.00	2153.0
74.00	8609.0
75.00	26736.0
75.90	2134.0
76.90	351.0
78.00	245.0
78.90	1474.0
79.90	537.0
80.90	1584.0
82.00	361.0
87.00	2308.0
87.90	2205.0
90.90	212.0
91.90	1529.0
93.00	2161.0
94.00	6065.0
95.00	52976.0
96.00	3552.0
96.90	154.0
103.90	289.0
105.00	126.0
105.90	240.0
115.80	263.0
116.80	388.0
117.70	181.0
118.90	405.0
127.90	232.0
128.80	133.0
129.80	168.0
131.00	125.0
141.00	624.0
142.80	734.0
147.70	155.0
156.70	131.0
173.00	473.0
173.90	43448.0
174.90	3537.0
175.90	42672.0
177.00	3084.0

Instrument :
MSVOA_V
ClientSampleId :
BFB216

m/z	Abundance
35.90	373.0
37.00	2275.0
38.00	2193.0
39.00	810.0
39.90	268.0
43.10	162.0
44.00	579.0
45.00	447.0
46.10	127.0
47.00	668.0
47.80	326.0
49.00	1827.0
50.00	9763.0
51.00	2749.0
51.90	206.0
54.90	152.0
55.90	690.0
57.00	1493.0
59.90	392.0
61.00	2494.0
62.00	2301.0
63.00	1947.0
64.00	233.0
66.90	180.0
68.00	5440.0
69.00	5521.0
69.90	474.0
71.90	484.0
73.00	2283.0
74.00	9300.0
75.00	27904.0
76.00	2248.0
77.00	366.0
77.80	260.0
78.90	1518.0
79.90	548.0
80.80	1684.0
82.00	516.0
87.00	2607.0
87.90	2505.0
90.90	203.0
92.00	1423.0
93.00	2399.0
94.00	6020.0
95.00	57448.0
96.00	3919.0
103.90	256.0
104.90	110.0
105.90	338.0
110.80	102.0
115.90	291.0
116.80	442.0
117.90	257.0
118.80	290.0
127.90	201.0
128.80	146.0
129.80	252.0
130.90	114.0
135.00	131.0
140.90	565.0
142.90	707.0
147.90	180.0
149.90	107.0
173.00	565.0
173.90	50568.0
175.00	3785.0
175.90	48824.0
177.00	3434.0

Instrument :
MSVOA_V
ClientSampleId :
BFB216