
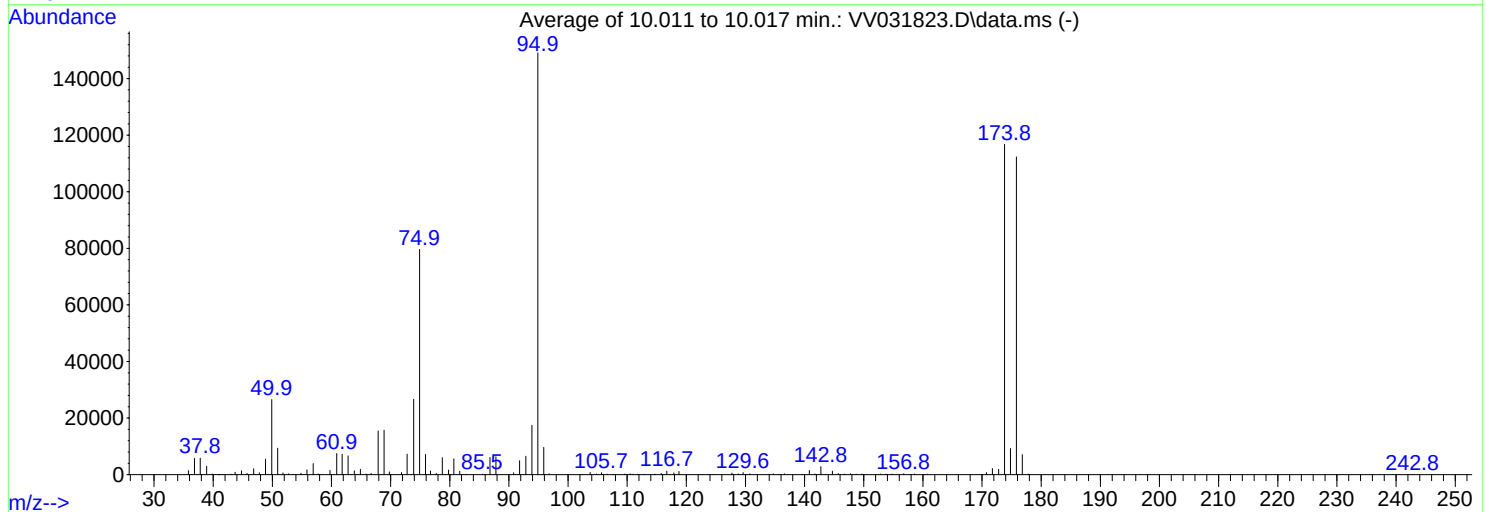


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081723\
 Data File : VV031823.D
 Acq On : 17 Aug 2023 10:42
 Operator : SY/MD
 Sample : BFB286
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB286

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081723WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Aug 18 02:24:23 2023

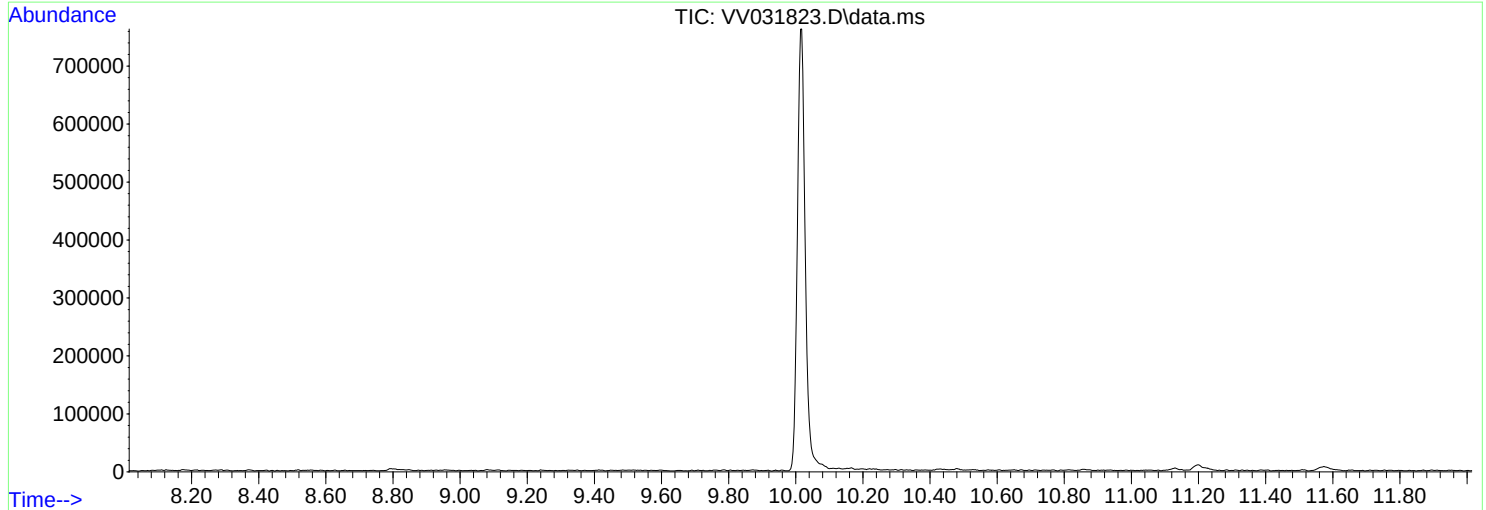

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	26557	PASS
75	95	30	80	53.4	79635	PASS
95	95	100	100	100.0	149099	PASS
96	95	5	9	6.4	9610	PASS
173	174	0.00	2	1.6	1867	PASS
174	95	50	120	78.3	116731	PASS
175	174	5	9	7.9	9248	PASS
176	174	95	105	96.2	112317	PASS
177	176	5	10	6.3	7095	PASS

m/z	Abundance
35.80	1346.0
36.90	6116.0
37.80	5553.0
38.90	2947.0
39.90	580.0
41.00	217.0
43.00	271.0
43.80	1460.0
44.80	1388.0
45.80	435.0
46.80	2131.0
47.80	694.0
48.80	5481.0
49.90	27432.0
50.90	9589.0
51.80	548.0
52.80	263.0
53.50	133.0
54.00	159.0
54.90	461.0
55.90	1866.0
56.90	3955.0
57.80	227.0
59.70	1369.0
60.90	7684.0
61.80	7252.0
62.80	6701.0
63.80	1319.0
64.90	1919.0
65.80	278.0
66.70	435.0
67.90	15989.0
68.90	16199.0
69.80	998.0
71.90	733.0
72.80	7782.0
73.90	26752.0
74.90	81952.0
75.90	6909.0
76.80	1321.0
77.70	606.0
78.80	5853.0
79.80	1630.0
80.70	5734.0
81.70	1136.0
82.70	137.0
85.60	177.0
86.80	5931.0
87.80	6106.0
90.80	705.0
91.80	5034.0
92.80	6916.0
93.90	18064.0
94.90	153536.0
95.90	9844.0
96.80	211.0
103.70	775.0
104.80	250.0
105.60	586.0
106.70	141.0
107.60	132.0
109.60	183.0
110.50	203.0
111.00	223.0
111.80	228.0
112.90	182.0
114.80	238.0
115.70	506.0
116.70	1162.0
117.90	611.0
118.80	1012.0
122.70	123.0
127.70	689.0
128.70	284.0
129.60	788.0
130.70	275.0
134.70	310.0
135.60	112.0
136.60	345.0
139.60	118.0
140.80	1682.0
141.70	248.0
142.70	2819.0
143.60	105.0
144.70	1369.0
145.70	383.0
146.70	174.0
147.80	439.0
148.70	146.0
149.70	277.0
152.80	236.0
153.80	151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB286

154.90	279.0
156.70	361.0
157.90	119.0
158.60	195.0
160.20	123.0
160.70	169.0
170.70	792.0
171.80	2336.0
172.80	1887.0
173.80	123656.0
174.80	9237.0
175.80	119224.0
176.80	7413.0
177.90	169.0

Instrument :
MSVOA_V
ClientSampleId :
BFB286

m/z	Abundance
35.10	105.0
36.60	102.0
38.10	121.0
39.80	297.0
40.90	109.0
43.60	612.0
55.70	120.0
56.90	117.0
68.60	170.0
77.80	105.0
92.30	119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB286

m/z	Abundance
35.80	1424.0
36.80	5221.0
37.80	5810.0
38.90	2898.0
39.90	448.0
40.40	152.0
41.60	159.0
43.80	1471.0
44.80	1253.0
45.70	297.0
46.90	1950.0
47.80	677.0
48.90	5368.0
49.90	24840.0
50.90	8682.0
51.80	659.0
52.70	257.0
53.50	107.0
54.80	507.0
55.90	1811.0
56.90	3989.0
57.70	213.0
58.40	106.0
59.80	1595.0
60.90	7044.0
61.80	6880.0
62.80	6280.0
63.90	1330.0
64.90	1742.0
65.90	219.0
66.70	425.0
67.90	14321.0
68.90	14708.0
69.80	975.0
71.80	706.0
72.80	6412.0
73.90	25528.0
74.90	74816.0
75.90	7106.0
76.70	1269.0
77.70	485.0
78.70	5921.0
79.80	1562.0
80.70	5252.0
81.70	1198.0
82.90	120.0
85.50	121.0
85.80	102.0
86.80	6007.0
87.80	6358.0
90.80	596.0
91.80	4605.0
92.90	6045.0
93.90	16310.0
94.90	139648.0
95.90	8970.0
96.80	324.0
102.40	236.0
103.70	749.0
104.80	267.0
105.70	764.0
106.70	132.0
109.60	249.0
110.50	343.0
111.80	104.0
114.60	311.0
115.70	475.0
116.70	1313.0
117.90	626.0
118.70	1257.0
123.80	120.0
127.70	461.0
128.90	332.0
129.60	672.0
130.80	269.0
134.80	288.0
135.70	122.0
136.60	240.0
140.80	1242.0
141.80	159.0
142.80	2815.0
143.60	168.0
144.70	1187.0
145.70	407.0
146.80	137.0
147.70	302.0
148.70	151.0
149.70	124.0
152.80	184.0
153.70	128.0
154.70	226.0
156.80	263.0

Instrument :
MSVOA_V
ClientSampleId :
BFB286

158.60	205.0
160.80	142.0
170.80	708.0
171.70	1963.0
172.80	1798.0
173.80	105864.0
174.80	8812.0
175.80	101808.0
176.80	6552.0
177.80	330.0
242.80	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB286

m/z	Abundance
35.80	1444.0
36.90	5740.0
37.80	6154.0
38.90	3081.0
39.90	586.0
40.40	218.0
41.00	157.0
41.60	135.0
43.00	230.0
43.80	1508.0
44.80	1438.0
45.80	396.0
46.90	2183.0
47.80	704.0
48.90	5552.0
49.90	27400.0
50.90	9788.0
51.80	665.0
52.80	284.0
53.50	128.0
54.90	532.0
55.90	1798.0
56.90	4182.0
57.80	220.0
59.70	1536.0
60.90	7696.0
61.80	7357.0
62.80	6842.0
63.90	1362.0
64.90	1973.0
65.90	254.0
66.70	460.0
67.90	16030.0
68.90	16287.0
69.80	996.0
71.90	721.0
72.80	7535.0
73.90	27648.0
74.90	82136.0
75.90	7398.0
76.70	1386.0
77.70	545.0
78.80	6160.0
79.80	1751.0
80.70	5797.0
81.70	1172.0
82.80	135.0
85.40	157.0
85.90	121.0
86.80	6393.0
87.80	6589.0
90.80	720.0
91.80	5200.0
92.80	6565.0
93.90	17936.0
94.90	154112.0
95.90	10017.0
96.80	296.0
102.40	173.0
103.80	802.0
104.80	282.0
105.60	778.0
106.70	164.0
109.60	241.0
110.50	314.0
111.00	224.0
111.80	168.0
112.90	142.0
114.60	271.0
115.80	481.0
116.70	1306.0
117.90	642.0
118.70	1200.0
124.60	107.0
127.70	609.0
128.80	326.0
129.60	717.0
130.70	319.0
134.70	333.0
135.70	139.0
136.60	303.0
139.70	103.0
140.80	1511.0
141.70	227.0
142.80	2929.0
143.60	108.0
144.70	1251.0
145.70	424.0
146.70	169.0
147.70	364.0
148.70	158.0
149.70	230.0

Instrument :
MSVOA_V
ClientSampleId :
BFB286

152.80	255.0
153.80	177.0
154.80	228.0
156.70	348.0
157.90	118.0
158.60	216.0
160.30	120.0
160.80	184.0
170.70	773.0
171.70	2232.0
172.80	1915.0
173.80	120672.0
174.80	9696.0
175.80	115920.0
176.80	7321.0
177.80	260.0

Instrument :
MSVOA_V
ClientSampleId :
BFB286