


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081820\
 Data File : VV018040.D
 Acq On : 18 Aug 2020 09:07
 Operator : SY/MD
 Sample : BFB76
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB76

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Title : VOC Analysis
 Last Update : Thu Aug 20 01:57:03 2020

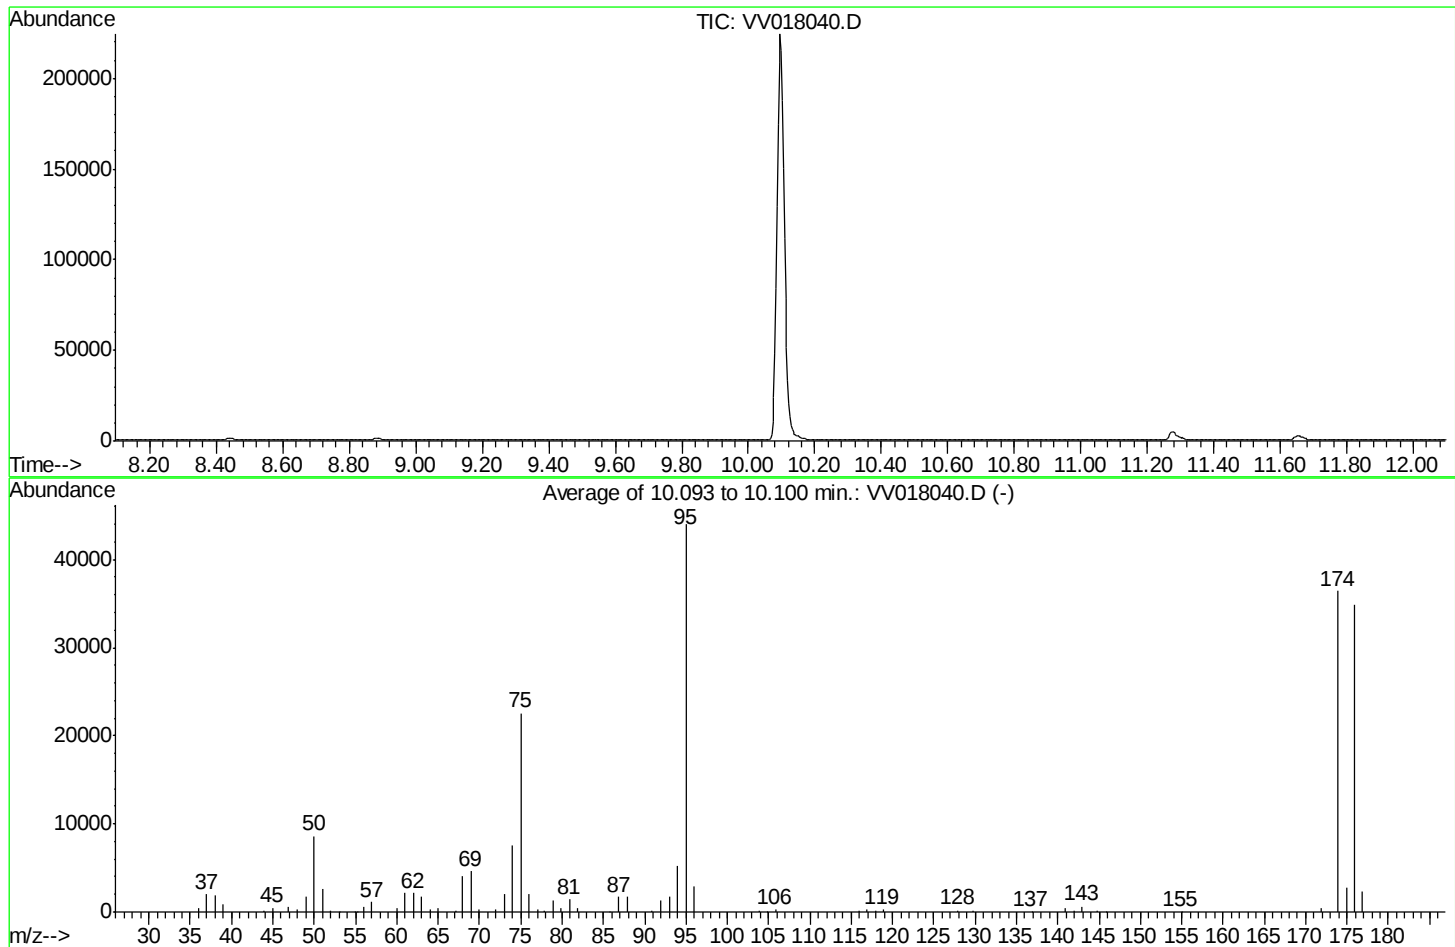

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	8634	PASS
75	95	30	80	51.3	22568	PASS
95	95	100	100	100.0	43997	PASS
96	95	5	9	6.7	2934	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.7	36402	PASS
175	174	5	9	7.6	2762	PASS
176	174	95	101	95.6	34810	PASS
177	176	5	9	6.6	2308	PASS

Scan 2790 (10.061 min): VV018040.D
BFB76

m/z	Abundance
40.00	207.0
43.90	279.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

m/z	Abundance
35.00	415.0
37.00	1886.0
38.00	1901.0
39.00	889.0
40.00	217.0
44.00	524.0
44.90	411.0
46.90	581.0
48.00	280.0
49.00	1672.0
50.00	8477.0
51.00	2637.0
52.00	150.0
53.00	101.0
55.20	114.0
56.00	600.0
57.00	1105.0
60.00	403.0
61.00	2040.0
62.00	2071.0
63.00	1732.0
64.00	256.0
64.90	435.0
67.00	138.0
68.00	3815.0
69.00	4558.0
69.90	394.0
72.00	306.0
73.00	1996.0
74.00	7303.0
75.00	22184.0
76.00	2081.0
77.00	234.0
77.90	245.0
78.90	1283.0
79.90	413.0
80.90	1361.0
81.90	381.0
86.90	1761.0
88.00	1668.0
90.80	142.0
91.90	1264.0
93.00	1787.0
94.00	5247.0
95.00	42720.0
96.00	2990.0
103.90	189.0
105.80	244.0
115.90	161.0
117.00	272.0
117.90	161.0
118.80	257.0
127.90	184.0
129.70	166.0
136.90	107.0
140.90	446.0
142.90	602.0
144.80	164.0
155.00	117.0
171.90	435.0
173.90	34720.0
174.90	2736.0
175.90	32888.0
176.90	2234.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

m/z	Abundance
36.00	431.0
37.00	2035.0
38.00	1936.0
39.00	956.0
40.00	211.0
44.00	482.0
44.90	446.0
46.90	653.0
47.90	307.0
49.00	1776.0
50.00	8987.0
51.00	2767.0
52.00	165.0
55.10	115.0
56.00	672.0
57.00	1149.0
60.00	418.0
61.00	2182.0
62.00	2245.0
63.00	1861.0
64.00	266.0
65.00	457.0
67.10	137.0
68.00	4274.0
69.00	4791.0
70.00	353.0
72.00	333.0
73.00	2186.0
74.00	7856.0
75.00	23400.0
76.00	2094.0
77.00	250.0
77.90	214.0
78.90	1394.0
79.90	459.0
80.90	1465.0
81.90	431.0
85.80	106.0
86.90	1772.0
87.90	1786.0
90.80	185.0
91.90	1302.0
93.00	1840.0
94.00	5485.0
95.00	45576.0
96.00	3045.0
103.90	191.0
104.90	101.0
105.90	248.0
115.90	211.0
116.90	294.0
117.90	187.0
118.90	303.0
127.90	184.0
129.70	162.0
136.80	105.0
140.90	460.0
141.90	131.0
142.90	637.0
144.80	154.0
145.80	101.0
154.90	104.0
171.90	509.0
173.90	37736.0
174.90	2858.0
175.90	36128.0
176.90	2410.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

m/z	Abundance
36.00	407.0
37.00	2053.0
38.00	1813.0
39.00	917.0
40.00	184.0
44.00	452.0
45.00	460.0
46.90	665.0
47.90	296.0
49.00	1692.0
50.00	8439.0
51.00	2620.0
52.00	150.0
54.90	119.0
56.00	674.0
57.00	1077.0
59.90	408.0
61.00	2140.0
62.00	2161.0
63.00	1806.0
64.00	267.0
65.00	417.0
67.20	126.0
68.00	4186.0
69.00	4484.0
70.00	301.0
72.00	294.0
73.00	2061.0
74.00	7576.0
75.00	22120.0
76.00	1915.0
77.00	262.0
77.90	173.0
78.90	1348.0
79.90	466.0
80.90	1383.0
81.90	436.0
85.80	109.0
86.90	1679.0
87.90	1756.0
90.80	202.0
91.90	1217.0
93.00	1774.0
94.00	5093.0
95.00	43696.0
96.00	2769.0
103.90	180.0
104.80	107.0
105.90	217.0
115.90	229.0
116.90	276.0
117.90	206.0
118.90	300.0
127.90	167.0
129.70	154.0
140.90	415.0
141.90	154.0
143.00	575.0
144.70	151.0
171.90	516.0
173.90	36752.0
174.90	2693.0
175.90	35416.0
176.90	2280.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76