

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
 Data File : VV021872.D
 Acq On : 18 Aug 2021 18:16
 Operator : SY/MD
 Sample : M3448-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 19 01:18:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 19 01:14:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	430648	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	402012	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	192545	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	141635	42.070	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	84.140%	
7) Chloroethane-d5	1.561	69	111935	44.059	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	88.120%	
11) 1,1-Dichloroethene-d2	2.105	63	108589	20.263	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	40.520%#	
21) 2-Butanone-d5	3.873	46	192885	92.120	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	92.120%	
24) Chloroform-d	4.349	84	254336	43.604	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	87.200%	
26) 1,2-Dichloroethane-d4	5.034	65	156993	46.792	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	93.580%	
32) Benzene-d6	5.050	84	536185	46.381	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	92.760%	
36) 1,2-Dichloropropane-d6	6.072	67	168377	46.771	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	93.540%	
41) Toluene-d8	7.317	98	485481	45.435	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	90.880%	
43) trans-1,3-Dichloroprop...	7.625	79	72586	40.969	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	81.940%	
47) 2-Hexanone-d5	8.088	63	116716	98.919	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	98.920%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	219315	49.160	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	98.320%	
66) 1,2-Dichlorobenzene-d4	11.625	152	187056	46.943	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	93.880%	
Target Compounds						
44) trans-1,3-Dichloropropene	7.622	75	2782	0.595	ug/L	Qvalue # 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
Data File : VV021872.D
Acq On : 18 Aug 2021 18:16
Operator : SY/MD
Sample : M3448-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Aug 19 01:18:53 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 19 01:14:55 2021
Response via : Initial Calibration

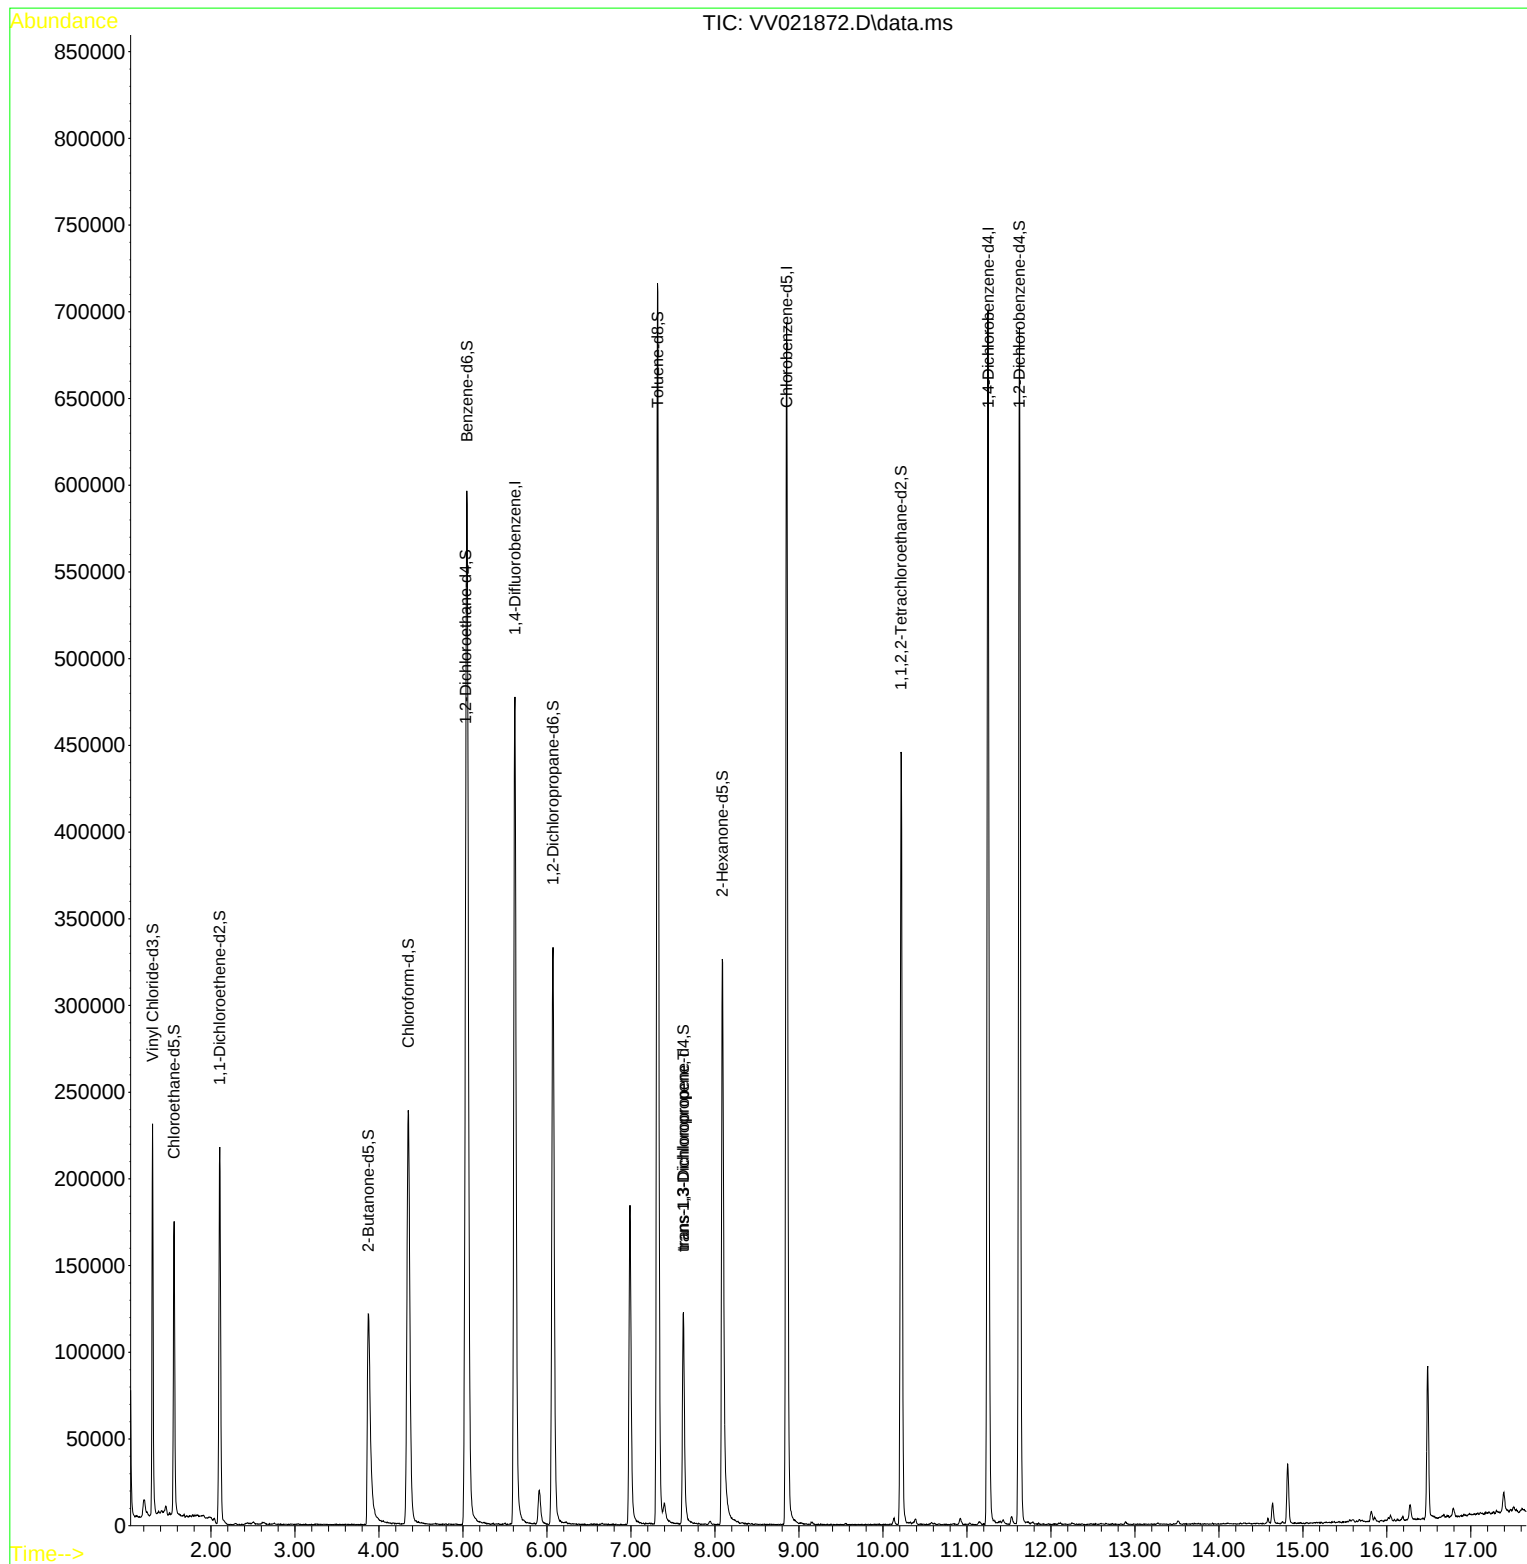

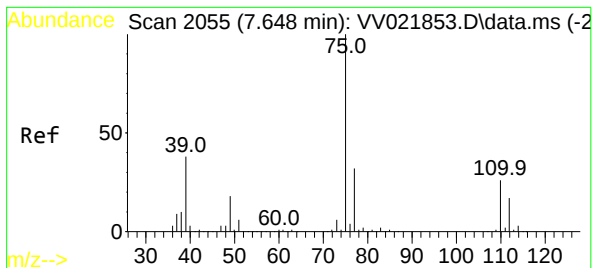

#44
 trans-1,3-Dichloropropene
 Concen: 0.595 ug/L
 RT: 7.622 min Scan# 2047
 Delta R.T. -0.026 min
 Lab File: VV021872.D
 Acq: 18 Aug 2021 18:16

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 2782
 Ion Ratio Lower Upper
 75 100
 77 41.3 22.2 41.2#

