

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
 Data File : VV021860.D
 Acq On : 18 Aug 2021 13:02
 Operator : SY/MD
 Sample : M3422-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKA5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M

Title : VOC Analysis

Signal : TIC: VV021860.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rBV	228430	229708	14.91%	1.999%
2	1.558	154	161	179	rVB	171353	205583	13.34%	1.789%
3	2.105	321	331	345	rBV	329762	453830	29.45%	3.948%
4	2.497	449	453	454	rBV3	1325	892	0.06%	0.008%
5	2.545	466	468	471	rBV2	702	373	0.02%	0.003%
6	2.587	479	481	486	rBV3	408	341	0.02%	0.003%
7	2.619	486	491	496	rBV5	1195	1450	0.09%	0.013%
8	2.770	525	538	555	rBV2	18268	39421	2.56%	0.343%
9	2.973	599	601	603	rBV2	355	183	0.01%	0.002%
10	3.002	607	610	613	rBV2	379	272	0.02%	0.002%
11	3.133	647	651	652	rBV2	290	189	0.01%	0.002%
12	3.297	698	702	707	rBV3	780	732	0.05%	0.006%
13	3.349	714	718	720	rBV	295	189	0.01%	0.002%
14	3.394	730	732	735	rBV2	547	293	0.02%	0.003%
15	3.487	758	761	764	rBV2	356	212	0.01%	0.002%
16	3.542	775	778	781	rBV	308	262	0.02%	0.002%
17	3.664	812	816	817	rBV	250	172	0.01%	0.001%
18	3.738	836	839	841	rBV2	404	233	0.02%	0.002%
19	3.773	848	850	852	rBV3	476	269	0.02%	0.002%
20	3.799	856	858	863	rVB3	331	242	0.02%	0.002%
21	3.876	872	882	917	rBV	125654	335161	21.75%	2.916%
22	4.349	1012	1029	1058	rBV	239494	598140	38.82%	5.204%
23	4.674	1128	1130	1133	rVB2	444	226	0.01%	0.002%
24	4.712	1140	1142	1146	rBV2	277	175	0.01%	0.002%
25	4.966	1220	1221	1227	rVB3	476	338	0.02%	0.003%
26	5.047	1227	1246	1273	rBV2	606299	1540869	100.00%	13.406%
27	5.487	1380	1383	1384	rBV2	466	246	0.02%	0.002%
28	5.619	1411	1424	1454	rBV	444202	909371	59.02%	7.912%
29	5.908	1503	1514	1536	rBV3	18868	39532	2.57%	0.344%
30	6.072	1550	1565	1590	rBV	336779	688694	44.70%	5.992%
31	6.371	1657	1658	1661	rBV	311	187	0.01%	0.002%
32	6.526	1703	1706	1707	rBV	331	184	0.01%	0.002%
33	6.583	1720	1724	1725	rBV2	406	322	0.02%	0.003%
34	6.612	1732	1733	1736	rBV	342	191	0.01%	0.002%
35	6.632	1736	1739	1740	rVV	371	208	0.01%	0.002%
36	6.683	1753	1755	1761	rVV3	532	365	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
 Data File : VV021860.D
 Acq On : 18 Aug 2021 13:02
 Operator : SY/MD
 Sample : M3422-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKA5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Title : VOC Analysis

37	6.709	1761	1763	1766	rVB2	499	306	0.02%	0.003%
38	6.747	1773	1775	1778	rVB	390	179	0.01%	0.002%
39	6.767	1778	1781	1785	rBV2	437	341	0.02%	0.003%
40	6.786	1785	1787	1788	rBV	398	190	0.01%	0.002%
41	6.837	1800	1803	1808	rBV	394	296	0.02%	0.003%
42	6.860	1808	1810	1813	rBV3	241	177	0.01%	0.002%
43	6.940	1830	1835	1839	rBV2	349	326	0.02%	0.003%
44	6.989	1839	1850	1873	rBV	186343	340334	22.09%	2.961%
45	7.320	1941	1953	1972	rBV	725656	1264756	82.08%	11.004%
46	7.625	2038	2048	2069	rBV	125169	219700	14.26%	1.911%
47	7.751	2085	2087	2091	rBV4	780	603	0.04%	0.005%
48	7.882	2126	2128	2131	rVB2	478	284	0.02%	0.002%
49	7.905	2131	2135	2136	rBV2	607	434	0.03%	0.004%
50	7.940	2142	2146	2153	rBV5	1122	1678	0.11%	0.015%
51	7.985	2153	2160	2171	rVB6	2144	3555	0.23%	0.031%
52	8.091	2183	2193	2235	rBV	340982	629001	40.82%	5.472%
53	8.448	2301	2304	2306	rBV2	325	212	0.01%	0.002%
54	8.593	2345	2349	2352	rBV3	428	384	0.02%	0.003%
55	8.628	2356	2360	2364	rVB3	481	452	0.03%	0.004%
56	8.693	2378	2380	2382	rBV2	514	259	0.02%	0.002%
57	8.853	2418	2430	2459	rBV	666143	1075492	69.80%	9.357%
58	9.291	2563	2566	2570	rVB3	401	249	0.02%	0.002%
59	9.313	2570	2573	2575	rBV	332	184	0.01%	0.002%
60	9.419	2602	2606	2608	rBV2	270	183	0.01%	0.002%
61	9.461	2616	2619	2620	rBV	342	182	0.01%	0.002%
62	9.522	2634	2638	2643	rBV2	612	619	0.04%	0.005%
63	9.554	2644	2648	2651	rBV2	848	609	0.04%	0.005%
64	9.680	2685	2687	2692	rVB4	459	336	0.02%	0.003%
65	9.722	2697	2700	2706	rBV2	406	318	0.02%	0.003%
66	9.789	2718	2721	2726	rVB	365	232	0.02%	0.002%
67	9.815	2726	2729	2732	rBV2	262	171	0.01%	0.001%
68	9.982	2779	2781	2784	rBV	344	213	0.01%	0.002%
69	10.088	2811	2814	2818	rBV3	406	330	0.02%	0.003%
70	10.133	2818	2828	2840	rVV4	3272	5581	0.36%	0.049%
71	10.220	2843	2855	2882	rBV	456341	724508	47.02%	6.303%
72	10.361	2893	2899	2904	rBV3	3201	4195	0.27%	0.036%
73	10.474	2932	2934	2937	rVV2	592	333	0.02%	0.003%
74	10.545	2954	2956	2958	rBV	407	218	0.01%	0.002%
75	10.921	3067	3073	3085	rVB7	3320	5434	0.35%	0.047%
76	11.027	3103	3106	3107	rBV2	686	350	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
 Data File : VV021860.D
 Acq On : 18 Aug 2021 13:02
 Operator : SY/MD
 Sample : M3422-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKA5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Title : VOC Analysis

77	11.075	3117	3121	3125	rBV3	264	269	0.02%	0.002%
78	11.149	3138	3144	3148	rBV5	1862	2321	0.15%	0.020%
79	11.252	3164	3176	3197	rBV	649463	1026328	66.61%	8.929%
80	11.464	3239	3242	3244	rBV	516	260	0.02%	0.002%
81	11.538	3262	3265	3268	rBV3	644	347	0.02%	0.003%
82	11.625	3280	3292	3317	rBV	702145	1107722	71.89%	9.637%
83	11.844	3356	3360	3362	rBV4	1023	813	0.05%	0.007%
84	12.008	3409	3411	3416	rVB2	781	477	0.03%	0.004%
85	12.085	3431	3435	3436	rBV3	684	447	0.03%	0.004%
86	12.300	3499	3502	3506	rVB2	502	346	0.02%	0.003%
87	12.368	3513	3523	3531	rBV7	3796	6016	0.39%	0.052%
88	12.474	3552	3556	3559	rBV5	3759	3815	0.25%	0.033%
89	12.657	3609	3613	3616	rBV2	489	409	0.03%	0.004%
90	12.828	3664	3666	3669	rBV	367	212	0.01%	0.002%
91	12.895	3683	3687	3689	rBV2	580	406	0.03%	0.004%
92	12.992	3714	3717	3723	rVB	400	400	0.03%	0.003%
93	13.024	3723	3727	3731	rBV2	401	329	0.02%	0.003%
94	13.075	3739	3743	3747	rBV2	418	466	0.03%	0.004%
95	13.172	3771	3773	3778	rBV2	346	271	0.02%	0.002%
96	13.230	3788	3791	3792	rBV2	377	201	0.01%	0.002%
97	13.271	3800	3804	3807	rBV2	346	265	0.02%	0.002%
98	13.448	3856	3859	3865	rBV	656	558	0.04%	0.005%
99	13.509	3873	3878	3887	rBV6	2046	3133	0.20%	0.027%
100	13.631	3908	3916	3925	rBV4	3694	5912	0.38%	0.051%




Sum of corrected areas: 11493982

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
Data File : VV021860.D
Acq On : 18 Aug 2021 13:02
Operator : SY/MD
Sample : M3422-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

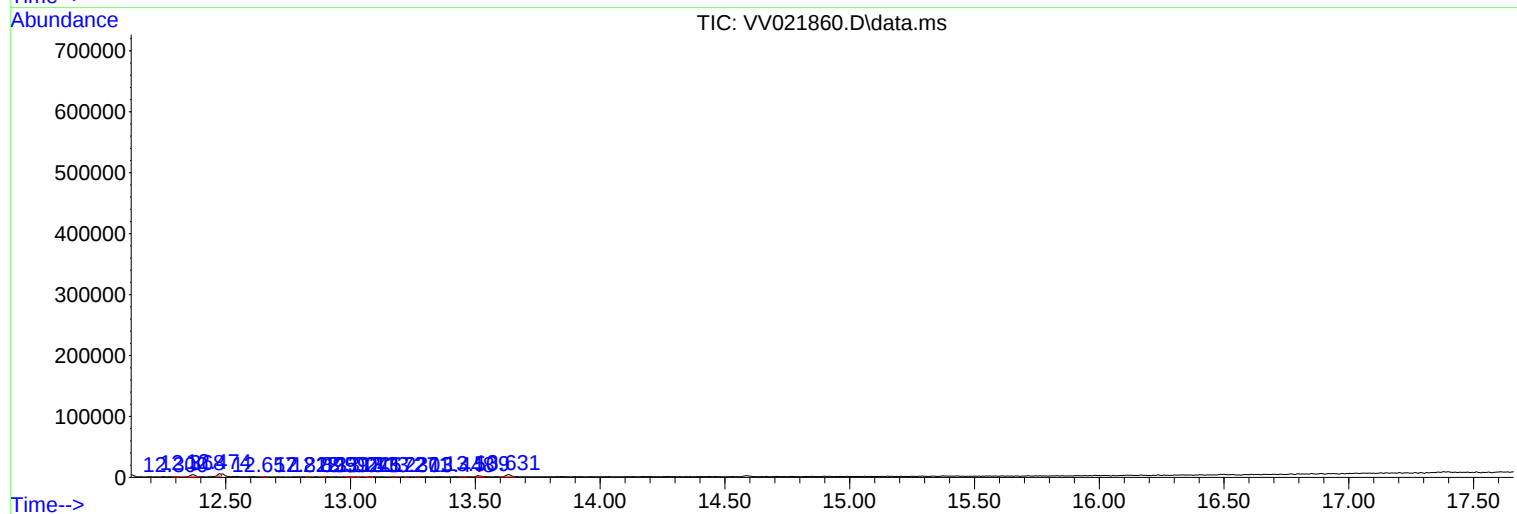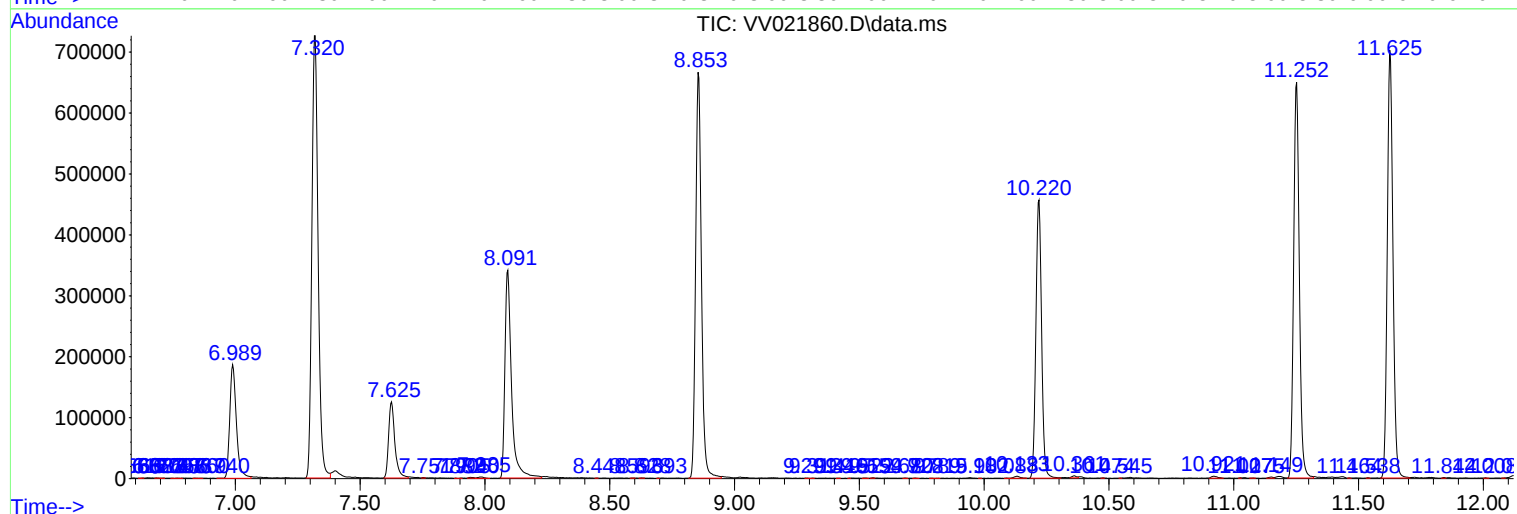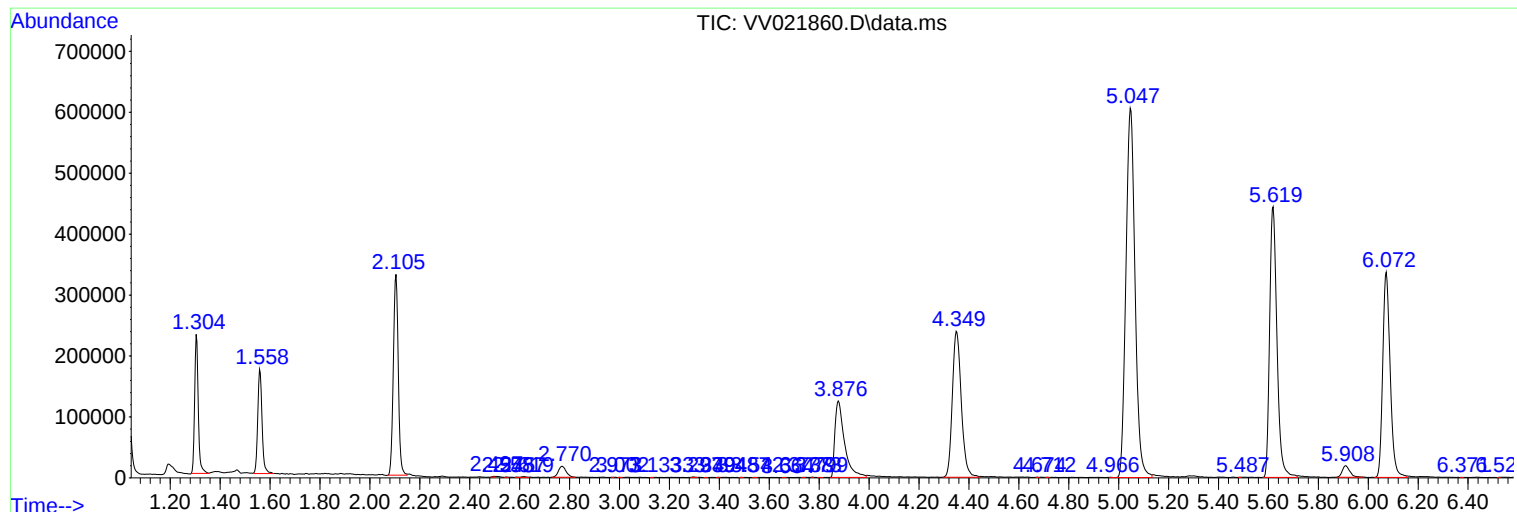

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
Data File : VV021860.D
Acq On : 18 Aug 2021 13:02
Operator : SY/MD
Sample : M3422-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
Data File : VV021860.D
Acq On : 18 Aug 2021 13:02
Operator : SY/MD
Sample : M3422-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
