

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
 Data File : VV021863.D
 Acq On : 18 Aug 2021 14:17
 Operator : SY/MD
 Sample : M3422-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKB1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Title : VOC Analysis

Signal : TIC: VV021863.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	98	rBV	230284	227167	15.20%	2.033%
2	1.558	155	161	173	rVB	164073	192192	12.86%	1.720%
3	2.101	321	330	345	rBV	311965	452207	30.25%	4.047%
4	2.388	417	419	422	rVB2	632	245	0.02%	0.002%
5	2.539	463	466	469	rBV	478	278	0.02%	0.002%
6	2.658	501	503	506	rBV2	427	243	0.02%	0.002%
7	2.773	528	539	548	rBV3	7080	13799	0.92%	0.123%
8	2.857	563	565	570	rVB2	591	334	0.02%	0.003%
9	2.896	570	577	581	rBV3	449	475	0.03%	0.004%
10	2.973	597	601	602	rBV	382	321	0.02%	0.003%
11	3.027	614	618	621	rVB3	371	274	0.02%	0.002%
12	3.076	631	633	638	rVB3	605	417	0.03%	0.004%
13	3.095	638	639	643	rVB2	541	255	0.02%	0.002%
14	3.121	643	647	652	rBV2	562	500	0.03%	0.004%
15	3.172	660	663	667	rVB2	318	216	0.01%	0.002%
16	3.211	670	675	676	rBV	315	239	0.02%	0.002%
17	3.249	685	687	691	rVB2	364	217	0.01%	0.002%
18	3.275	691	695	698	rBV3	443	299	0.02%	0.003%
19	3.297	698	702	704	rBV4	498	331	0.02%	0.003%
20	3.616	798	801	806	rVB2	350	284	0.02%	0.003%
21	3.777	847	851	854	rBV3	399	324	0.02%	0.003%
22	3.873	871	881	910	rBV2	122476	321684	21.52%	2.879%
23	4.275	1003	1006	1008	rBV2	438	298	0.02%	0.003%
24	4.349	1013	1029	1056	rVV	234737	585487	39.17%	5.240%
25	4.596	1104	1106	1109	rVB2	499	270	0.02%	0.002%
26	4.683	1131	1133	1137	rVB	555	369	0.02%	0.003%
27	4.703	1137	1139	1144	rBV3	484	301	0.02%	0.003%
28	4.744	1149	1152	1153	rBV	442	253	0.02%	0.002%
29	4.802	1167	1170	1175	rBV2	250	327	0.02%	0.003%
30	4.924	1205	1208	1212	rVB3	498	270	0.02%	0.002%
31	5.047	1229	1246	1275	rBV2	583711	1494742	100.00%	13.377%
32	5.619	1411	1424	1459	rBV	439116	897696	60.06%	8.034%
33	5.911	1503	1515	1532	rBV4	17403	36923	2.47%	0.330%
34	6.072	1550	1565	1592	rBV	322657	669619	44.80%	5.993%
35	6.281	1628	1630	1636	rVB3	670	593	0.04%	0.005%
36	6.378	1657	1660	1666	rBV2	626	633	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW081821\
 Data File : VW021863.D
 Acq On : 18 Aug 2021 14:17
 Operator : SY/MD
 Sample : M3422-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKB1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Title : VOC Analysis

37	6.503	1696	1699	1701	rBV	489	288	0.02%	0.003%
38	6.555	1713	1715	1719	rVB2	509	273	0.02%	0.002%
39	6.628	1734	1738	1740	rBV2	294	214	0.01%	0.002%
40	6.645	1740	1743	1745	rBV2	450	244	0.02%	0.002%
41	6.664	1747	1749	1753	rVV3	559	299	0.02%	0.003%
42	6.770	1779	1782	1785	rBV	429	320	0.02%	0.003%
43	6.802	1789	1792	1794	rBV2	604	341	0.02%	0.003%
44	6.870	1809	1813	1815	rBV2	416	356	0.02%	0.003%
45	6.934	1828	1833	1835	rBV	326	295	0.02%	0.003%
46	6.989	1839	1850	1873	rBV	180173	327155	21.89%	2.928%
47	7.317	1940	1952	1971	rBV	705926	1226767	82.07%	10.979%
48	7.622	2037	2047	2074	rBV	118191	214237	14.33%	1.917%
49	7.860	2117	2121	2128	rBV3	402	522	0.03%	0.005%
50	7.895	2129	2132	2136	rVB3	565	416	0.03%	0.004%
51	7.921	2136	2140	2141	rBV2	528	375	0.03%	0.003%
52	8.008	2164	2167	2170	rBV	566	383	0.03%	0.003%
53	8.088	2183	2192	2229	rBV	332425	617453	41.31%	5.526%
54	8.526	2324	2328	2331	rBV2	650	456	0.03%	0.004%
55	8.603	2350	2352	2355	rVB2	397	241	0.02%	0.002%
56	8.625	2355	2359	2360	rBV3	440	249	0.02%	0.002%
57	8.667	2370	2372	2376	rBV3	459	345	0.02%	0.003%
58	8.789	2408	2410	2416	rVB4	558	454	0.03%	0.004%
59	8.853	2416	2430	2459	rBV	646361	1065449	71.28%	9.535%
60	9.124	2510	2514	2515	rBV	384	303	0.02%	0.003%
61	9.262	2554	2557	2561	rVB2	359	266	0.02%	0.002%
62	9.297	2562	2568	2571	rBV2	380	381	0.03%	0.003%
63	9.342	2578	2582	2586	rBV3	523	357	0.02%	0.003%
64	9.397	2597	2599	2601	rVB	488	231	0.02%	0.002%
65	9.471	2613	2622	2625	rBV2	452	440	0.03%	0.004%
66	9.812	2724	2728	2729	rBV	378	230	0.02%	0.002%
67	9.898	2750	2755	2757	rVB2	312	256	0.02%	0.002%
68	9.940	2766	2768	2772	rBV	302	269	0.02%	0.002%
69	10.008	2785	2789	2791	rBV3	433	309	0.02%	0.003%
70	10.056	2801	2804	2805	rBV2	399	237	0.02%	0.002%
71	10.130	2819	2827	2837	rVB3	3215	5545	0.37%	0.050%
72	10.217	2840	2854	2880	rBV	447155	711194	47.58%	6.365%
73	10.429	2916	2920	2922	rBV2	439	299	0.02%	0.003%
74	10.513	2944	2946	2948	rBV2	485	218	0.01%	0.002%
75	10.542	2952	2955	2957	rBV2	552	307	0.02%	0.003%
76	10.577	2963	2966	2967	rBV2	969	555	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
 Data File : VV021863.D
 Acq On : 18 Aug 2021 14:17
 Operator : SY/MD
 Sample : M3422-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKB1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Title : VOC Analysis

77	10.744	3016	3018	3020	rBV	541	299	0.02%	0.003%
78	10.792	3031	3033	3038	rBV2	335	296	0.02%	0.003%
79	10.841	3043	3048	3050	rBV4	617	614	0.04%	0.005%
80	10.924	3066	3074	3083	rVB7	4185	6466	0.43%	0.058%
81	11.033	3102	3108	3110	rBV3	976	1004	0.07%	0.009%
82	11.146	3138	3143	3154	rVV5	2304	3216	0.22%	0.029%
83	11.249	3163	3175	3195	rBV	643999	1011857	67.69%	9.056%
84	11.625	3280	3292	3315	rBV	672632	1064891	71.24%	9.530%
85	11.776	3335	3339	3340	rBV3	892	587	0.04%	0.005%
86	11.847	3355	3361	3365	rBV5	1055	1323	0.09%	0.012%
87	11.918	3379	3383	3386	rBV4	617	401	0.03%	0.004%
88	11.956	3390	3395	3396	rBV	525	359	0.02%	0.003%
89	12.049	3421	3424	3427	rBV2	538	319	0.02%	0.003%
90	12.217	3472	3476	3480	rVB2	475	355	0.02%	0.003%
91	12.249	3480	3486	3488	rBV3	765	845	0.06%	0.008%
92	12.487	3557	3560	3561	rBV2	427	216	0.01%	0.002%
93	12.876	3678	3681	3684	rBV2	370	267	0.02%	0.002%
94	12.921	3693	3695	3699	rBV2	374	207	0.01%	0.002%
95	12.988	3713	3716	3721	rBV2	537	484	0.03%	0.004%
96	13.033	3727	3730	3734	rBV	413	227	0.02%	0.002%
97	13.184	3775	3777	3781	rVB3	574	318	0.02%	0.003%
98	13.297	3810	3812	3814	rBV2	431	258	0.02%	0.002%
99	13.596	3902	3905	3908	rVB	395	222	0.01%	0.002%
100	13.773	3957	3960	3962	rBV3	267	206	0.01%	0.002%

Sum of corrected areas: 11173848




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
Data File : VV021863.D
Acq On : 18 Aug 2021 14:17
Operator : SY/MD
Sample : M3422-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKB1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

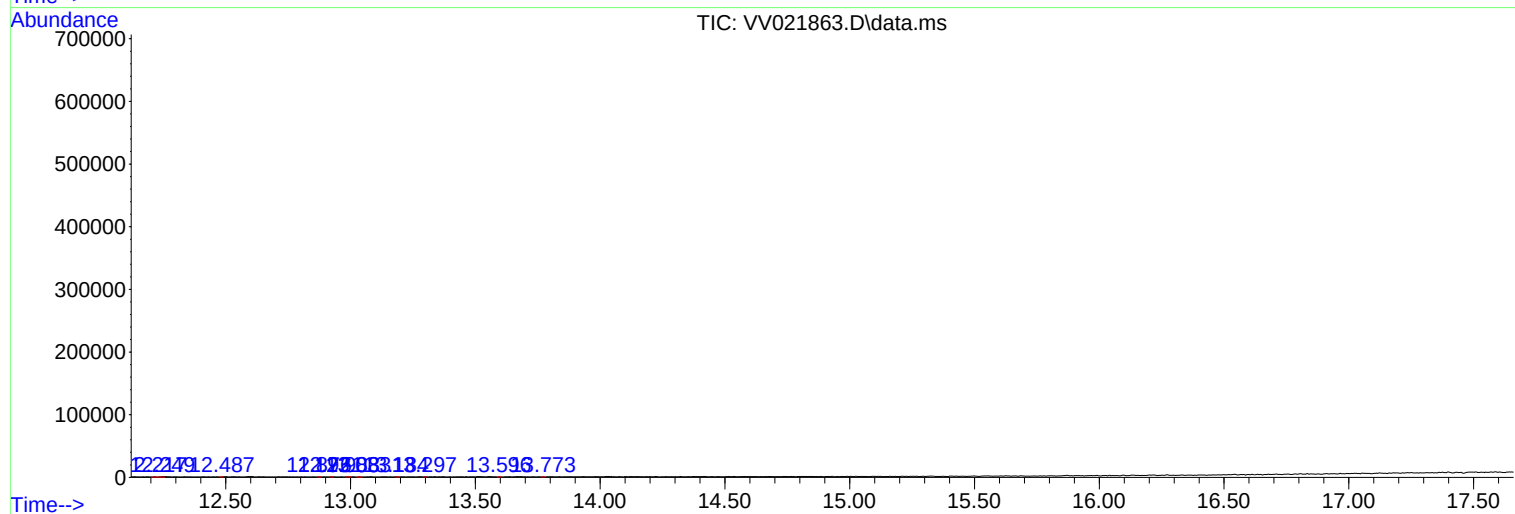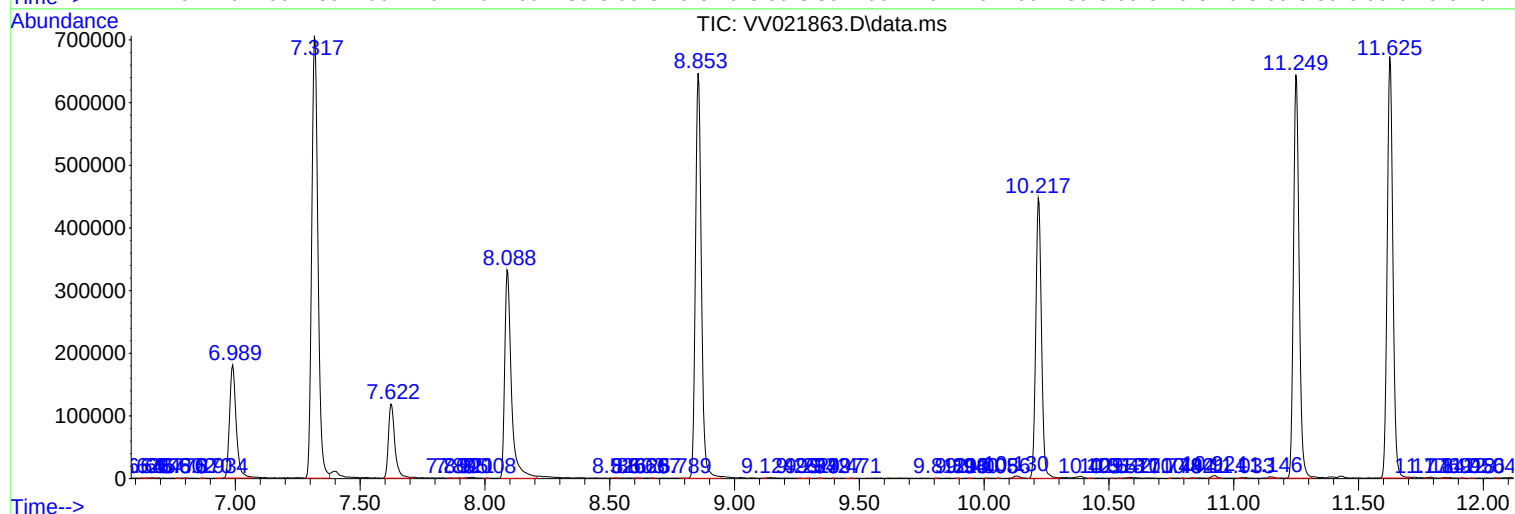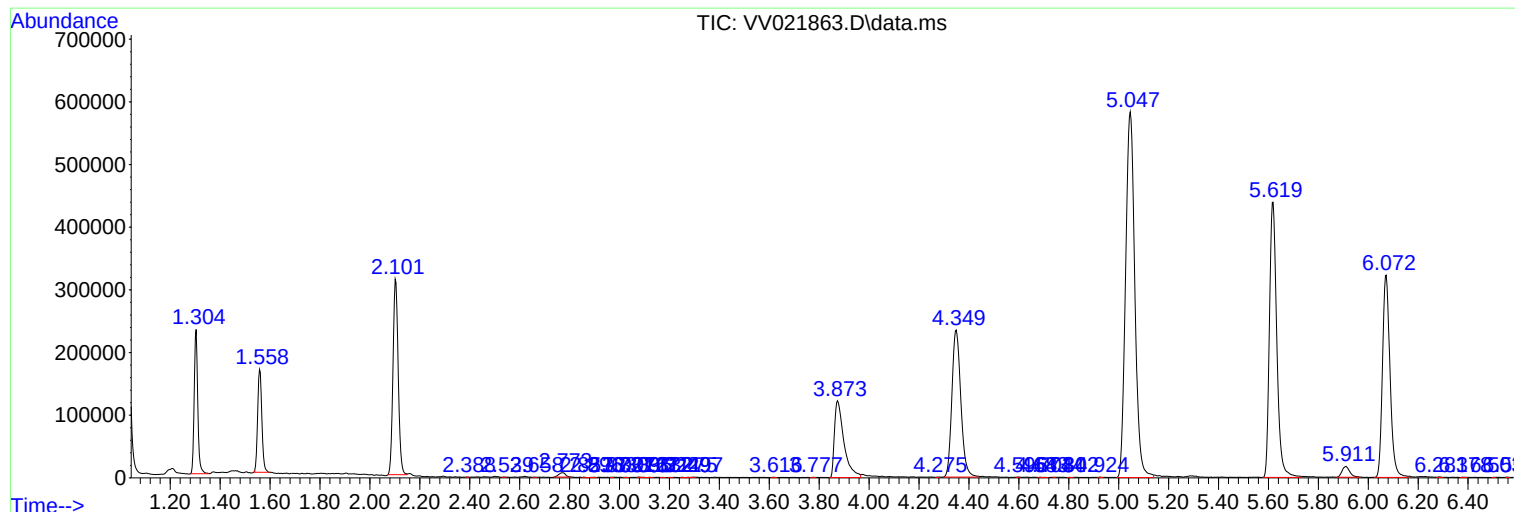

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
Data File : VV021863.D
Acq On : 18 Aug 2021 14:17
Operator : SY/MD
Sample : M3422-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKB1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
Data File : VV021863.D
Acq On : 18 Aug 2021 14:17
Operator : SY/MD
Sample : M3422-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKB1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
