

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
 Data File : VV021868.D
 Acq On : 18 Aug 2021 16:15
 Operator : SY/MD
 Sample : M3448-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M

Title : VOC Analysis

Signal : TIC: VV021868.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	25	29	41	rVB	23055	25739	1.93%	0.241%
2	1.304	76	82	90	rBV	185867	183638	13.75%	1.719%
3	1.561	156	162	175	rVB	146046	170799	12.79%	1.599%
4	2.105	323	331	345	rVB	270305	390709	29.25%	3.658%
5	2.870	567	569	572	rBV2	409	195	0.01%	0.002%
6	2.973	599	601	603	rBV2	468	218	0.02%	0.002%
7	3.175	659	664	665	rBV3	603	458	0.03%	0.004%
8	3.269	690	693	696	rVB2	452	277	0.02%	0.003%
9	3.433	742	744	749	rBV2	430	275	0.02%	0.003%
10	3.491	757	762	765	rBV3	354	340	0.03%	0.003%
11	3.687	821	823	831	rVB2	483	468	0.04%	0.004%
12	3.761	844	846	851	rBV2	340	262	0.02%	0.002%
13	3.876	873	882	927	rBV	130898	358841	26.87%	3.360%
14	4.352	1014	1030	1059	rBV	221046	550939	41.25%	5.158%
15	4.552	1090	1092	1095	rBB3	593	244	0.02%	0.002%
16	4.722	1143	1145	1150	rBV3	622	386	0.03%	0.004%
17	4.748	1150	1153	1155	rBV2	517	340	0.03%	0.003%
18	4.851	1183	1185	1188	rBV2	286	169	0.01%	0.002%
19	4.870	1188	1191	1194	rVV2	344	248	0.02%	0.002%
20	4.892	1195	1198	1201	rVB2	392	255	0.02%	0.002%
21	4.941	1211	1213	1216	rVV2	380	186	0.01%	0.002%
22	4.976	1221	1224	1226	rBV2	312	207	0.02%	0.002%
23	5.050	1230	1247	1274	rBV2	521863	1335602	100.00%	12.505%
24	5.500	1385	1387	1389	rBV	416	227	0.02%	0.002%
25	5.574	1407	1410	1411	rBV2	616	327	0.02%	0.003%
26	5.619	1412	1424	1450	rVV	454176	916662	68.63%	8.583%
27	5.912	1506	1515	1531	rVB3	8349	17847	1.34%	0.167%
28	6.072	1552	1565	1591	rBV	298671	618911	46.34%	5.795%
29	6.323	1640	1643	1646	rBV3	789	482	0.04%	0.005%
30	6.384	1660	1662	1664	rBV2	534	189	0.01%	0.002%
31	6.397	1664	1666	1671	rVB2	730	392	0.03%	0.004%
32	6.474	1685	1690	1692	rBV	693	574	0.04%	0.005%
33	6.706	1759	1762	1766	rBV4	538	381	0.03%	0.004%
34	6.722	1766	1767	1772	rVB3	507	328	0.02%	0.003%
35	6.770	1779	1782	1785	rVB	348	213	0.02%	0.002%
36	6.789	1785	1788	1790	rBV	374	256	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
 Data File : VV021868.D
 Acq On : 18 Aug 2021 16:15
 Operator : SY/MD
 Sample : M3448-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Title : VOC Analysis

37	6.831	1799	1801	1806	rVB3	361	226	0.02%	0.002%
38	6.860	1806	1810	1814	rBV3	324	269	0.02%	0.003%
39	6.989	1838	1850	1878	rBV2	159516	298269	22.33%	2.793%
40	7.130	1890	1894	1895	rBV3	615	379	0.03%	0.004%
41	7.320	1941	1953	1972	rBV	589818	1026863	76.88%	9.614%
42	7.625	2036	2048	2072	rBV	108444	191006	14.30%	1.788%
43	7.944	2139	2147	2153	rBV6	1347	1877	0.14%	0.018%
44	7.998	2161	2164	2169	rBV2	440	375	0.03%	0.004%
45	8.024	2169	2172	2175	rBV2	660	507	0.04%	0.005%
46	8.092	2181	2193	2225	rBV	364348	651468	48.78%	6.100%
47	8.445	2300	2303	2307	rBV3	558	498	0.04%	0.005%
48	8.699	2379	2382	2384	rVV2	383	251	0.02%	0.002%
49	8.805	2412	2415	2418	rBV3	399	304	0.02%	0.003%
50	8.854	2418	2430	2455	rBV	667515	1096520	82.10%	10.267%
51	9.159	2523	2525	2532	rVB4	1080	944	0.07%	0.009%
52	9.227	2543	2546	2551	rVB2	237	199	0.01%	0.002%
53	9.313	2570	2573	2577	rVB2	385	236	0.02%	0.002%
54	9.391	2594	2597	2601	rBV2	390	257	0.02%	0.002%
55	9.474	2619	2623	2625	rBV	239	183	0.01%	0.002%
56	9.490	2626	2628	2630	rVB2	460	189	0.01%	0.002%
57	9.503	2630	2632	2635	rBV	249	184	0.01%	0.002%
58	9.519	2635	2637	2640	rVB2	428	212	0.02%	0.002%
59	9.686	2685	2689	2691	rBV	342	183	0.01%	0.002%
60	9.703	2691	2694	2696	rBV3	334	202	0.02%	0.002%
61	9.828	2724	2733	2738	rBV5	1682	2363	0.18%	0.022%
62	9.883	2748	2750	2754	rVB2	490	269	0.02%	0.003%
63	10.011	2788	2790	2795	rVB2	330	257	0.02%	0.002%
64	10.043	2795	2800	2802	rBV2	309	214	0.02%	0.002%
65	10.127	2822	2826	2827	rBV2	1256	821	0.06%	0.008%
66	10.220	2841	2855	2879	rBV	454429	731003	54.73%	6.844%
67	10.384	2899	2906	2915	rBV5	1885	2518	0.19%	0.024%
68	10.461	2926	2930	2932	rBV2	485	392	0.03%	0.004%
69	10.474	2932	2934	2936	rVB2	490	189	0.01%	0.002%
70	10.580	2963	2967	2969	rBV3	566	390	0.03%	0.004%
71	10.744	3015	3018	3020	rBV2	445	289	0.02%	0.003%
72	10.876	3057	3059	3064	rBV	680	343	0.03%	0.003%
73	10.921	3064	3073	3074	rBV5	1565	1610	0.12%	0.015%
74	11.043	3107	3111	3112	rBV5	356	278	0.02%	0.003%
75	11.149	3141	3144	3146	rVV3	412	277	0.02%	0.003%
76	11.252	3164	3176	3195	rBV	684818	1057501	79.18%	9.901%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
 Data File : VV021868.D
 Acq On : 18 Aug 2021 16:15
 Operator : SY/MD
 Sample : M3448-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Title : VOC Analysis

77	11.484	3245	3248	3251	rBV2	525	419	0.03%	0.004%
78	11.538	3257	3265	3272	rBV6	3703	6673	0.50%	0.062%
79	11.625	3280	3292	3312	rBV	634768	1008007	75.47%	9.438%
80	11.815	3349	3351	3354	rVB2	531	232	0.02%	0.002%
81	11.834	3354	3357	3358	rBV2	457	249	0.02%	0.002%
82	11.889	3373	3374	3377	rBV2	333	179	0.01%	0.002%
83	12.030	3415	3418	3420	rBV	460	198	0.01%	0.002%
84	12.072	3428	3431	3436	rBV2	562	376	0.03%	0.004%
85	12.127	3444	3448	3451	rBV2	566	416	0.03%	0.004%
86	12.297	3499	3501	3506	rVV2	553	379	0.03%	0.004%
87	12.599	3593	3595	3598	rBV3	590	370	0.03%	0.003%
88	12.696	3623	3625	3628	rBV2	344	217	0.02%	0.002%
89	12.889	3684	3685	3691	rVB3	611	395	0.03%	0.004%
90	12.918	3691	3694	3695	rBV	336	170	0.01%	0.002%
91	13.050	3731	3735	3738	rBV3	338	258	0.02%	0.002%
92	13.072	3740	3742	3745	rBV2	382	249	0.02%	0.002%
93	13.249	3794	3797	3798	rBV2	350	189	0.01%	0.002%
94	13.439	3853	3856	3858	rBV2	302	227	0.02%	0.002%
95	13.513	3873	3879	3881	rBV3	903	1046	0.08%	0.010%
96	13.609	3907	3909	3913	rVB	633	340	0.03%	0.003%
97	13.641	3913	3919	3922	rBV3	607	697	0.05%	0.007%
98	13.921	3999	4006	4009	rBV2	608	618	0.05%	0.006%
99	14.632	4225	4227	4228	rBV2	1073	460	0.03%	0.004%
100	14.824	4279	4287	4294	rBV5	7055	10273	0.77%	0.096%




Sum of corrected areas: 10680536

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
Data File : VV021868.D
Acq On : 18 Aug 2021 16:15
Operator : SY/MD
Sample : M3448-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

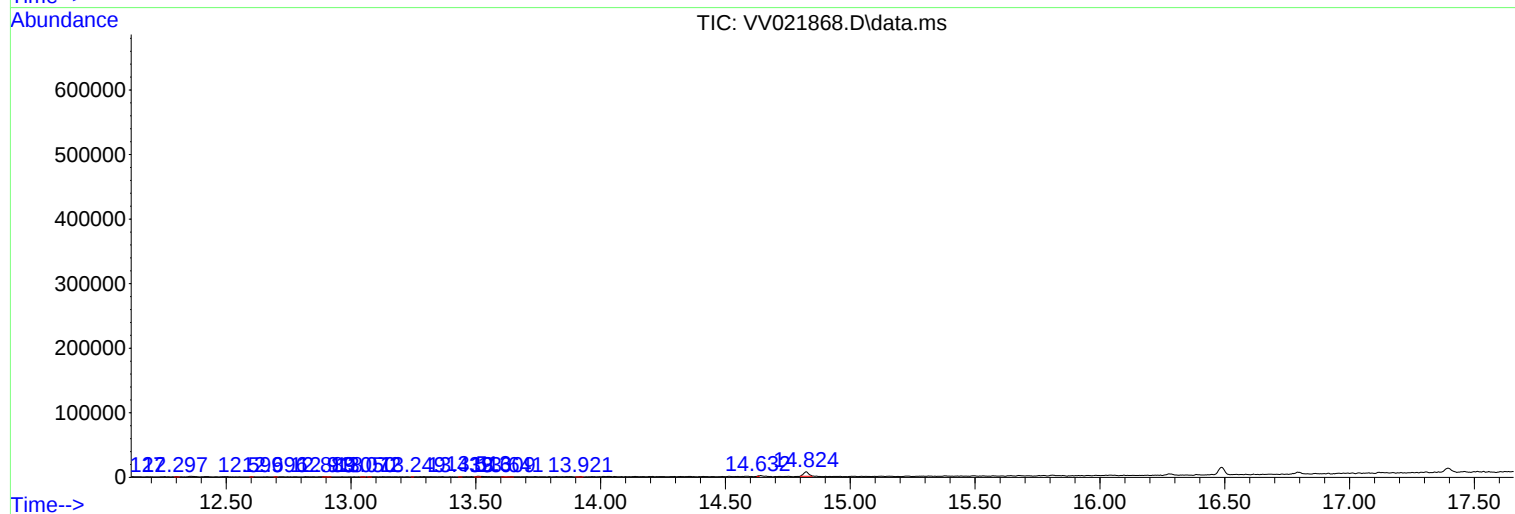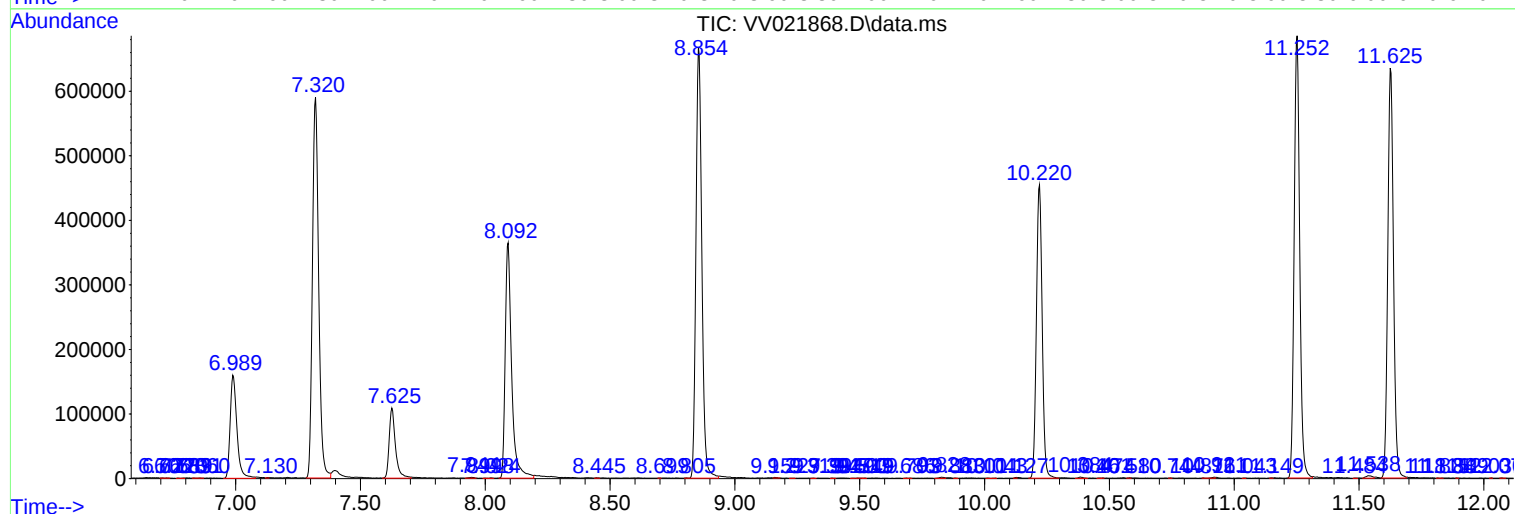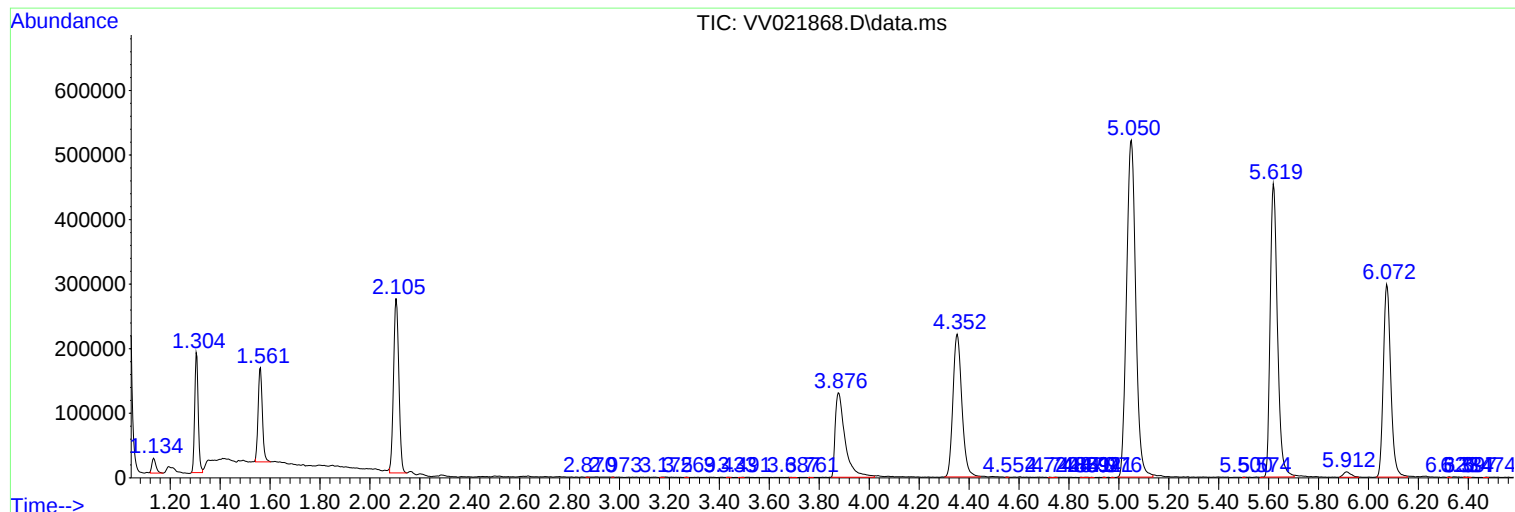

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
Data File : VV021868.D
Acq On : 18 Aug 2021 16:15
Operator : SY/MD
Sample : M3448-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
Data File : VV021868.D
Acq On : 18 Aug 2021 16:15
Operator : SY/MD
Sample : M3448-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
