

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
 Data File : VV021873.D
 Acq On : 18 Aug 2021 18:40
 Operator : SY/MD
 Sample : M3448-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Title : VOC Analysis

Signal : TIC: VV021873.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	222976	225381	14.91%	1.956%
2	1.558	154	161	180	rVB	165833	197215	13.05%	1.712%
3	2.105	321	331	364	rVB	327075	487789	32.27%	4.234%
4	2.568	473	475	477	rBV	439	306	0.02%	0.003%
5	2.658	501	503	506	rBV2	591	369	0.02%	0.003%
6	2.844	558	561	562	rBV	313	175	0.01%	0.002%
7	3.002	606	610	611	rBV	304	205	0.01%	0.002%
8	3.150	654	656	660	rVB2	378	235	0.02%	0.002%
9	3.185	665	667	670	rBV2	230	167	0.01%	0.001%
10	3.304	702	704	708	rBV	262	174	0.01%	0.002%
11	3.330	708	712	715	rVB	500	325	0.02%	0.003%
12	3.452	748	750	755	rBV2	256	193	0.01%	0.002%
13	3.519	769	771	776	rBV	252	182	0.01%	0.002%
14	3.651	809	812	814	rVB3	318	178	0.01%	0.002%
15	3.674	814	819	821	rVB	270	202	0.01%	0.002%
16	3.696	821	826	827	rBV2	359	257	0.02%	0.002%
17	3.812	860	862	867	rVV2	409	185	0.01%	0.002%
18	3.876	872	882	914	rBV	122731	328303	21.72%	2.850%
19	4.349	1013	1029	1064	rBV	238390	590357	39.06%	5.125%
20	4.748	1149	1153	1156	rBV3	510	462	0.03%	0.004%
21	4.821	1174	1176	1180	rBV	335	217	0.01%	0.002%
22	4.889	1194	1197	1199	rBV	328	185	0.01%	0.002%
23	5.047	1229	1246	1278	rBV2	587917	1511446	100.00%	13.120%
24	5.410	1354	1359	1363	rBV3	557	679	0.04%	0.006%
25	5.471	1375	1378	1380	rBV2	387	252	0.02%	0.002%
26	5.500	1385	1387	1391	rVB2	846	544	0.04%	0.005%
27	5.522	1391	1394	1397	rBV3	290	226	0.01%	0.002%
28	5.619	1411	1424	1456	rBV	477241	973517	64.41%	8.451%
29	5.908	1503	1514	1531	rBV2	22476	47705	3.16%	0.414%
30	6.072	1550	1565	1594	rBV	329902	675198	44.67%	5.861%
31	6.410	1663	1670	1672	rBV4	425	426	0.03%	0.004%
32	6.490	1689	1695	1700	rBV4	422	452	0.03%	0.004%
33	6.526	1700	1706	1714	rVV5	657	896	0.06%	0.008%
34	6.654	1742	1746	1750	rBV3	700	672	0.04%	0.006%
35	6.735	1768	1771	1773	rBV3	273	197	0.01%	0.002%
36	6.815	1793	1796	1800	rVB2	778	509	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
 Data File : VV021873.D
 Acq On : 18 Aug 2021 18:40
 Operator : SY/MD
 Sample : M3448-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Title : VOC Analysis

37	6.841	1800	1804	1808	rVB2	218	172	0.01%	0.001%
38	6.989	1837	1850	1877	rBV	179914	332119	21.97%	2.883%
39	7.320	1940	1953	1971	rBV	706208	1232220	81.53%	10.697%
40	7.580	2032	2034	2037	rBV3	390	335	0.02%	0.003%
41	7.622	2038	2047	2073	rVV	120445	212141	14.04%	1.842%
42	7.927	2135	2142	2144	rBV5	690	731	0.05%	0.006%
43	7.982	2154	2159	2167	rVB6	2140	3116	0.21%	0.027%
44	8.021	2168	2171	2172	rBV	362	217	0.01%	0.002%
45	8.088	2181	2192	2231	rBV	334271	625352	41.37%	5.428%
46	8.407	2287	2291	2295	rBV4	680	573	0.04%	0.005%
47	8.448	2302	2304	2306	rBV2	367	184	0.01%	0.002%
48	8.506	2320	2322	2324	rBV2	369	232	0.02%	0.002%
49	8.632	2357	2361	2362	rBV	265	194	0.01%	0.002%
50	8.796	2409	2412	2415	rVB2	424	224	0.01%	0.002%
51	8.815	2415	2418	2419	rBV	409	173	0.01%	0.002%
52	8.853	2419	2430	2460	rBV	706006	1148373	75.98%	9.969%
53	9.069	2495	2497	2499	rVB2	440	190	0.01%	0.002%
54	9.255	2551	2555	2558	rVV3	495	300	0.02%	0.003%
55	9.442	2612	2613	2615	rVV	448	167	0.01%	0.001%
56	9.477	2618	2624	2625	rBV2	240	196	0.01%	0.002%
57	9.487	2625	2627	2630	rVB2	324	167	0.01%	0.001%
58	9.509	2630	2634	2637	rBV2	292	243	0.02%	0.002%
59	9.532	2639	2641	2644	rBV	310	177	0.01%	0.002%
60	9.558	2644	2649	2651	rBV3	400	349	0.02%	0.003%
61	9.593	2659	2660	2664	rBV3	373	175	0.01%	0.002%
62	9.677	2680	2686	2687	rBV	429	376	0.02%	0.003%
63	9.734	2701	2704	2708	rBV2	280	209	0.01%	0.002%
64	9.908	2755	2758	2763	rVB3	338	264	0.02%	0.002%
65	10.024	2792	2794	2798	rVB2	383	238	0.02%	0.002%
66	10.075	2808	2810	2816	rVB2	423	286	0.02%	0.002%
67	10.130	2817	2827	2835	rBV5	3002	5196	0.34%	0.045%
68	10.217	2842	2854	2877	rBV	439766	699716	46.29%	6.074%
69	10.384	2901	2906	2916	rVB6	2180	3745	0.25%	0.033%
70	10.548	2955	2957	2958	rBV6	588	253	0.02%	0.002%
71	10.844	3047	3049	3051	rVB2	427	188	0.01%	0.002%
72	10.857	3051	3053	3057	rBV2	261	235	0.02%	0.002%
73	10.927	3063	3075	3084	rBV5	3299	6151	0.41%	0.053%
74	11.037	3104	3109	3116	rBV4	1046	1237	0.08%	0.011%
75	11.082	3119	3123	3125	rBV2	388	325	0.02%	0.003%
76	11.149	3133	3144	3152	rBV5	1553	2991	0.20%	0.026%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
 Data File : VV021873.D
 Acq On : 18 Aug 2021 18:40
 Operator : SY/MD
 Sample : M3448-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Title : VOC Analysis

77	11.252	3164	3176	3197	rBV	704291	1104148	73.05%	9.585%
78	11.487	3245	3249	3252	rBV2	475	306	0.02%	0.003%
79	11.522	3256	3260	3261	rBV	1119	613	0.04%	0.005%
80	11.538	3261	3265	3269	rBV4	1562	1641	0.11%	0.014%
81	11.625	3281	3292	3315	rVB	678450	1081164	71.53%	9.385%
82	11.934	3385	3388	3391	rVB2	292	192	0.01%	0.002%
83	11.950	3391	3393	3398	rBV2	397	242	0.02%	0.002%
84	12.046	3417	3423	3425	rBV2	537	371	0.02%	0.003%
85	12.082	3432	3434	3436	rBV2	351	238	0.02%	0.002%
86	12.246	3482	3485	3490	rVB3	831	669	0.04%	0.006%
87	12.297	3500	3501	3505	rVB2	430	181	0.01%	0.002%
88	12.429	3539	3542	3545	rVB	350	205	0.01%	0.002%
89	12.490	3560	3561	3566	rVB2	410	184	0.01%	0.002%
90	12.596	3588	3594	3595	rBV3	499	558	0.04%	0.005%
91	12.731	3633	3636	3638	rBV	279	231	0.02%	0.002%
92	12.773	3647	3649	3653	rVB2	465	196	0.01%	0.002%
93	12.837	3664	3669	3672	rBV3	330	375	0.02%	0.003%
94	12.869	3675	3679	3682	rBV2	442	330	0.02%	0.003%
95	13.078	3742	3744	3746	rBV	373	172	0.01%	0.001%
96	13.230	3787	3791	3793	rBV	390	296	0.02%	0.003%
97	13.509	3875	3878	3879	rBV2	594	360	0.02%	0.003%
98	13.667	3923	3927	3932	rBV3	528	615	0.04%	0.005%
99	13.757	3952	3955	3959	rBV3	575	518	0.03%	0.004%
100	13.979	4021	4024	4028	rBV2	709	500	0.03%	0.004%




Sum of corrected areas: 11519816

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
Data File : VV021873.D
Acq On : 18 Aug 2021 18:40
Operator : SY/MD
Sample : M3448-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

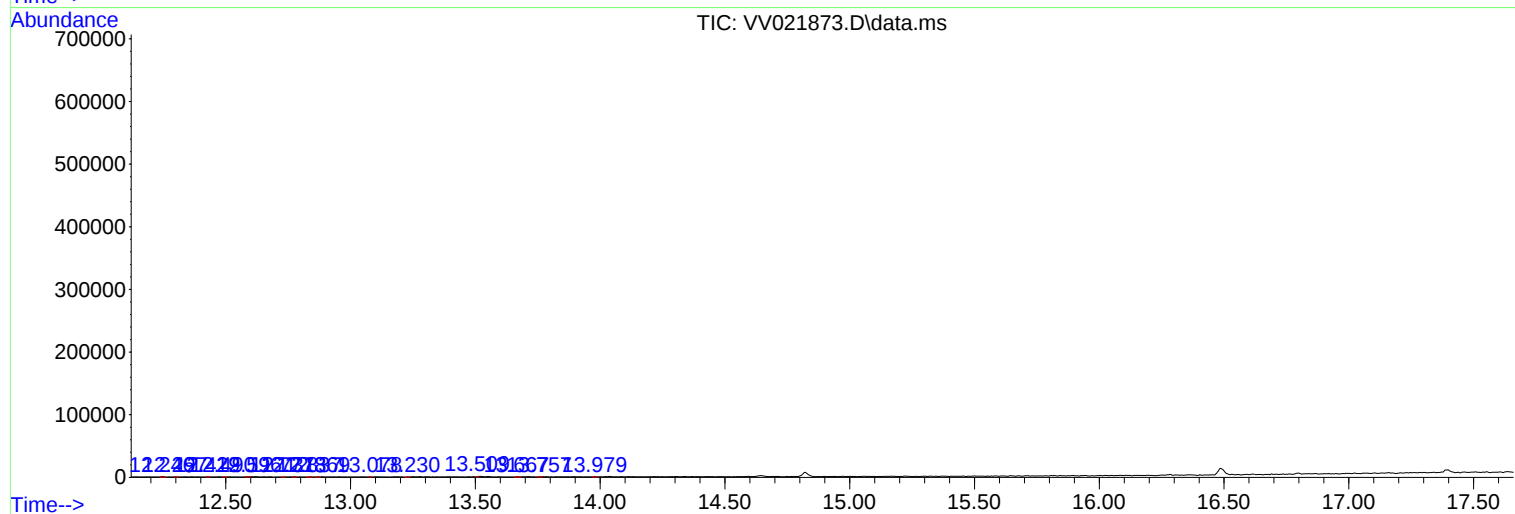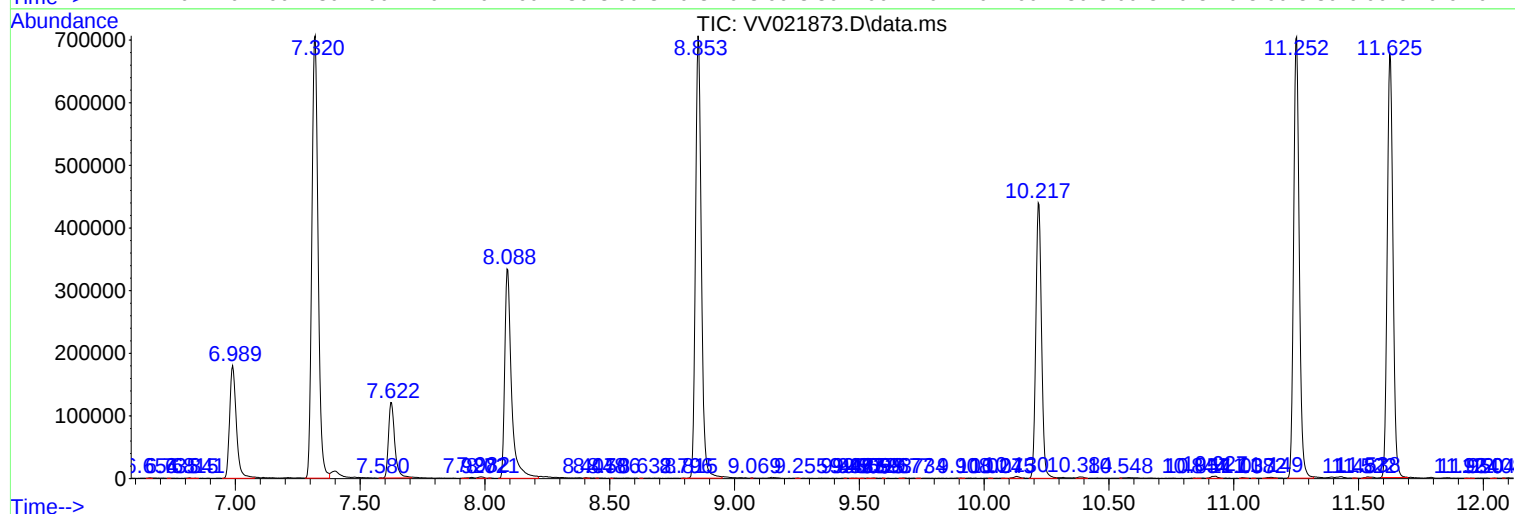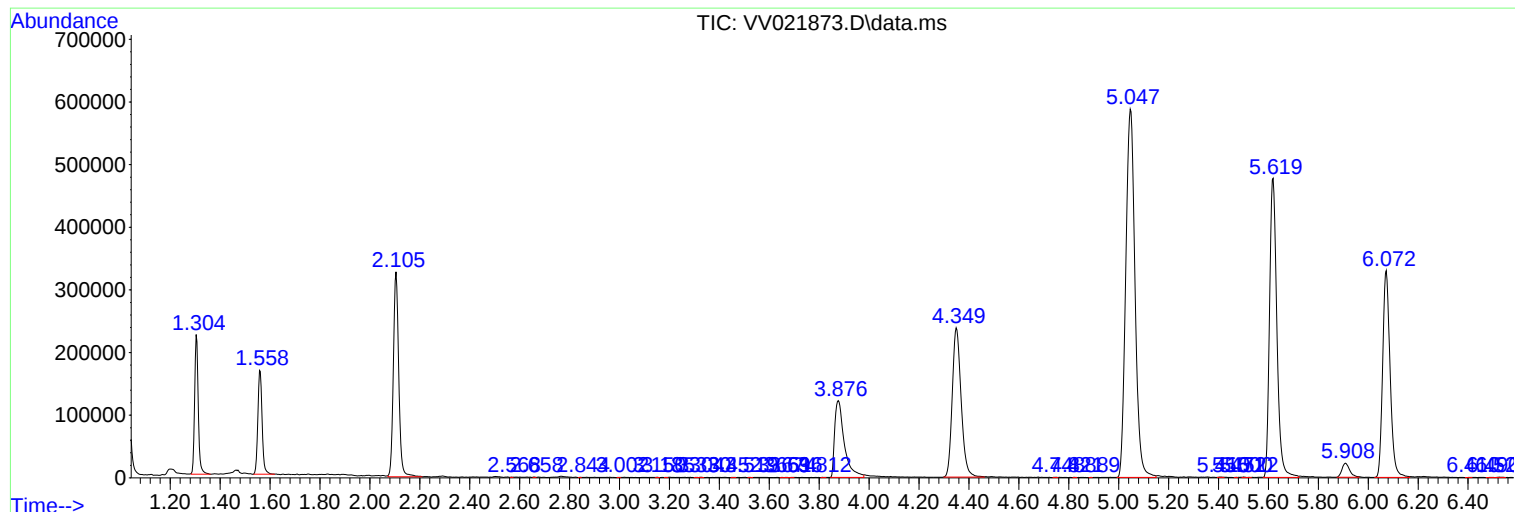

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
Data File : VV021873.D
Acq On : 18 Aug 2021 18:40
Operator : SY/MD
Sample : M3448-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
Data File : VV021873.D
Acq On : 18 Aug 2021 18:40
Operator : SY/MD
Sample : M3448-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
