


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081821\
 Data File : VV021852.D
 Acq On : 18 Aug 2021 09:04
 Operator : SY/MD
 Sample : BFB217
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB217

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Title : VOC Analysis
 Last Update : Thu Aug 19 01:14:55 2021

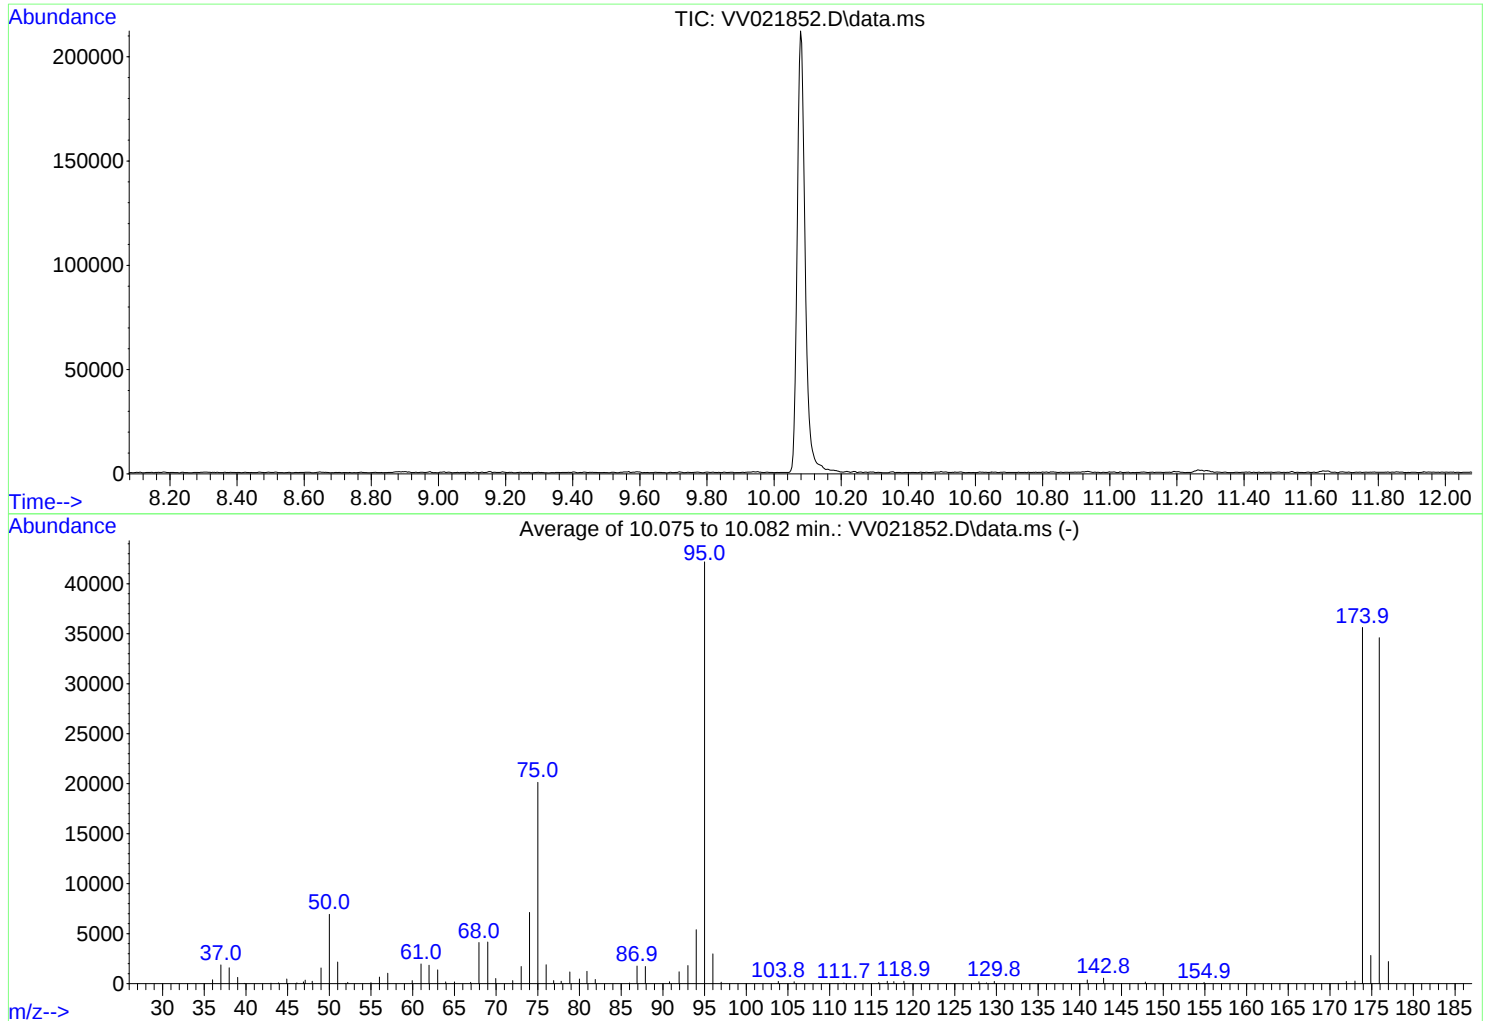

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	6934	PASS
75	95	30	80	47.7	20139	PASS
95	95	100	100	100.0	42192	PASS
96	95	5	9	7.0	2974	PASS
173	174	0.00	2	0.7	260	PASS
174	95	50	120	84.5	35635	PASS
175	174	5	9	7.9	2817	PASS
176	174	95	105	97.1	34597	PASS
177	176	5	10	6.4	2202	PASS

Scan 2800 (10.043 min): VV021852.D\data.ms
BFB217

m/z	Abundance
39.90	192.0
44.00	536.0

Instrument :
MSVOA_V
ClientSampleId :
BFB217

m/z	Abundance
36.00	337.0
37.00	1774.0
38.00	1653.0
39.00	621.0
39.80	195.0
43.00	138.0
43.90	603.0
44.90	433.0
46.10	112.0
46.90	551.0
48.00	209.0
49.00	1432.0
50.00	6742.0
51.00	2068.0
51.90	119.0
52.30	143.0
56.00	756.0
57.00	1009.0
59.90	288.0
61.00	1831.0
61.90	1845.0
63.00	1262.0
63.90	199.0
65.00	174.0
66.90	158.0
68.00	3895.0
69.00	4126.0
70.00	490.0
72.00	268.0
73.00	1730.0
74.00	7102.0
75.00	19632.0
76.00	1852.0
76.90	299.0
77.80	234.0
78.90	1201.0
80.00	432.0
80.90	1301.0
81.90	399.0
86.90	1826.0
87.90	1623.0
90.80	205.0
91.90	1114.0
93.00	1787.0
94.00	5540.0
95.00	40120.0
96.00	2889.0
97.00	120.0
103.90	207.0
105.80	227.0
111.70	108.0
116.90	219.0
117.70	195.0
118.90	225.0
127.90	183.0
129.70	206.0
140.90	338.0
142.90	565.0
147.90	194.0
154.90	128.0
172.00	183.0
173.90	33336.0
174.90	2742.0
175.90	32720.0
177.00	2143.0

Instrument :
MSVOA_V
ClientSampleId :
BFB217

m/z	Abundance
36.00	387.0
37.00	1945.0
38.00	1631.0
39.00	645.0
39.80	228.0
43.90	620.0
44.90	485.0
46.10	117.0
47.10	562.0
47.90	242.0
49.00	1586.0
50.00	7150.0
51.00	2235.0
52.20	131.0
55.00	133.0
56.00	675.0
57.00	1054.0
60.00	332.0
61.00	2097.0
62.00	1894.0
63.00	1413.0
63.90	187.0
65.00	194.0
66.90	129.0
68.00	4210.0
69.00	4294.0
69.90	527.0
72.00	327.0
73.00	1789.0
74.00	7326.0
75.00	20856.0
76.00	2003.0
76.90	329.0
77.80	234.0
78.90	1211.0
80.00	492.0
80.90	1273.0
81.90	450.0
86.00	101.0
86.90	1825.0
87.90	1769.0
90.80	200.0
91.90	1236.0
93.00	1889.0
94.00	5617.0
95.00	43688.0
96.00	3066.0
97.00	154.0
103.90	230.0
105.70	190.0
111.70	111.0
115.90	157.0
116.90	221.0
117.70	231.0
118.90	232.0
127.90	202.0
128.80	115.0
129.80	248.0
140.90	372.0
142.80	590.0
147.90	169.0
154.90	131.0
171.90	236.0
173.00	373.0
173.90	36896.0
174.90	2899.0
175.90	35544.0
177.00	2262.0

Instrument :
MSVOA_V
ClientSampleId :
BFB217

m/z	Abundance
36.00	423.0
37.00	1881.0
38.00	1488.0
39.00	596.0
39.80	276.0
43.90	619.0
44.90	461.0
47.10	479.0
47.90	262.0
49.00	1695.0
50.00	6910.0
51.00	2197.0
52.10	132.0
55.00	152.0
56.00	554.0
57.00	1048.0
60.00	300.0
61.00	1963.0
62.00	1798.0
63.00	1465.0
64.00	139.0
65.00	162.0
67.00	124.0
67.90	4231.0
69.00	4082.0
69.90	542.0
72.00	337.0
73.00	1616.0
74.00	6920.0
75.00	19928.0
76.00	1815.0
76.90	295.0
77.80	235.0
78.80	1120.0
80.00	483.0
80.90	1120.0
81.90	412.0
86.00	105.0
86.90	1644.0
87.90	1758.0
90.80	174.0
92.00	1183.0
93.00	1748.0
94.00	5016.0
95.00	42768.0
96.00	2968.0
97.00	142.0
103.80	216.0
105.70	156.0
115.90	200.0
116.90	263.0
117.70	195.0
118.90	250.0
127.90	194.0
128.80	133.0
129.80	238.0
140.90	396.0
142.80	500.0
147.80	123.0
154.90	128.0
171.90	244.0
173.00	406.0
173.90	36672.0
174.90	2809.0
175.90	35528.0
177.00	2201.0

Instrument :
MSVOA_V
ClientSampleId :
BFB217