

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081919\

Data File : VV012275.D

Acq On : 19 Aug 2019 13:01

Operator : SY/MD

Sample : VSTD0.532

Misc : 25mL/MSVOA V/WATER

ALS Vial : 2 Sample Multiplier: 1

Quant Time: Aug 19 18:53:06 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081919WMA.M

Quant Title : TRACE VOA SOM01.0


QLast Update : Mon Aug 19 18:23:47 2019

Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.532

Manual Integrations
APPROVED

MMDadoda
8/20/2019 12:41:22 PM

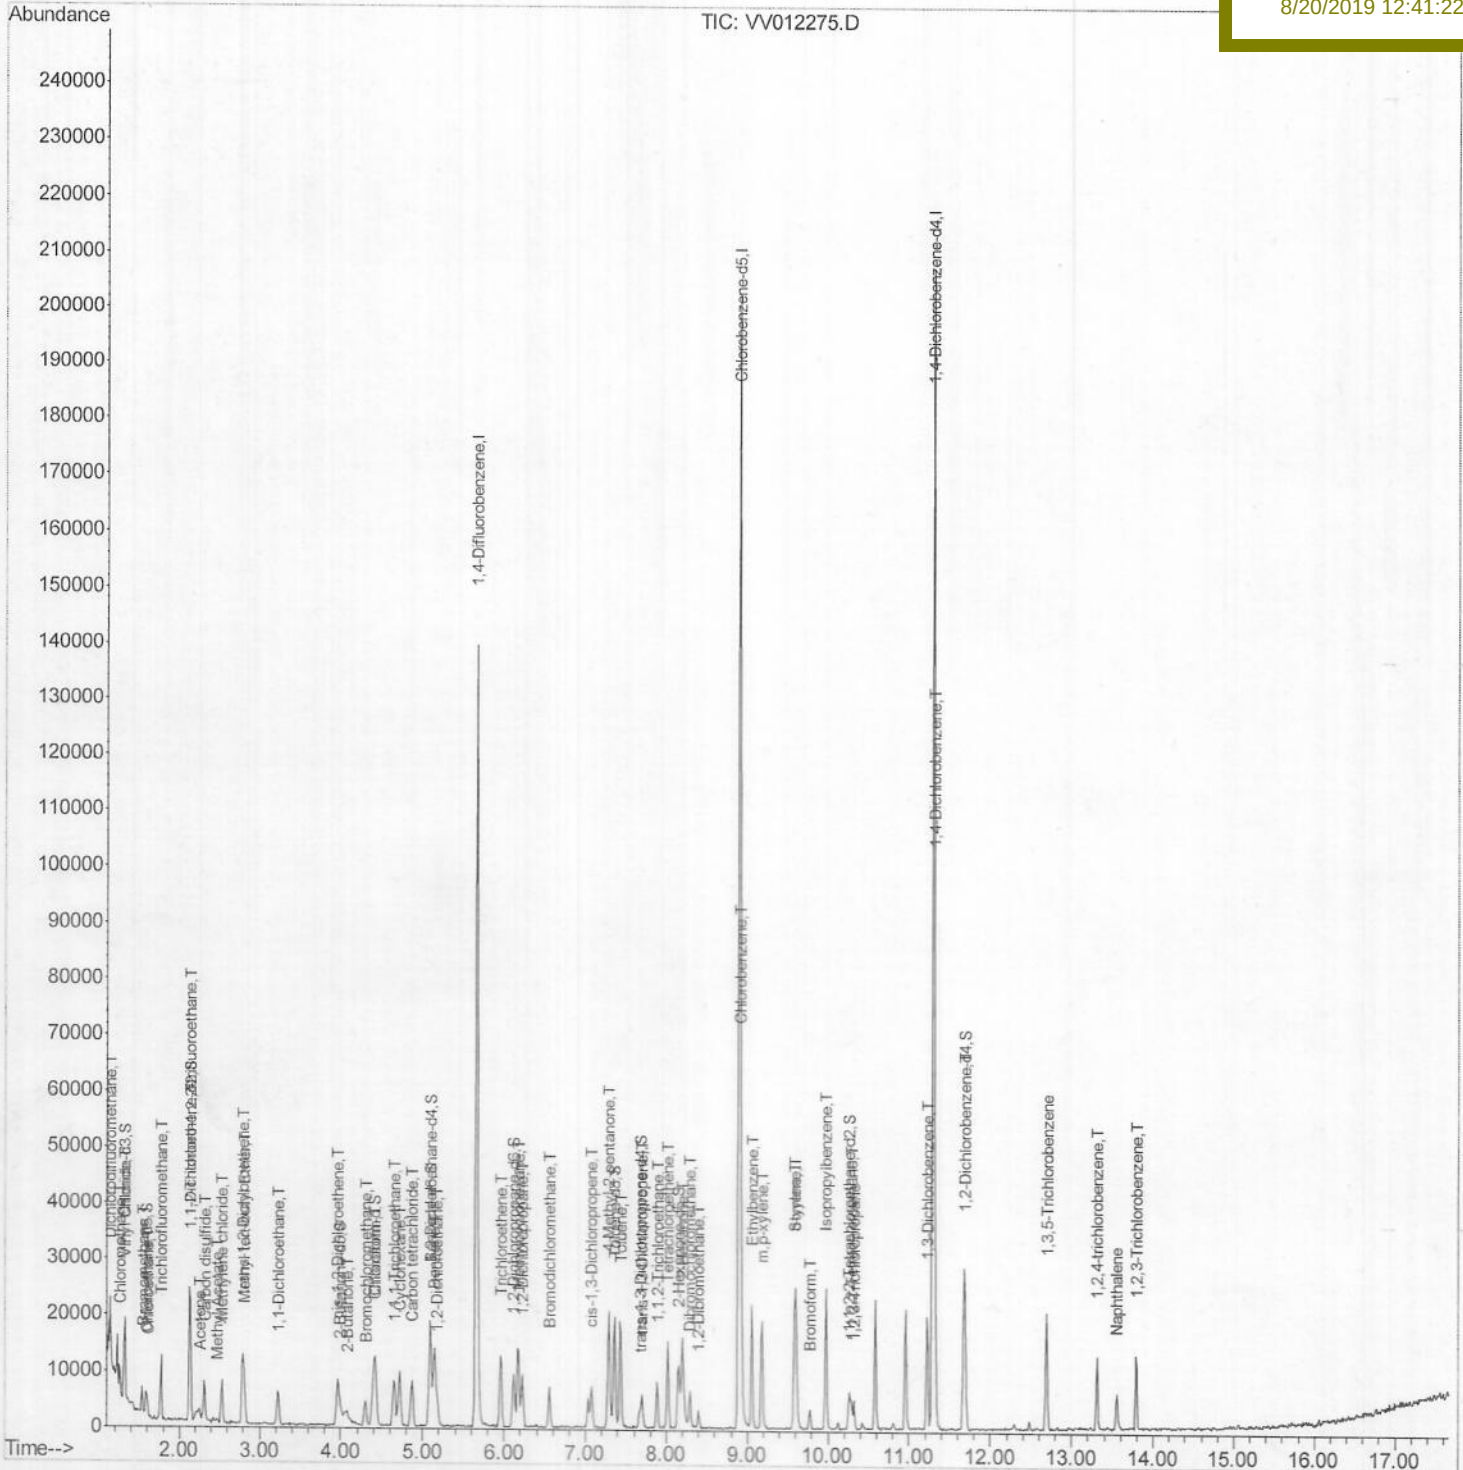

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081919\

Data File : VV012275.D

Acq On : 19 Aug 2019 13:01

Operator : SY/MD

Sample : VSTD0.532

Misc : 25mL/MSVOA V/WATER

ALS Vial : 2 Sample Multiplier: 1

Quant Time: Aug 19 18:26:49 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081919WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Mon Aug 19 18:23:47 2019

Response via : Initial Calibration

Instrument :

MSVOA_V


ClientSampleId :

VSTD0.532

Manual Integrations
APPROVED

MMDadoda

8/20/2019 12:41:22 PM

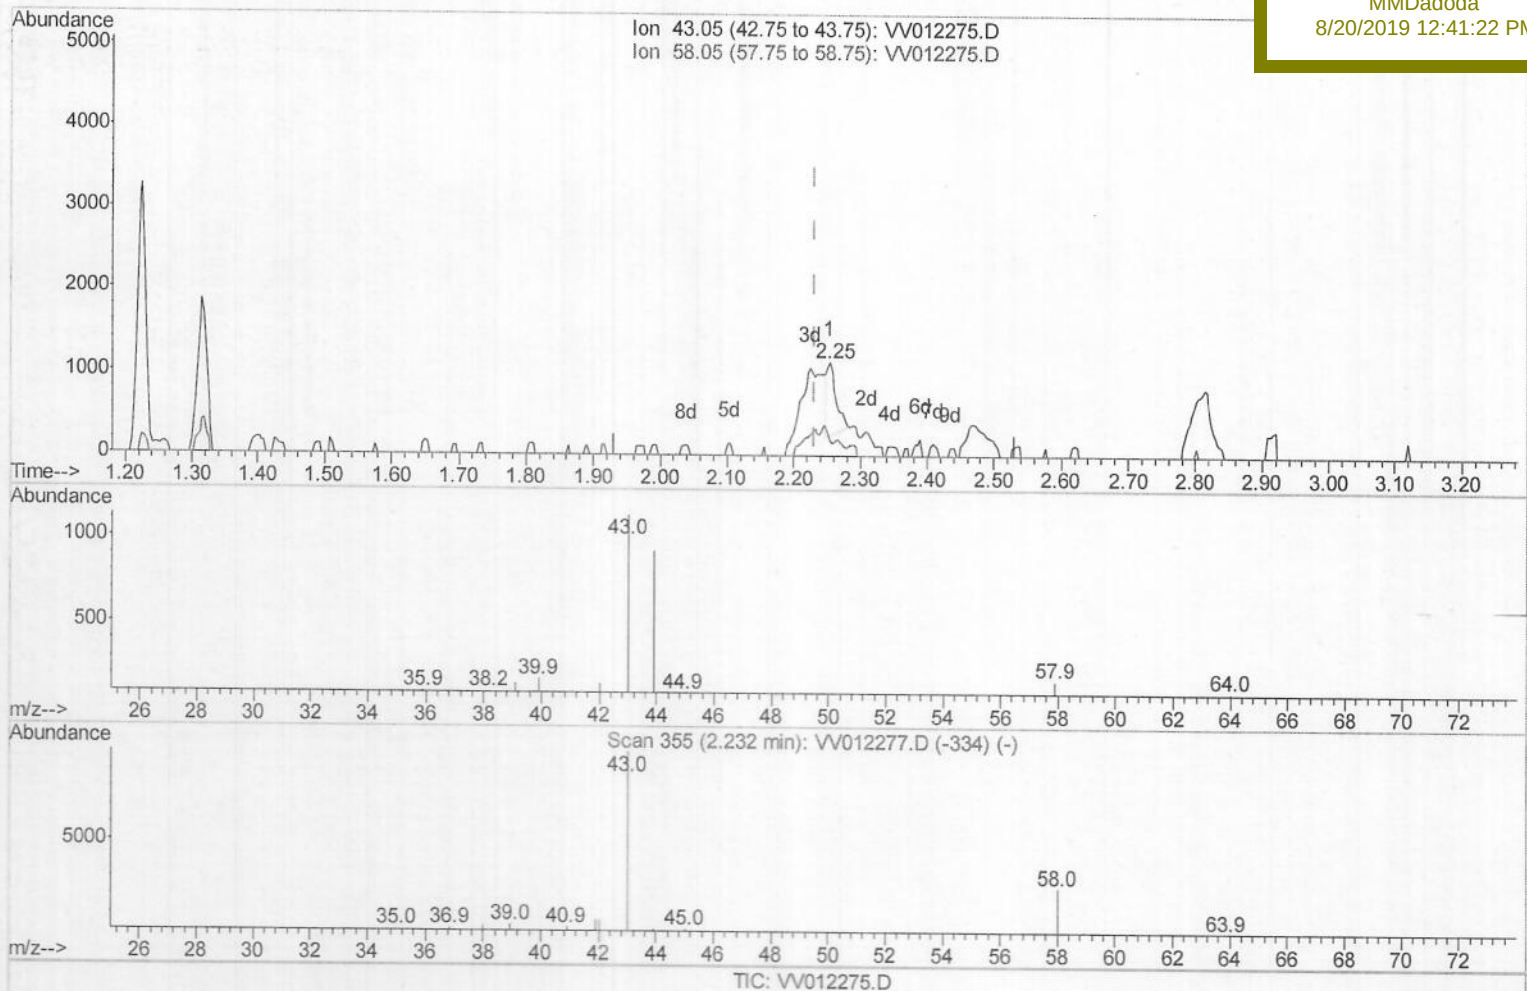

(13) Acetone (T)

2.254min (+0.022) 0.81ug/L

response 813

Ion	Exp%	Act%
43.05	100	100
58.05	12.80	22.14
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081919\

Data File : VV012275.D

Acq On : 19 Aug 2019 13:01

Operator : SY/MD

Sample : VSTD0.532

Misc : 25mL/MSVOA V/WATER

ALS Vial : 2 Sample Multiplier: 1

Quant Time: Aug 19 18:26:49 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081919WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Mon Aug 19 18:23:47 2019

Response via : Initial Calibration

Instrument :

MSVOA_V

ClientSampled :




VSTD0.532

Manual Integrations

APPROVED

MMDadoda

8/20/2019 12:41:22 PM

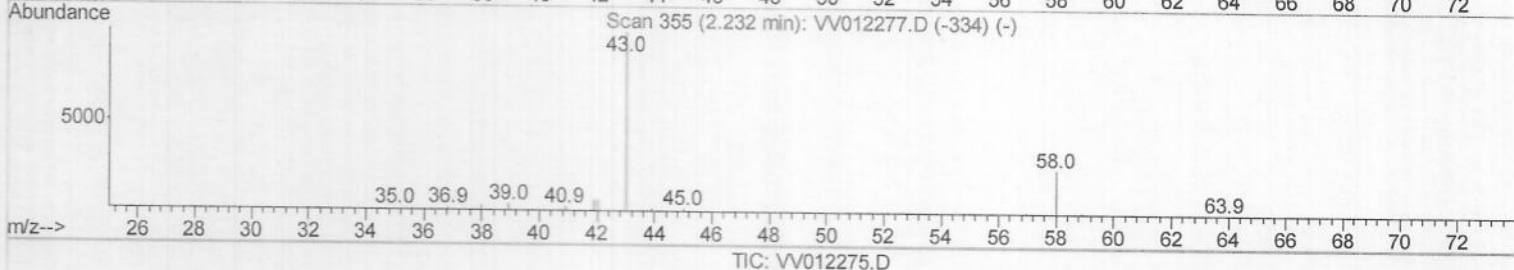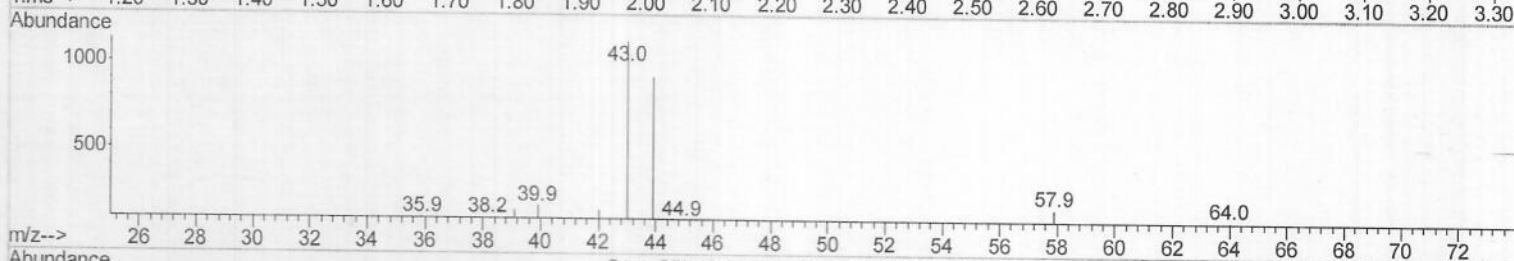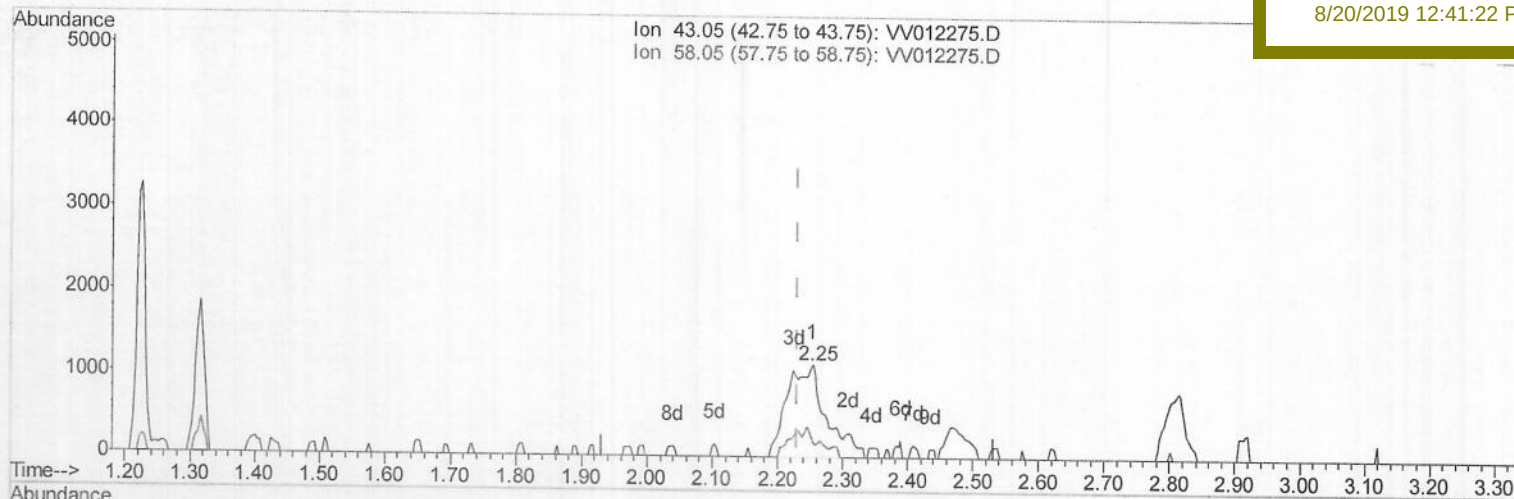

(13) Acetone (T)

2.254min (+0.022) 4.70ug/L m>MD08128119

response 4716

Ion	Exp%	Act%
43.05	100	100
58.05	12.80	3.82
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081919\

Data File : VV012275.D

Acq On : 19 Aug 2019 13:01

Operator : SY/MD

Sample : VSTD0.532

Misc : 25mL/MSVOA V/WATER

ALS Vial : 2 Sample Multiplier: 1

Quant Time: Aug 19 18:26:49 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081919WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Mon Aug 19 18:23:47 2019

Response via : Initial Calibration

Instrument :

MSVOA_V

ClientSampleId :




VSTD0.532

Manual Integrations

APPROVED

MMDadoda

8/20/2019 12:41:22 PM

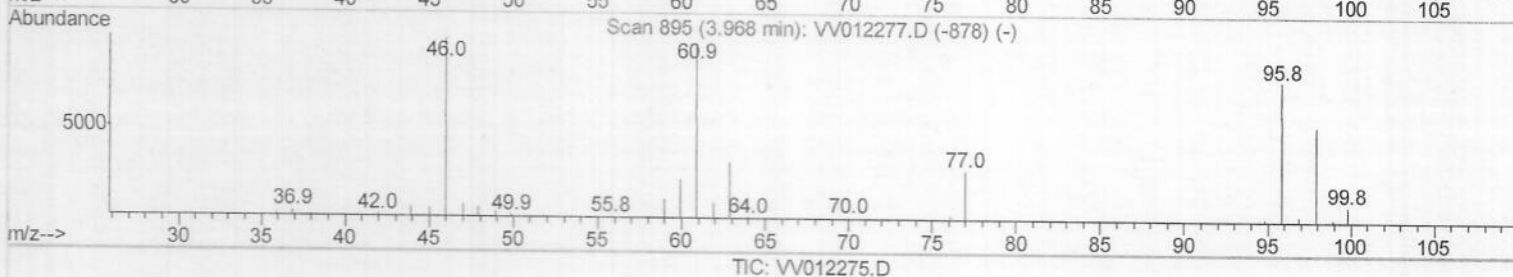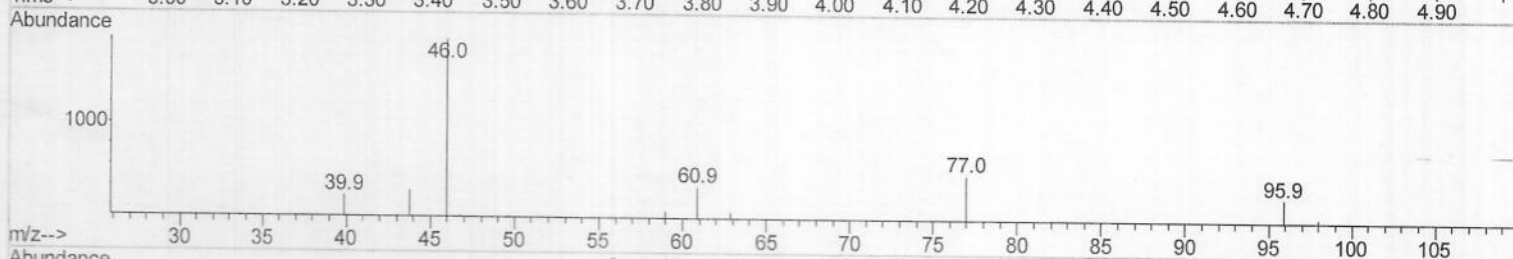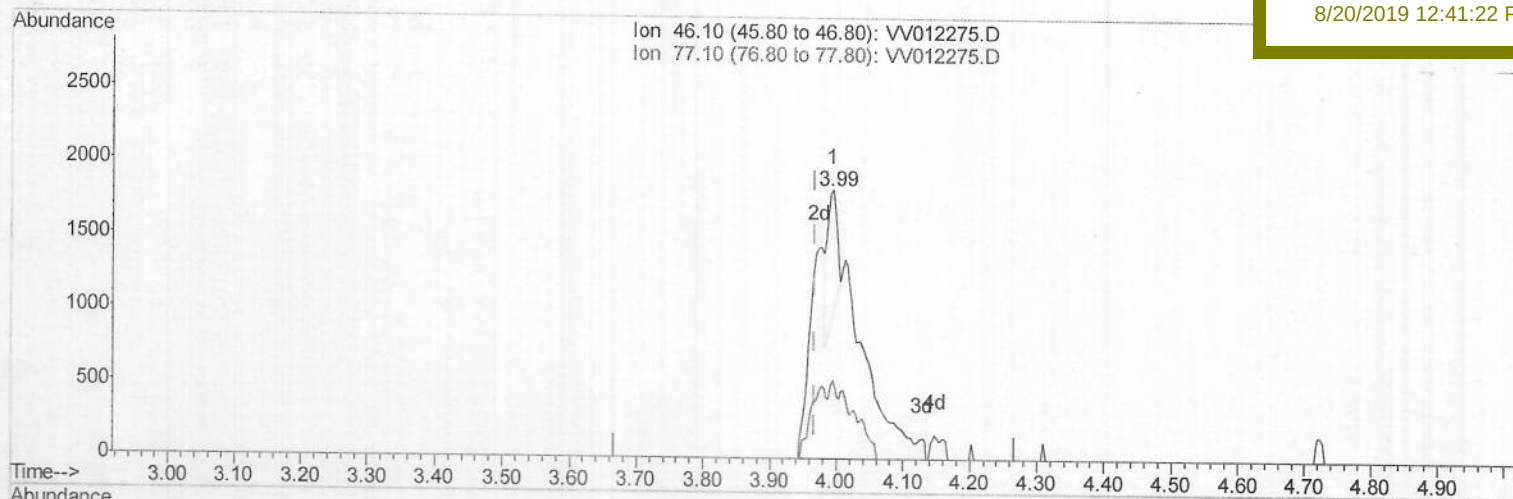

(20) 2-Butanone-d5 (S)

3.994min (+0.026) 0.56ug/L

response 908

Ion	Exp%	Act%
46.10	100	100
77.10	15.10	12.44
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081919\

Data File : VV012275.D

Acq On : 19 Aug 2019 13:01

Operator : SY/MD

Sample : VSTD0.532

Misc : 25mL/MSVOA V/WATER

ALS Vial : 2 Sample Multiplier: 1

Quant Time: Aug 19 18:26:49 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081919WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Mon Aug 19 18:23:47 2019

Response via : Initial Calibration

Instrument :

MSVOA_V


ClientSampled :

VSTD0.532

Manual Integrations
APPROVED

MMDadoda

8/20/2019 12:41:22 PM

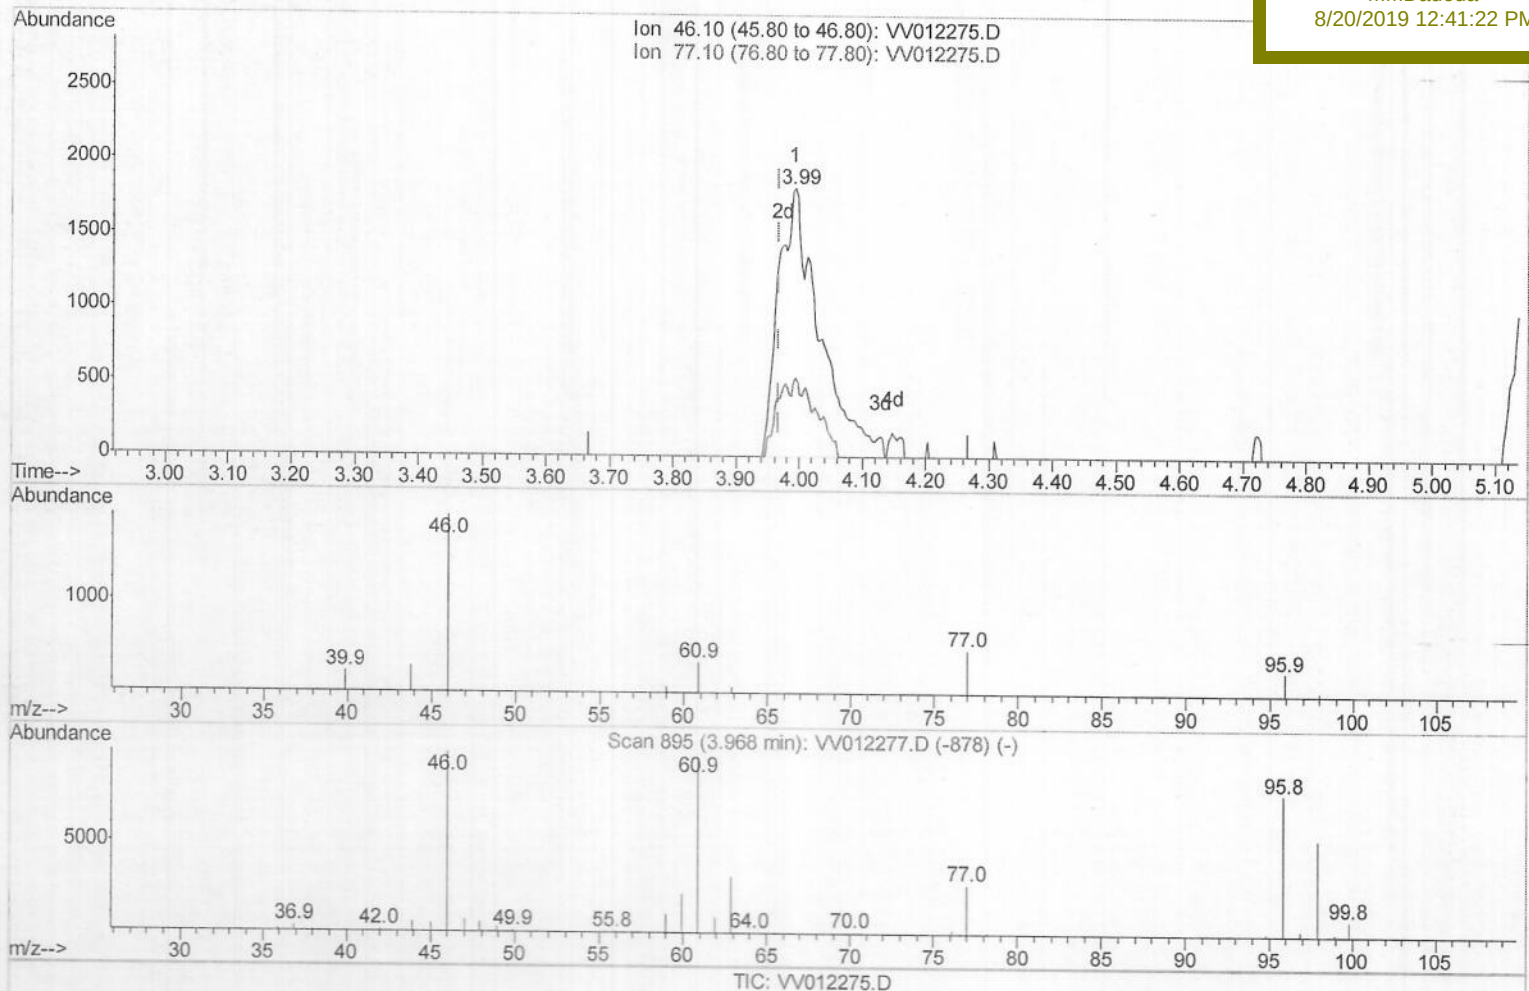

(20) 2-Butanone-d5 (S)

3.994min (+0.026) 5.02ug/L m) M08/28/19

response 8198

Ion	Exp%	Act%
46.10	100	100
77.10	15.10	1.38#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081919\

Data File : VV012275.D

Acq On : 19 Aug 2019 13:01

Operator : SY/MD

Sample : VSTD0.532

Misc : 25mL/MSVOA V/WATER

ALS Vial : 2 Sample Multiplier: 1

Quant Time: Aug 19 18:52:40 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081919WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Mon Aug 19 18:23:47 2019

Response via : Initial Calibration

Instrument :

MSVOA_V

ClientSampleId :


VSTD0.532

Manual Integrations

APPROVED

MMDadoda

8/20/2019 12:41:22 PM

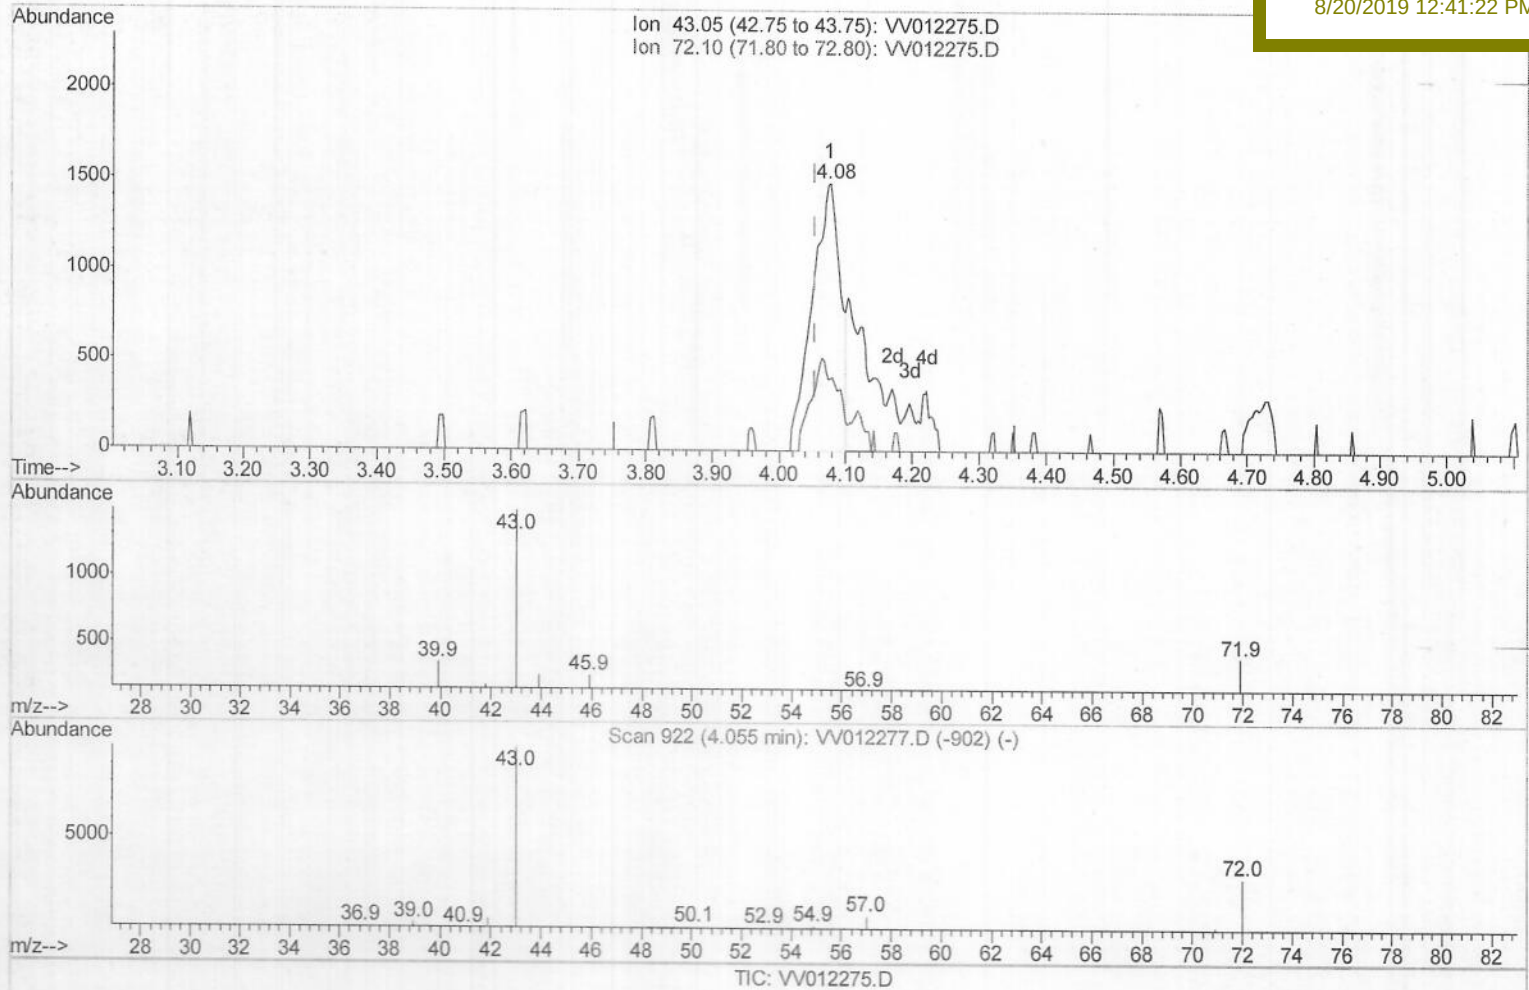

(21) 2-Butanone (T)

4.077min (+0.022) 2.21ug/L

response 4338

Ion	Exp%	Act%
43.05	100	100
72.10	29.60	32.60
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081919\

Data File : VV012275.D

Acq On : 19 Aug 2019 13:01

Operator : SY/MD

Sample : VSTD0.532

Misc : 25mL/MSVOA V/WATER

ALS Vial : 2 Sample Multiplier: 1

Quant Time: Aug 19 18:52:40 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081919WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Mon Aug 19 18:23:47 2019

Response via : Initial Calibration

Instrument :

MSVOA_V

ClientSampleId :




VSTD0.532

Manual Integrations

APPROVED

MMDadoda

8/20/2019 12:41:22 PM

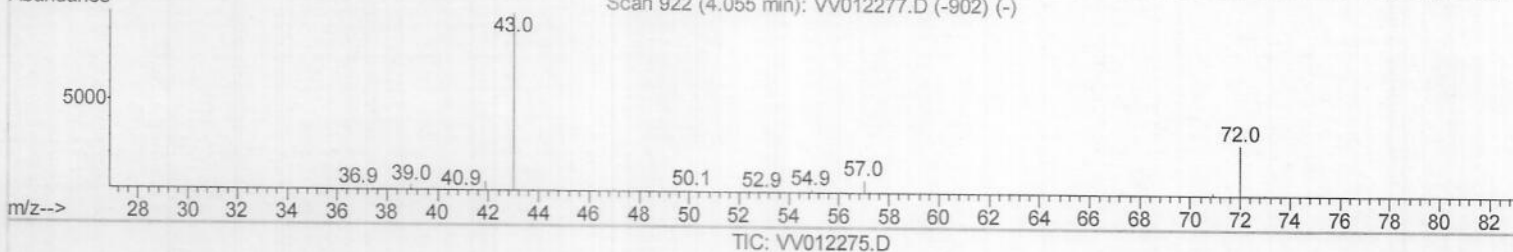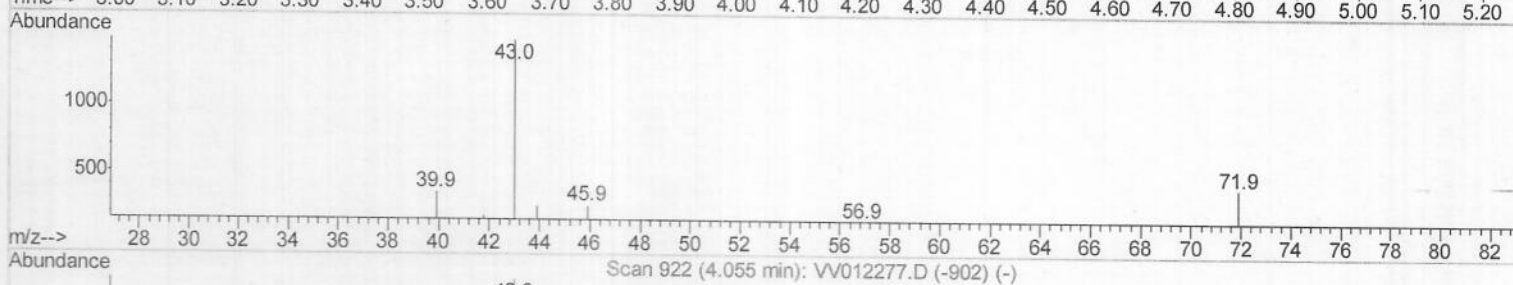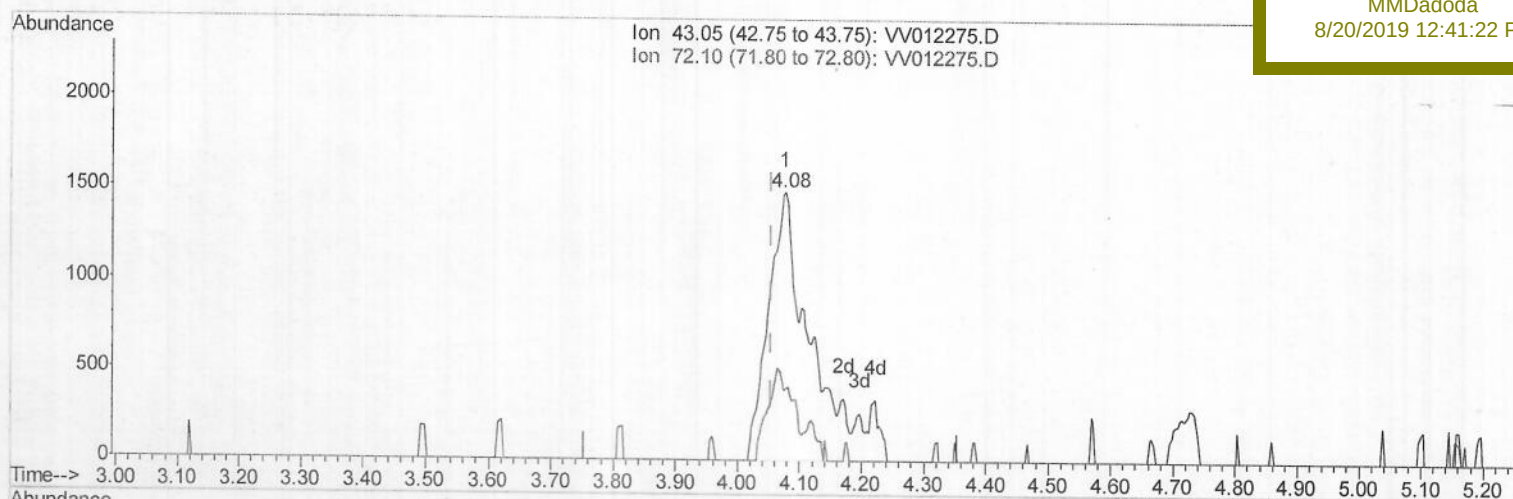

(21) 2-Butanone (T)

4.077min (+0.022) 3.72ug/L m > MD08128119

response 7290

Ion	Exp%	Act%
43.05	100	100
72.10	29.60	19.40
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081919\

Data File : VV012275.D

Acq On : 19 Aug 2019 13:01

Operator : SY/MD

Sample : VSTD0.532

Misc : 25mL/MSVOA V/WATER

ALS Vial : 2 Sample Multiplier: 1

Quant Time: Aug 19 18:53:06 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081919WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Mon Aug 19 18:23:47 2019

Response via : Initial Calibration

Instrument :

MSVOA_V

Client Sampled :

VSTD0.532

Manual Integrations

APPROVED

MMDadoda

8/20/2019 12:41:22 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.66	114	122635	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	118011	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	59415	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	3107	0.41	ug/L	0.00
7) Chloroethane-d5	1.58	69	2502	0.45	ug/L	0.00
11) 1,1-Dichloroethene-d2	2.13	63	6385	0.50	ug/L	0.00
20) 2-Butanone-d5	3.99	46	8198m)	5.02	ug/L	0.03
24) Chloroform-d	4.40	84	8581	0.56	ug/L	0.00
26) 1,2-Dichloroethane-d4	5.09	65	4526	0.61	ug/L	0.00
32) Benzene-d6	5.09	84	16346	0.54	ug/L	0.00
36) 1,2-Dichloropropane-d6	6.12	67	4692	0.54	ug/L	0.00
41) Toluene-d8	7.36	98	13495	0.48	ug/L	0.00
43) trans-1,3-Dichloropropene-	7.67	79	1578	0.45	ug/L	0.00
46) 2-Hexanone-d5	8.14	63	4533	4.14	ug/L	0.00
57) 1,1,2,2-Tetrachloroethane-	10.26	84	3585	0.58	ug/L	0.00
64) 1,2-Dichlorobenzene-d4	11.67	152	6915	0.66	ug/L	0.00

MD08/28/19

Target Compounds

						Ovalue
2) Dichlorodifluoromethane	1.14	85	6573	0.524	ug/L	98
3) Chloromethane	1.25	50	3471	0.340	ug/L	85
5) Vinyl chloride	1.32	62	3623	0.345	ug/L	95
6) Bromomethane	1.54	94	1949	0.337	ug/L	94
8) Chloroethane	1.60	64	2047	0.352	ug/L	94
9) Trichlorofluoromethane	1.77	101	6154	0.436	ug/L	93
10) 1,1,2-Trichloro-1,2,2-trif	2.14	101	2677	0.382	ug/L	88
12) 1,1-Dichloroethene	2.14	96	2319	0.357	ug/L	81
13) Acetone	2.25	43	4716m)	4.703	ug/L	
14) Carbon disulfide	2.32	76	7630	0.413	ug/L	97
15) Methyl Acetate	2.47	43	883	0.365	ug/L	# 64
16) Methylene chloride	2.53	84	3163	0.465	ug/L	96
17) Methyl tert-butyl Ether	2.81	73	7507	0.419	ug/L	97
18) trans-1,2-Dichloroethene	2.78	96	3760	0.438	ug/L	95
19) 1,1-Dichloroethane	3.23	63	5925	0.382	ug/L	92
21) 2-Butanone	4.08	43	7290m)	3.716	ug/L	
22) cis-1,2-Dichloroethene	3.96	96	3685	0.393	ug/L	98
23) Bromochloromethane	4.30	128	1744	0.431	ug/L	95
25) Chloroform	4.42	83	9009	0.502	ug/L	93
27) 1,2-Dichloroethane	5.18	62	4080	0.410	ug/L	97
29) 1,1,1-Trichloroethane	4.66	97	6739	0.460	ug/L	99
30) Cyclohexane	4.73	56	4594	0.335	ug/L	96
31) Carbon tetrachloride	4.87	117	6045	0.453	ug/L	97
33) Benzene	5.14	78	13503	0.390	ug/L	100
34) Trichloroethene	5.96	95	4059	0.423	ug/L	96
35) Methylcyclohexane	6.17	83	5681	0.387	ug/L	98
37) 1,2-Dichloropropane	6.22	63	3288	0.385	ug/L	# 91
38) Bromodichloromethane	6.55	83	4860	0.424	ug/L	# 94
39) cis-1,3-Dichloropropene	7.07	75	4490	0.370	ug/L	98
40) 4-Methyl-2-pentanone	7.28	43	14788	3.168	ug/L	100

MD08/28/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081919\

Data File : VV012275.D

Acq On : 19 Aug 2019 13:01

Operator : SY/MD

Sample : VSTD0.532

Misc : 25mL/MSVOA V/WATER

ALS Vial : 2 Sample Multiplier: 1

Quant Time: Aug 19 18:53:06 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081919WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Mon Aug 19 18:23:47 2019

Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.532

Manual Integrations
APPROVED

MMDadoda
8/20/2019 12:41:22 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
42) Toluene	7.43	91	13772	0.369	uq/L	100
44) trans-1,3-Dichloropropene	7.70	75	3769	0.390	uq/L	94
45) 1,1,2-Trichloroethane	7.88	97	2549	0.434	uq/L	91
47) Tetrachloroethene	8.02	164	3937	0.486	uq/L	91
48) 2-Hexanone	8.20	43	11143	3.405	uq/L	95
49) Dibromochloromethane	8.29	129	3326	0.447	uq/L	96
50) 1,2-Dibromoethane	8.40	107	2261	0.400	uq/L #	93
51) Chlorobenzene	8.92	112	10379	0.425	uq/L	94
52) Ethylbenzene	9.05	91	15384	0.382	uq/L	94
53) m,p-xylene	9.18	106	5608	0.360	uq/L	92
54) o-xylene	9.59	106	5582	0.379	uq/L	85
55) Styrene	9.60	104	9454	0.385	uq/L	90
56) Isopropylbenzene	9.97	105	15929	0.402	uq/L	98
58) 1,1,2,2-Tetrachloroethane	10.29	83	2105	0.316	uq/L #	83
59) 1,2,3-Trichloropropane	10.32	75	1950	0.394	uq/L	92
61) Bromoform	9.77	173	1642	0.426	uq/L #	87
62) 1,3-Dichlorobenzene	11.22	146	8997	0.457	uq/L	99
63) 1,4-Dichlorobenzene	11.32	146	9171	0.466	uq/L	95
65) 1,2-Dichlorobenzene	11.69	146	8274	0.458	uq/L	92
67) 1,3,5-Trichlorobenzene	12.69	180	7096	0.468	uq/L	98
68) 1,2,4-trichlorobenzene	13.31	180	4591	0.406	uq/L	94
69) Naphthalene	13.55	128	5766	0.362	uq/L #	95
70) 1,2,3-Trichlorobenzene	13.79	180	4429	0.419	uq/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed