

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081919\
 Data File : VV012284.D
 Acq On : 19 Aug 2019 18:33
 Operator : SY/MD
 Sample : K4395-01
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ5

Quant Time: Aug 20 02:48:23 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Aug 20 02:35:23 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	115255	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	111638	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	51933	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	28022	4.76	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.20%
7) Chloroethane-d5	1.58	69	21348	4.96	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.20%
11) 1,1-Dichloroethene-d2	2.13	63	40701	3.64	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.80%
20) 2-Butanone-d5	3.94	46	83985	52.89	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.78%
24) Chloroform-d	4.40	84	81045	5.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.80%
26) 1,2-Dichloroethane-d4	5.08	65	42272	5.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.00%
32) Benzene-d6	5.10	84	150288	5.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.80%
36) 1,2-Dichloropropane-d6	6.12	67	42691	5.11	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.20%
41) Toluene-d8	7.36	98	131902	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.00%
43) trans-1,3-Dichloropropene-	7.66	79	17607	4.91	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.20%
46) 2-Hexanone-d5	8.13	63	50818	44.91	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.82%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	28438	4.48	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	55151	5.28	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.60%


Target Compounds				Ovalue
13) Acetone	2.20	43	7103	8.552 ug/L # 55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081919\
Data File : VV012284.D
Acq On : 19 Aug 2019 18:33
Operator : SY/MD
Sample : K4395-01
Misc : 25mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ5

Quant Time: Aug 20 02:48:23 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 20 02:35:23 2019
Response via : Initial Calibration

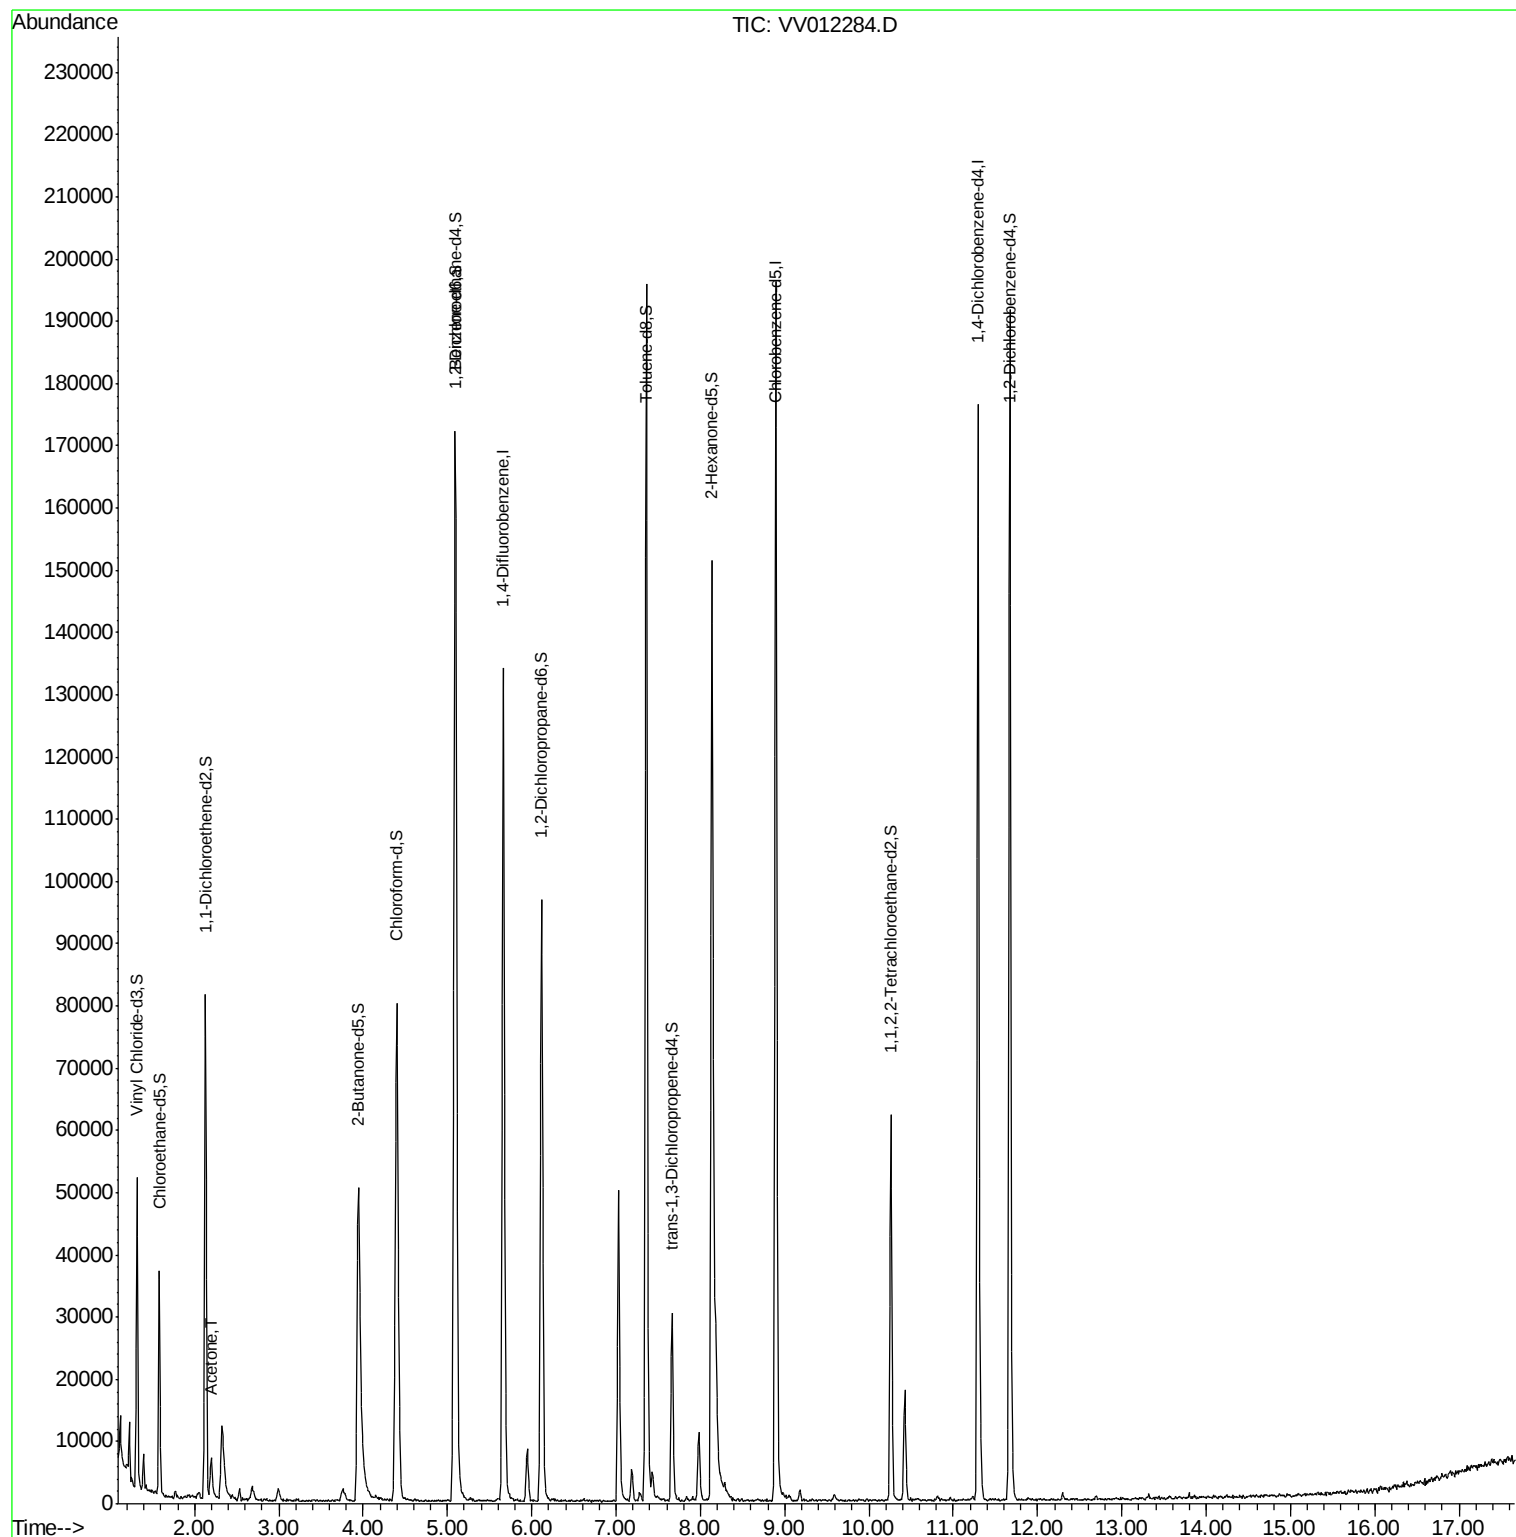

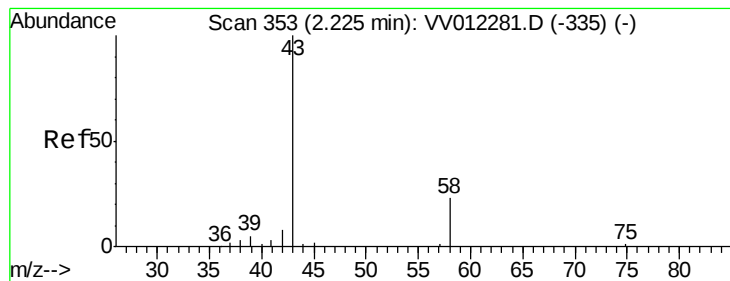

#13
 Acetone
 Concen: 8.552 ug/L
 RT: 2.20 min Scan# 344
 Delta R.T. -0.03 min
 Lab File: VV012284.D
 Acq: 19 Aug 2019 18:33

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ5

Tot Ion: 43 Resp: 7103
 Ion Ratio Lower Upper
 43 100
 58 30.8 0.0 25.6#

