

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081919\
 Data File : VV012290.D
 Acq On : 19 Aug 2019 21:19
 Operator : SY/MD
 Sample : K4395-05
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF0

Quant Time: Aug 20 03:58:55 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Aug 20 02:35:23 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	151241	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	146976	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	80474	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	29093	3.76	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.20%
7) Chloroethane-d5	1.58	69	21616	3.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	76.60%
11) 1,1-Dichloroethene-d2	2.13	63	40508	2.76	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	55.20%#
20) 2-Butanone-d5	3.94	46	89255	42.84	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	85.68%
24) Chloroform-d	4.40	84	79693	3.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	76.20%
26) 1,2-Dichloroethane-d4	5.08	65	44560	4.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.80%
32) Benzene-d6	5.10	84	149601	3.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	77.00%
36) 1,2-Dichloropropane-d6	6.12	67	42496	3.87	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	77.40%
41) Toluene-d8	7.36	98	140201	3.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.40%
43) trans-1,3-Dichloropropene-	7.66	79	18170	3.85	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.00%
46) 2-Hexanone-d5	8.14	63	67561	45.35	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.70%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	34986	4.19	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	66639	4.12	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	82.40%


Target Compounds					Ovalue
13) Acetone	2.20	43	3348	3.072 ug/L	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081919\
Data File : VV012290.D
Acq On : 19 Aug 2019 21:19
Operator : SY/MD
Sample : K4395-05
Misc : 25mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF0

Quant Time: Aug 20 03:58:55 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 20 02:35:23 2019
Response via : Initial Calibration

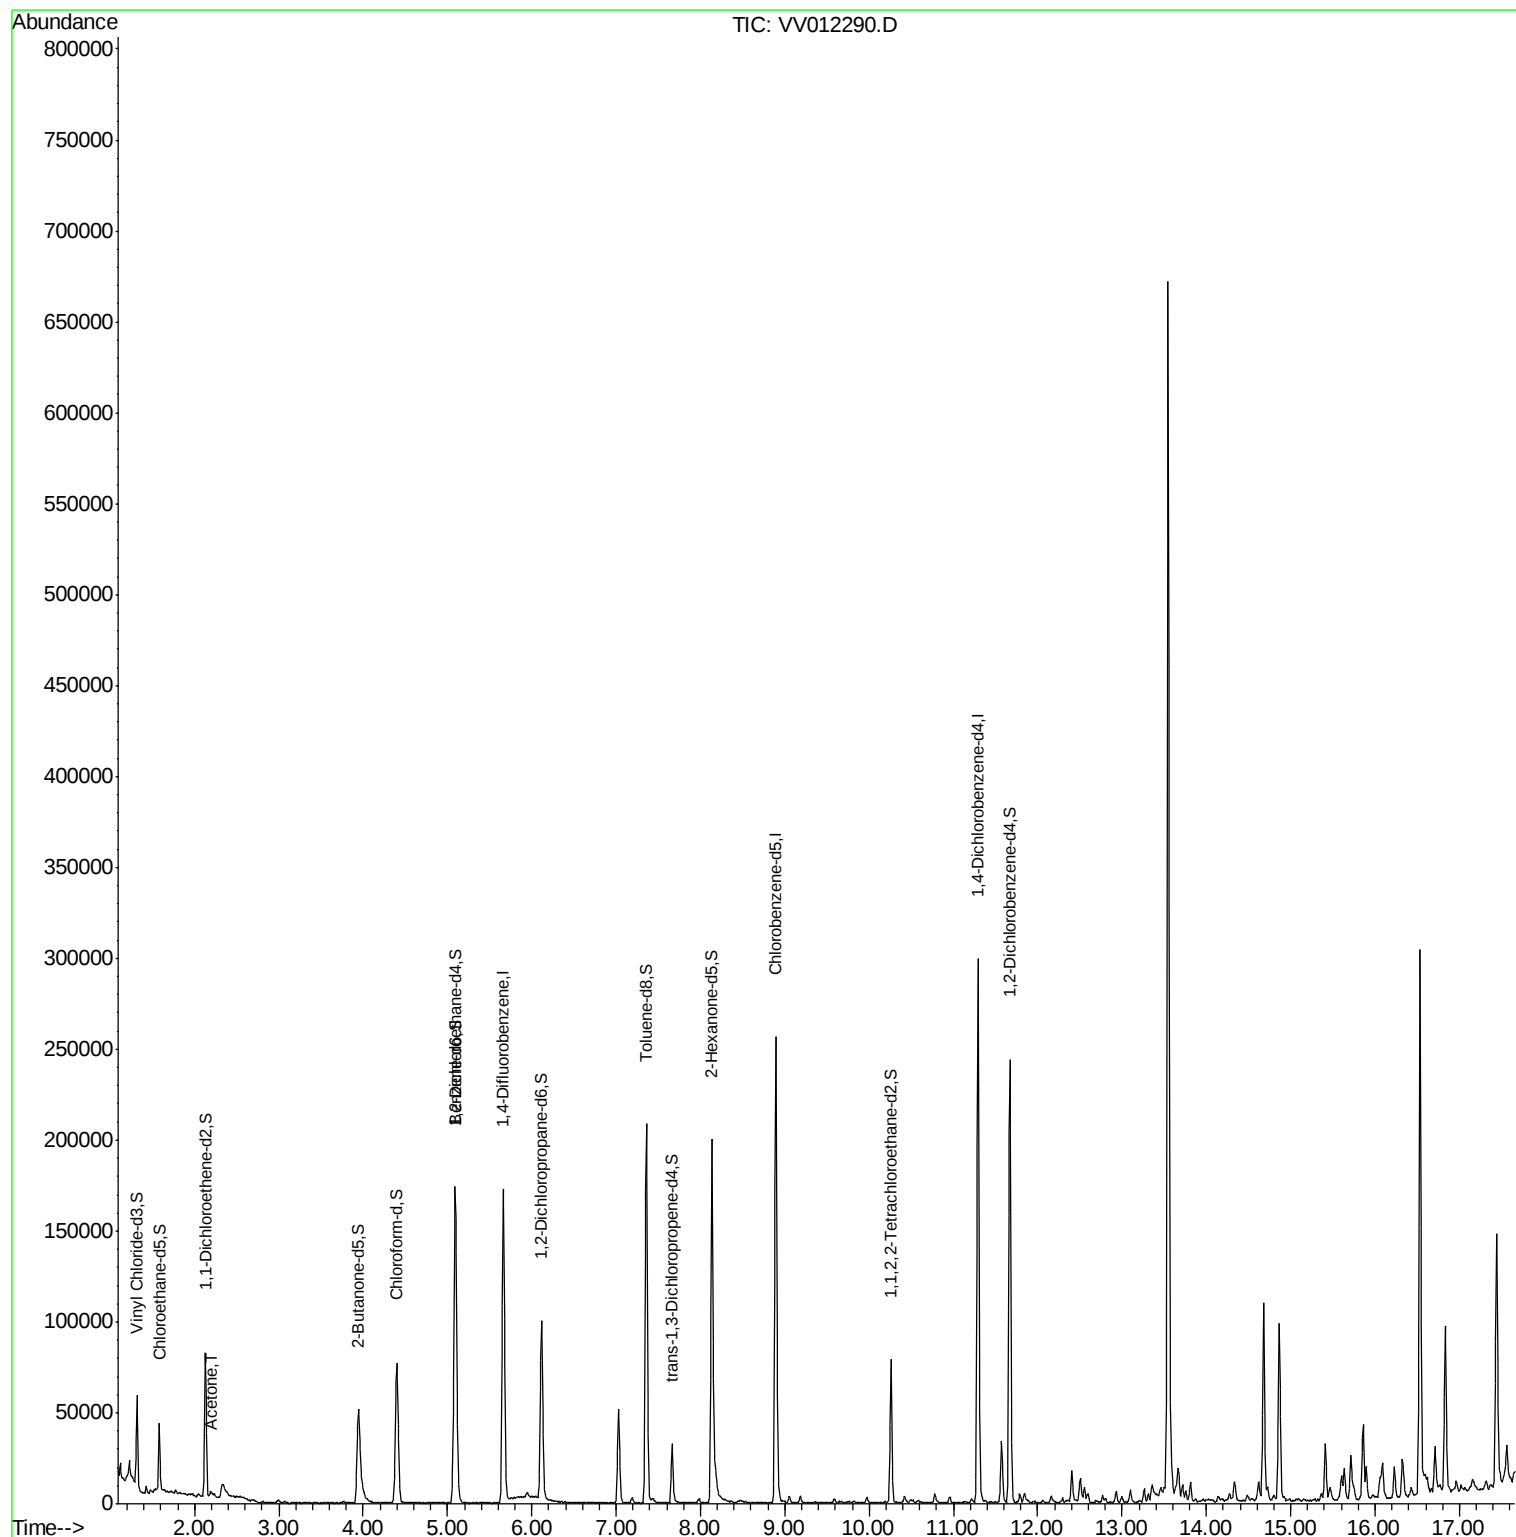

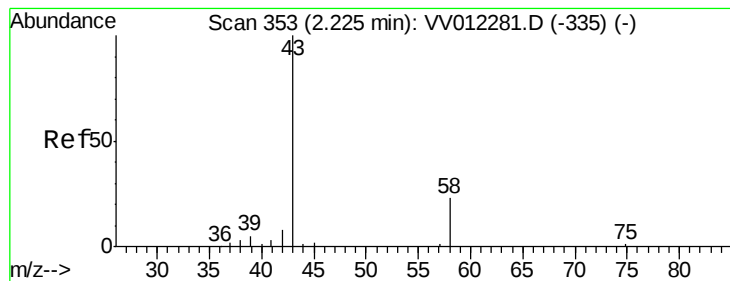

#13

Acetone

Concen: 3.072 ug/L

RT: 2.20 min Scan# 344

Delta R.T. -0.03 min

Lab File: VV012290.D

Acq: 19 Aug 2019 21:19

Instrument :
MSVOA_V
ClientSampleId :
C0AF0

Tot Ion: 43 Resp: 3348

Ion Ratio Lower Upper

43 100

58 23.2 0.0 25.6

