

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV081919\
 Data File : VV012298.D
 Acq On : 20 Aug 2019 00:59
 Operator : SY/MD
 Sample : K4373-17
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD8

Quant Time: Aug 20 04:35:43 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Aug 20 02:35:23 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	240975	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	224668	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	107409	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	66718	5.42	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	108.40%
7) Chloroethane-d5	1.58	69	55032	6.12	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	122.40%
11) 1,1-Dichloroethene-d2	2.13	63	81857	3.50	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.00%
20) 2-Butanone-d5	3.93	46	219106	66.00	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	132.00%#
24) Chloroform-d	4.40	84	142847	4.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.80%
26) 1,2-Dichloroethane-d4	5.08	65	75417	4.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.00%
32) Benzene-d6	5.10	84	292900	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.60%
36) 1,2-Dichloropropane-d6	6.12	67	89337	5.32	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.40%
41) Toluene-d8	7.36	98	254293	4.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.00%
43) trans-1,3-Dichloropropene-	7.66	79	32725	4.53	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.60%
46) 2-Hexanone-d5	8.13	63	163052	71.60	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	143.20%#
57) 1,1,2,2-Tetrachloroethane-	10.26	84	71078	5.57	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	111.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	103837	4.81	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.20%


Target Compounds					Ovalue
13) Acetone	2.18	43	3267	1.881 ug/L	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV081919\
Data File : VV012298.D
Acq On : 20 Aug 2019 00:59
Operator : SY/MD
Sample : K4373-17
Misc : 25mL/MSVOA V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD8

Quant Time: Aug 20 04:35:43 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 20 02:35:23 2019
Response via : Initial Calibration

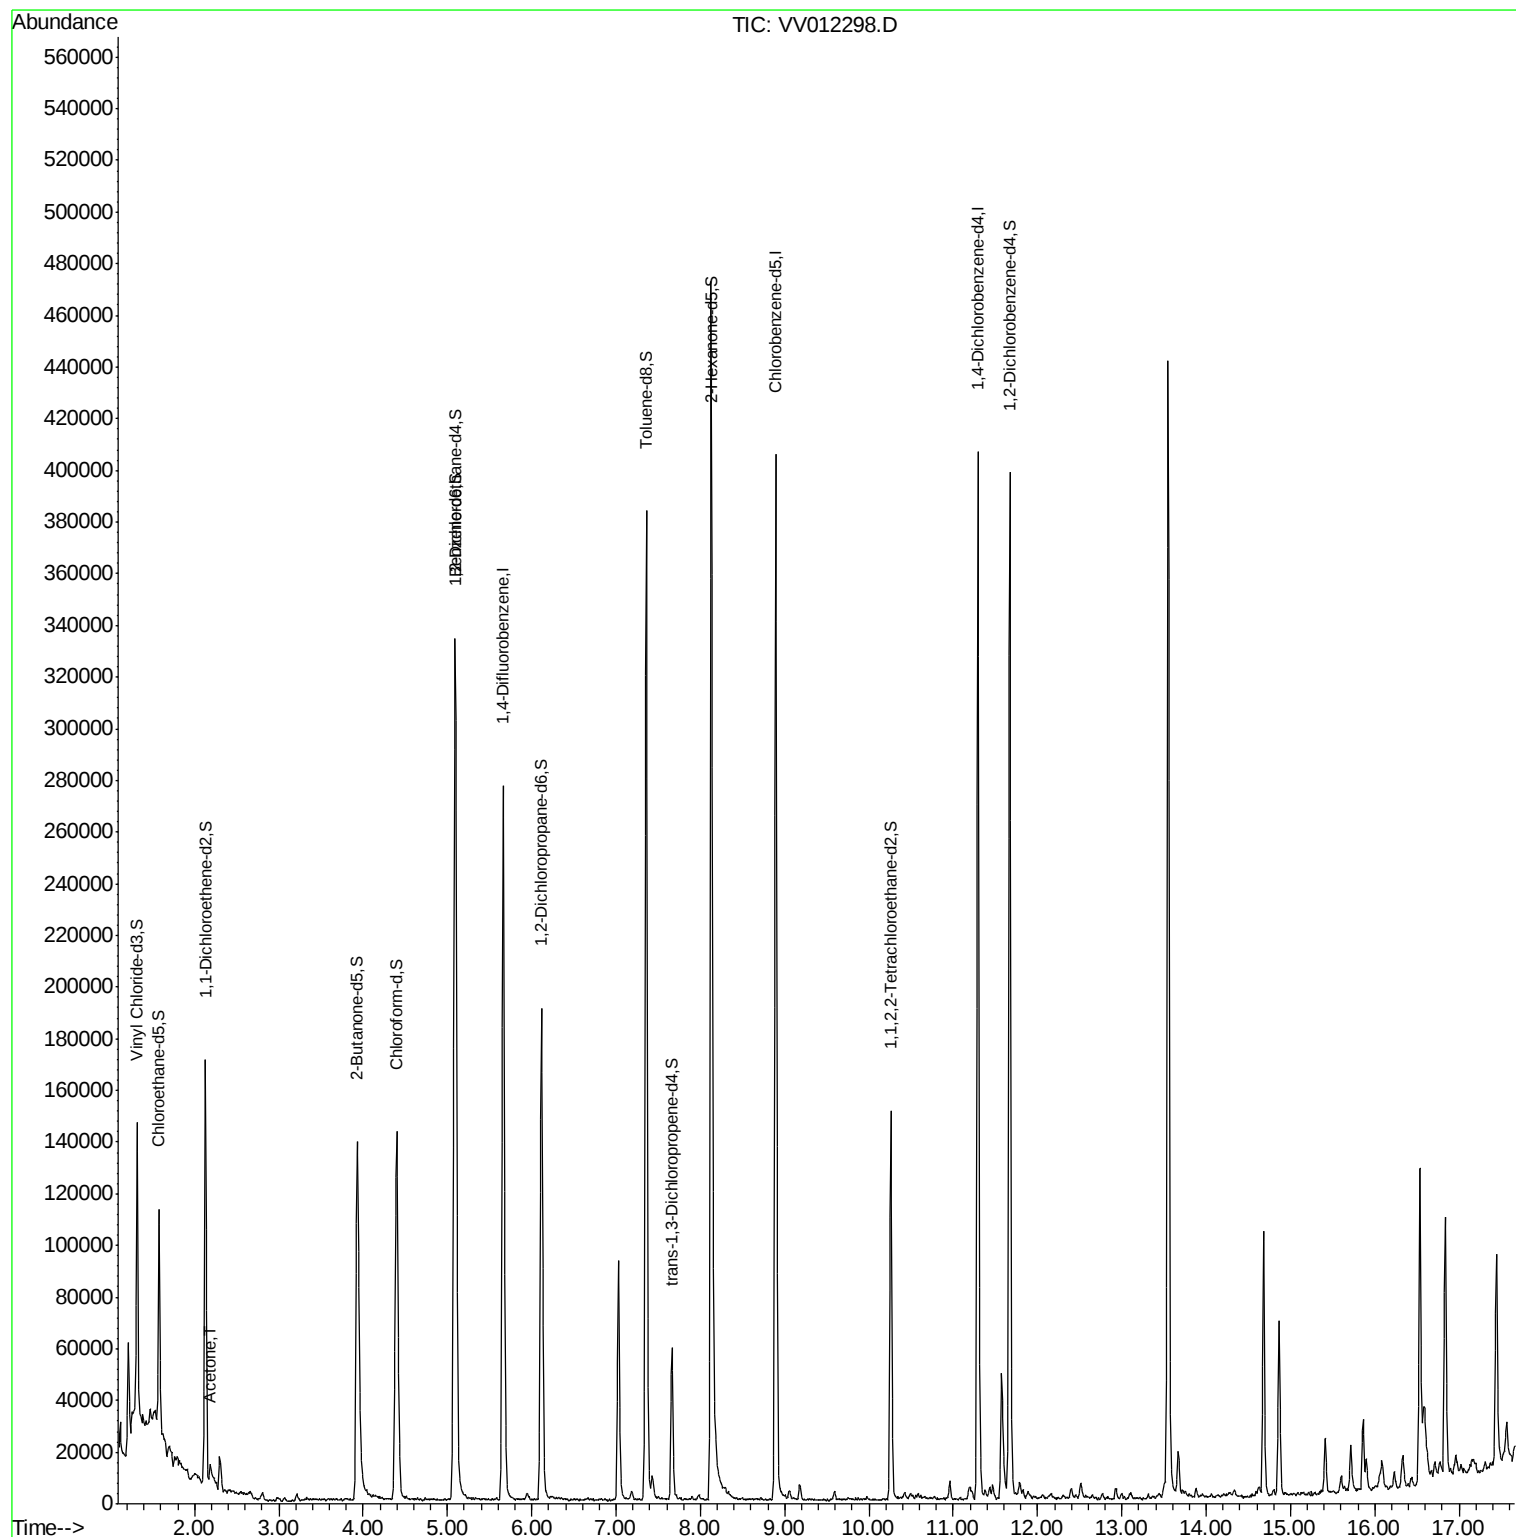

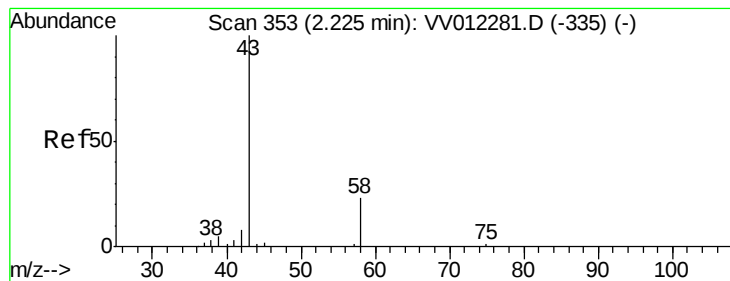

#13

Acetone

Concen: 1.881 ug/L

RT: 2.18 min Scan# 340

Delta R.T. -0.04 min

Lab File: VV012298.D

Acq: 20 Aug 2019 00:59

Instrument :
MSVOA_V
ClientSampleId :
C0AD8

Tot Ion: 43 Resp: 3267

Ion Ratio Lower Upper

43 100

58 25.2 0.0 25.6

