


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV081919\
 Data File : VV012274.D
 Acq On : 19 Aug 2019 12:31
 Operator : SY/MD
 Sample : BFB50
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB50

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081919WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Aug 21 01:13:54 2019

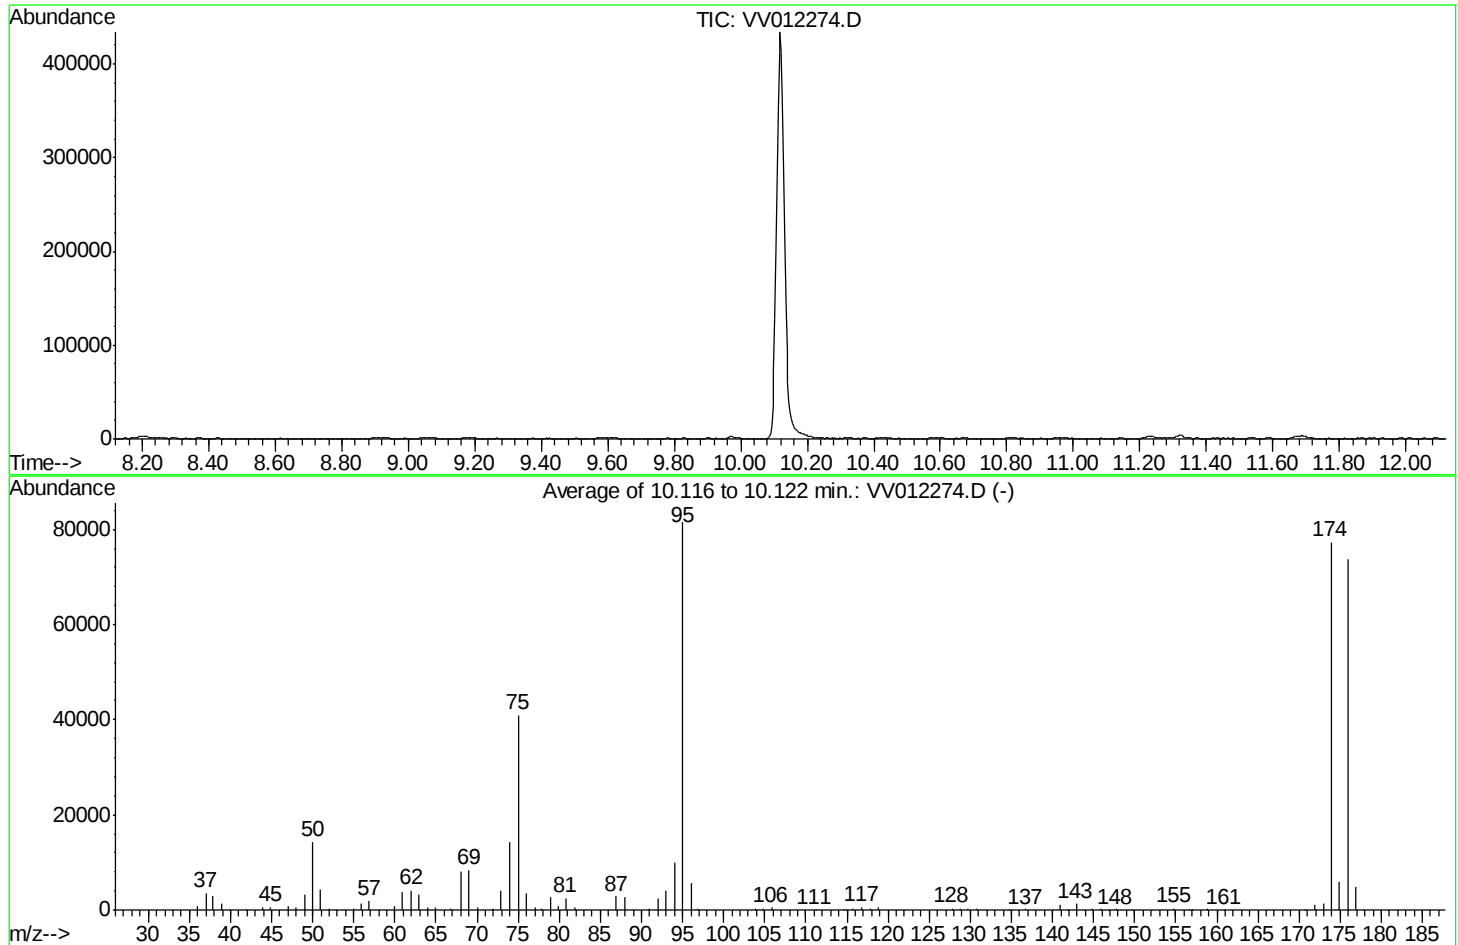

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	14274	PASS
75	95	30	80	50.3	40994	PASS
95	95	100	100	100.0	81477	PASS
96	95	5	9	7.1	5768	PASS
173	174	0.00	2	1.7	1283	PASS
174	95	50	120	94.9	77328	PASS
175	174	5	9	7.5	5809	PASS
176	174	95	101	95.3	73666	PASS
177	176	5	9	6.7	4953	PASS

m/z	Abundance
36.00	771.0
37.00	3406.0
37.90	2948.0
38.90	1217.0
39.80	347.0
41.90	108.0
43.90	754.0
44.90	654.0
47.10	742.0
48.00	450.0
49.00	3114.0
50.00	14115.0
50.90	4513.0
51.90	188.0
52.80	104.0
55.00	189.0
55.90	1426.0
56.90	1897.0
58.00	146.0
60.00	824.0
60.90	3856.0
62.00	4048.0
62.90	3117.0
64.00	435.0
64.90	579.0
66.80	216.0
68.00	8086.0
69.00	8400.0
70.10	460.0
72.10	412.0
72.90	4299.0
74.00	13933.0
75.00	40640.0
76.00	3740.0
77.00	507.0
77.80	372.0
78.90	2670.0
80.00	718.0
80.80	2509.0
81.80	517.0
86.00	167.0
86.90	2751.0
87.90	2690.0
90.90	279.0
91.90	2409.0
92.90	4032.0
94.00	9711.0
95.00	81064.0
96.00	5875.0
96.90	204.0
103.90	429.0
104.80	140.0
105.80	401.0
114.90	142.0
115.70	333.0
116.80	584.0
117.90	304.0
118.80	432.0
127.80	312.0
128.80	208.0
129.70	330.0
130.90	160.0
134.70	136.0
135.00	131.0
136.70	155.0
140.80	1030.0
142.90	1276.0
143.90	115.0
144.80	218.0
145.90	146.0
147.70	229.0
154.90	291.0
156.70	116.0
158.90	134.0
160.90	155.0
170.80	153.0
171.90	965.0
173.00	1322.0
173.90	74328.0
174.90	5659.0
175.90	70832.0
176.90	4805.0
177.80	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB50

m/z	Abundance
36.00	818.0
37.00	3615.0
37.90	3057.0
38.90	1340.0
39.80	351.0
41.90	125.0
43.90	687.0
44.90	575.0
47.10	758.0
47.90	546.0
49.00	3260.0
50.00	14710.0
51.00	4514.0
52.00	217.0
54.90	218.0
55.90	1408.0
56.90	1987.0
58.00	127.0
59.90	773.0
60.90	3942.0
62.00	4251.0
62.90	3243.0
63.90	455.0
64.90	495.0
66.90	250.0
68.00	8244.0
69.00	8610.0
70.00	493.0
72.00	407.0
72.90	4324.0
74.00	14678.0
75.00	42192.0
76.00	3712.0
77.00	499.0
77.90	360.0
78.90	2910.0
80.00	731.0
80.80	2641.0
81.80	585.0
86.00	137.0
86.90	2989.0
87.90	2843.0
90.90	268.0
92.00	2449.0
92.90	4204.0
94.00	10356.0
95.00	84176.0
96.00	6072.0
96.90	212.0
103.90	361.0
104.70	164.0
105.80	450.0
111.10	104.0
114.80	144.0
115.70	391.0
116.80	619.0
117.90	338.0
118.80	481.0
127.80	386.0
128.80	210.0
129.70	375.0
130.80	207.0
134.70	140.0
135.10	150.0
136.80	182.0
140.90	1037.0
141.90	140.0
142.90	1366.0
143.90	116.0
144.80	253.0
145.90	185.0
146.90	103.0
147.70	246.0
154.90	303.0
156.70	125.0
158.80	166.0
170.70	137.0
171.90	1022.0
173.00	1343.0
173.90	79944.0
174.90	6054.0
175.90	75960.0
176.90	5055.0

Instrument :
MSVOA_V
ClientSampleId :
BFB50

m/z	Abundance
36.00	762.0
37.00	3600.0
37.90	2864.0
39.00	1398.0
39.80	330.0
43.90	617.0
44.90	490.0
47.00	691.0
47.90	531.0
49.00	3165.0
50.00	13999.0
51.00	4187.0
52.00	225.0
54.90	218.0
55.90	1236.0
56.90	2015.0
59.90	707.0
60.90	3636.0
62.00	3879.0
63.00	3024.0
63.90	485.0
64.90	448.0
66.90	301.0
68.00	7681.0
69.00	8035.0
70.00	499.0
71.90	373.0
72.90	3809.0
74.00	14004.0
75.00	40152.0
76.00	3380.0
77.00	436.0
78.00	335.0
78.90	2740.0
79.90	649.0
80.80	2523.0
81.90	625.0
85.80	110.0
86.90	2909.0
87.90	2782.0
90.90	273.0
92.00	2394.0
92.90	3834.0
94.00	10036.0
95.00	79192.0
96.00	5359.0
96.90	183.0
103.90	293.0
104.80	167.0
105.90	472.0
114.60	125.0
115.70	389.0
116.80	628.0
118.00	321.0
118.80	518.0
127.80	404.0
128.80	182.0
129.70	373.0
130.70	199.0
134.70	135.0
135.10	136.0
136.80	191.0
140.90	986.0
141.90	174.0
142.90	1319.0
144.80	244.0
145.90	191.0
146.90	123.0
147.70	255.0
149.70	101.0
154.80	258.0
156.90	132.0
158.80	171.0
170.60	105.0
171.90	976.0
173.00	1184.0
173.90	77712.0
174.90	5715.0
175.90	74208.0
176.90	5001.0

Instrument :
MSVOA_V
ClientSampleId :
BFB50

Scan 2794 (10.074 min): VV012274.D
BFB50

m/z	Abundance
39.90	319.0
44.00	229.0

Instrument :
MSVOA_V
ClientSampleId :
BFB50