


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV081920\
 Data File : VV018055.D
 Acq On : 19 Aug 2020 09:27
 Operator : SY/MD
 Sample : BFB77
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB77

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Title : VOC Analysis
 Last Update : Thu Aug 20 04:32:09 2020

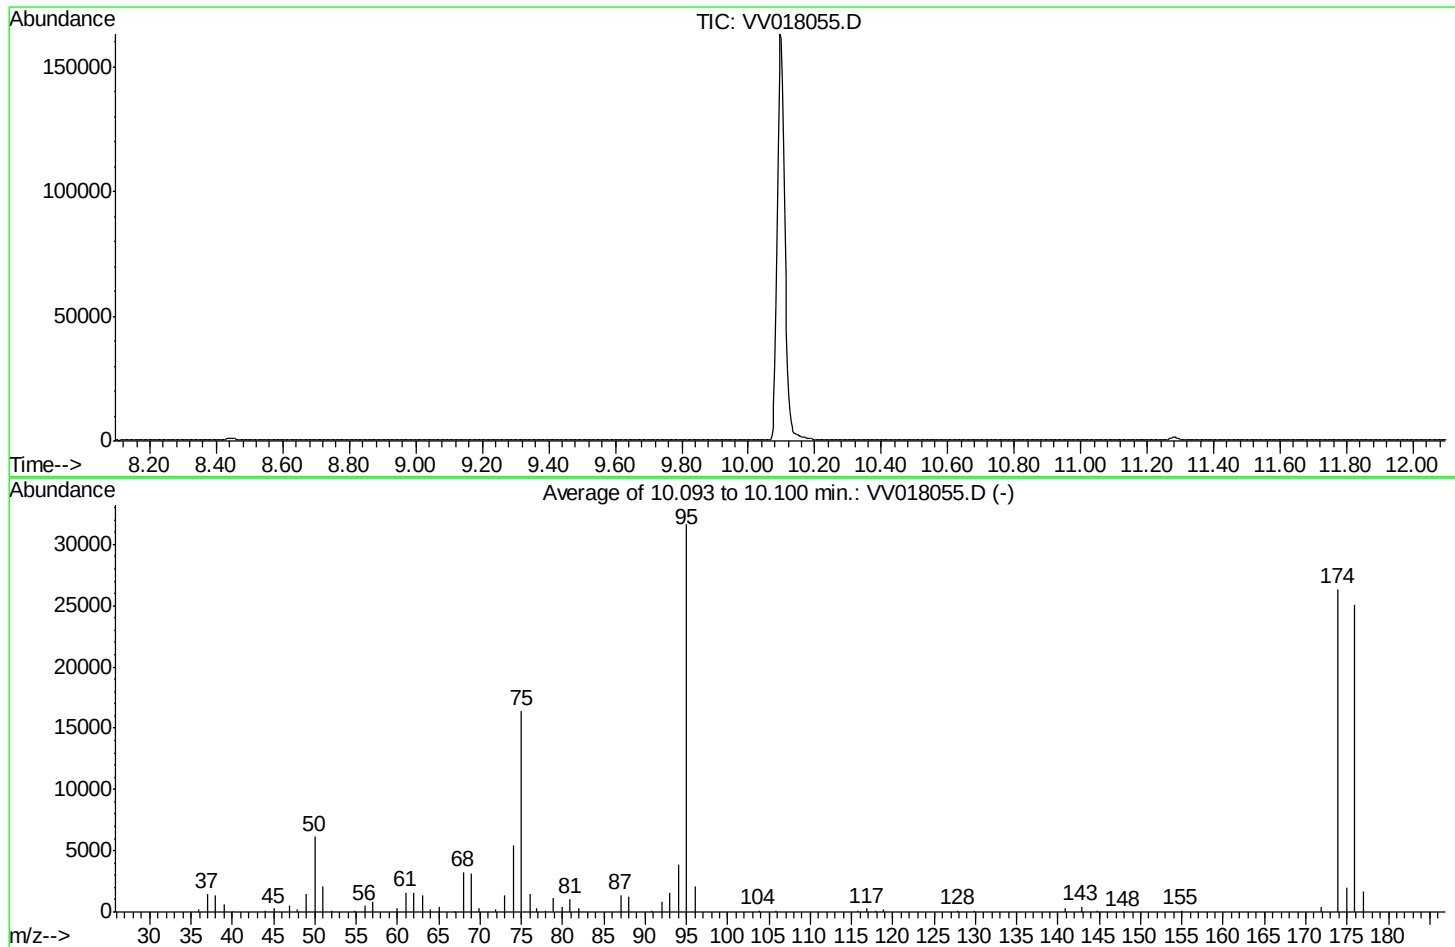

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	6135	PASS
75	95	30	80	51.9	16419	PASS
95	95	100	100	100.0	31637	PASS
96	95	5	9	6.5	2051	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.2	26328	PASS
175	174	5	9	7.4	1950	PASS
176	174	95	101	95.3	25085	PASS
177	176	5	9	6.6	1668	PASS

m/z	Abundance
35.00	268.0
37.00	1453.0
38.00	1242.0
39.00	619.0
40.00	193.0
44.00	432.0
45.00	251.0
47.00	487.0
47.90	179.0
49.00	1392.0
50.00	5859.0
51.00	1895.0
52.00	121.0
54.90	144.0
56.00	475.0
57.00	770.0
59.90	293.0
61.00	1447.0
62.00	1436.0
63.00	1306.0
64.00	222.0
65.00	444.0
66.90	102.0
68.00	3094.0
69.00	3035.0
69.90	272.0
71.90	211.0
73.00	1347.0
74.00	5060.0
75.00	15609.0
76.00	1366.0
76.90	281.0
77.90	140.0
78.90	1028.0
79.90	367.0
80.90	1008.0
81.90	307.0
87.00	1310.0
88.00	1231.0
90.80	151.0
92.00	875.0
93.00	1617.0
94.00	3686.0
95.00	29952.0
96.00	1950.0
103.80	133.0
105.90	114.0
115.80	123.0
116.80	306.0
117.90	131.0
118.80	182.0
127.90	138.0
129.90	109.0
140.80	302.0
142.90	408.0
144.80	124.0
154.90	146.0
171.90	410.0
173.90	24056.0
174.90	1795.0
175.90	23032.0
176.90	1561.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
35.00	268.0
37.00	1550.0
38.00	1363.0
39.00	629.0
39.00	194.0
44.00	473.0
45.00	292.0
47.00	488.0
47.80	181.0
49.00	1490.0
50.00	6388.0
51.00	2143.0
52.00	125.0
54.00	146.0
56.00	520.0
57.00	819.0
59.00	295.0
61.00	1651.0
62.00	1561.0
63.00	1452.0
64.00	276.0
65.00	453.0
68.00	3398.0
69.00	3268.0
69.90	268.0
71.00	236.0
73.00	1440.0
74.00	5590.0
75.00	17000.0
76.00	1531.0
76.90	299.0
78.00	142.0
78.90	1139.0
79.90	439.0
80.90	1102.0
81.90	337.0
87.00	1424.0
88.00	1348.0
90.90	152.0
92.00	914.0
93.00	1691.0
94.00	3996.0
95.00	32696.0
96.00	2126.0
103.80	144.0
105.80	111.0
115.80	126.0
116.90	316.0
117.90	124.0
118.80	208.0
127.90	144.0
129.80	137.0
140.80	349.0
142.90	439.0
144.80	120.0
147.90	105.0
155.00	137.0
171.90	445.0
173.90	27152.0
174.90	2002.0
175.90	26032.0
176.90	1722.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
35.00	242.0
37.00	1538.0
38.00	1376.0
39.00	591.0
39.90	193.0
44.00	498.0
45.00	280.0
47.00	457.0
47.90	198.0
49.00	1416.0
50.00	6160.0
51.00	2094.0
52.00	114.0
54.90	126.0
56.00	506.0
57.00	828.0
59.90	284.0
61.00	1608.0
61.90	1566.0
63.00	1413.0
63.90	286.0
65.00	406.0
68.00	3327.0
69.00	3175.0
69.90	280.0
71.90	227.0
73.00	1432.0
74.00	5538.0
75.00	16648.0
76.00	1547.0
76.90	267.0
78.00	128.0
78.90	1143.0
79.90	444.0
80.90	1081.0
81.90	356.0
87.00	1440.0
88.00	1277.0
90.90	130.0
92.00	867.0
93.00	1542.0
94.00	3894.0
95.00	32264.0
96.00	2077.0
103.80	146.0
115.80	113.0
116.90	277.0
118.80	233.0
127.90	139.0
129.80	144.0
140.90	355.0
142.80	441.0
144.80	125.0
155.00	112.0
171.90	429.0
173.90	27776.0
174.90	2053.0
175.90	26192.0
176.90	1722.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

Scan 2790 (10.061 min): VV018055.D
BFB77

m/z	Abundance
39.90	177.0
43.90	346.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77