

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081921\
 Data File : VV021882.D
 Acq On : 19 Aug 2021 11:36
 Operator : SY/MD
 Sample : M3464-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKF4

Quant Time: Aug 20 02:16:21 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 20 02:14:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	451214	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	418973	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	214300	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	131450	37.265	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	74.540%		
7) Chloroethane-d5	1.561	69	103361	38.830	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	77.660%		
11) 1,1-Dichloroethene-d2	2.105	63	143458	25.549	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	51.100%#		
21) 2-Butanone-d5	3.873	46	200787	91.523	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	91.520%		
24) Chloroform-d	4.349	84	253237	41.437	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	82.880%		
26) 1,2-Dichloroethane-d4	5.034	65	155654	44.278	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.560%		
32) Benzene-d6	5.050	84	532955	44.235	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.480%		
36) 1,2-Dichloropropane-d6	6.072	67	163895	43.683	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	87.360%		
41) Toluene-d8	7.317	98	495552	44.500	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	89.000%		
43) trans-1,3-Dichloroprop...	7.625	79	75648	40.969	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	81.940%		
47) 2-Hexanone-d5	8.088	63	119369	97.072	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	97.070%		
56) 1,1,2,2-Tetrachloroeth...	10.220	84	220400	47.403	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	94.800%		
66) 1,2-Dichlorobenzene-d4	11.628	152	203719	45.934	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.860%		
Target Compounds					Qvalue	
13) Acetone	2.162	43	5434	3.010	ug/L #	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081921\
Data File : VV021882.D
Acq On : 19 Aug 2021 11:36
Operator : SY/MD
Sample : M3464-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKF4

Quant Time: Aug 20 02:16:21 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 20 02:14:47 2021
Response via : Initial Calibration

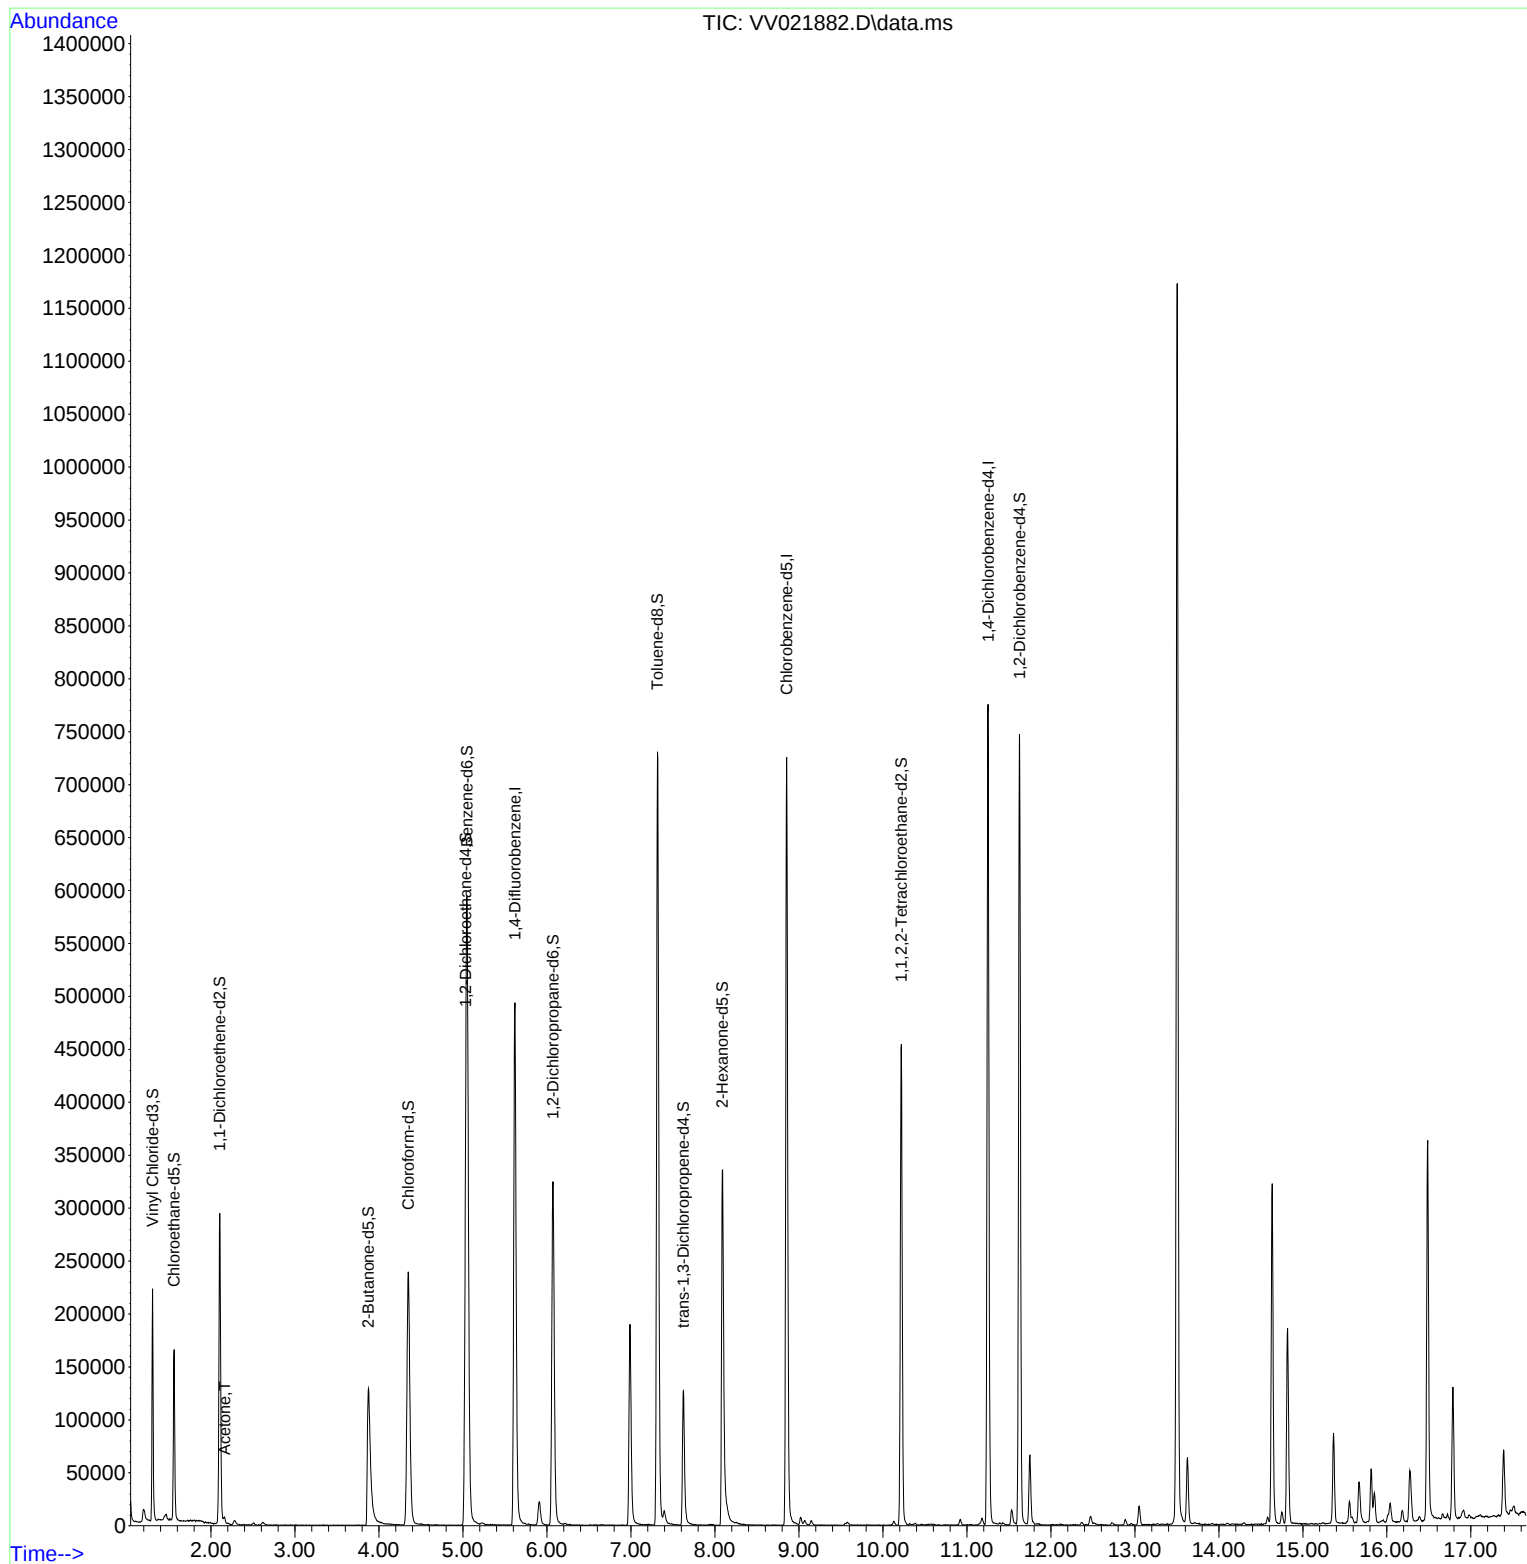

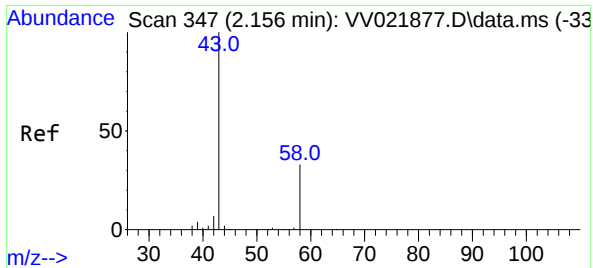

#13
 Acetone
 Concen: 3.010 ug/L
 RT: 2.162 min Scan# 349
 Delta R.T. 0.006 min
 Lab File: VV021882.D
 Acq: 19 Aug 2021 11:36

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKF4

Tgt Ion:	43	Resp:	5434
Ion	Ratio	Lower	Upper
43	100		
58	33.8	0.0	0.0#

