

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081921\
 Data File : VV021888.D
 Acq On : 19 Aug 2021 13:59
 Operator : SY/MD
 Sample : VIBLK205
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK205

Manual Integrations
 APPROVED

MMDadoda
 8/20/2021 12:53:17 PM

Quant Time: Aug 20 02:17:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 20 02:14:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	430299	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	395469	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	186720	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	120245	35.746	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	71.500%
7) Chloroethane-d5	1.558	69	101904	40.143	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	80.280%
11) 1,1-Dichloroethene-d2	2.105	63	153057	28.584	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	57.160%#
21) 2-Butanone-d5	3.876	46	204945	97.959	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.960%
24) Chloroform-d	4.349	84	239310	41.061	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.120%
26) 1,2-Dichloroethane-d4	5.034	65	153589	45.814	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.620%
32) Benzene-d6	5.050	84	504122	44.329	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.660%
36) 1,2-Dichloropropane-d6	6.072	67	163321	46.117	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	92.240%
41) Toluene-d8	7.317	98	460047	43.767	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.540%
43) trans-1,3-Dichloroprop...	7.622	79	71284	40.900	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.800%
47) 2-Hexanone-d5	8.088	63	118702	102.267	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	102.270%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	216940	49.432	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.860%
66) 1,2-Dichlorobenzene-d4	11.625	152	178098	46.089	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.180%
Target Compounds					Qvalue	
13) Acetone	2.159	43	3902m	2.267	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081921\
Data File : VV021888.D
Acq On : 19 Aug 2021 13:59
Operator : SY/MD
Sample : VIBLK205
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
VIBLK205

Manual Integrations
APPROVED

MMDadoda
8/20/2021 12:53:17 PM


Quant Time: Aug 20 02:17:30 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 20 02:14:47 2021
Response via : Initial Calibration

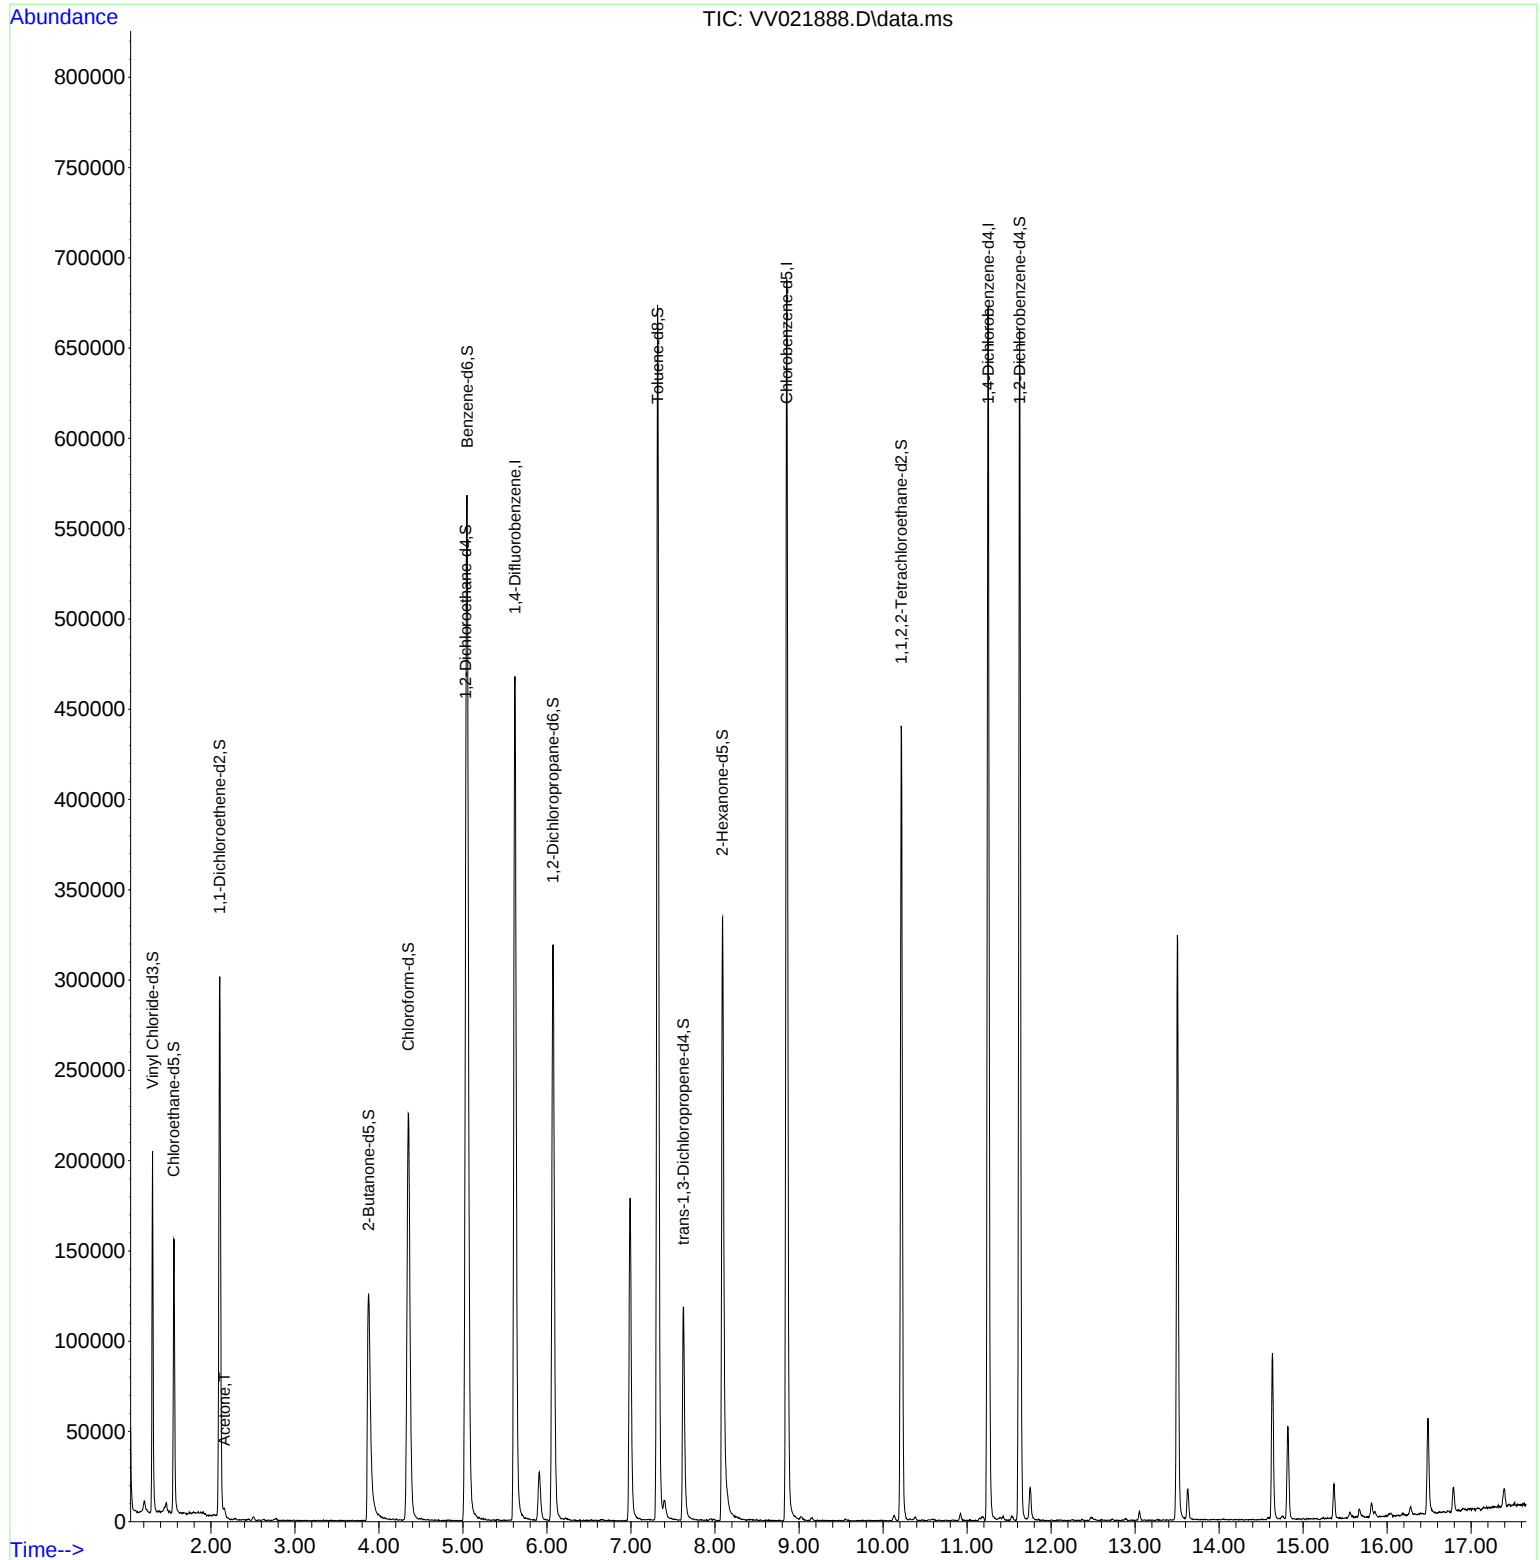

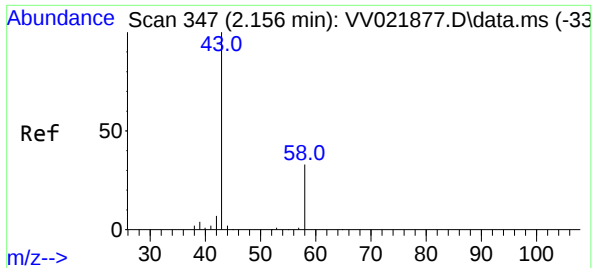

#13
Acetone
Concen: 2.267 ug/L m
RT: 2.159 min Scan# 348
Delta R.T. 0.003 min
Lab File: VV021888.D
Acq: 19 Aug 2021 13:59

Instrument :
MSVOA_V
ClientSampleId :
VIBLK205

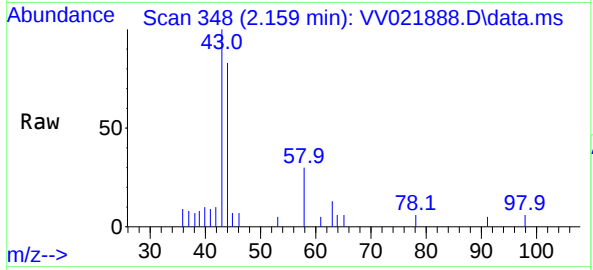

Tgt Ion:	43	Resp:	3902
Ion Ratio	Lower	Upper	
43	100		
58	34.3	0.0	0.0#

Manual Integrations
APPROVED
MMDadoda
8/20/2021 12:53:17 PM

